


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG091120\
 Data File : BG046593.D
 Acq On : 11 Sep 2020 12:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 02 15:06:53 2020

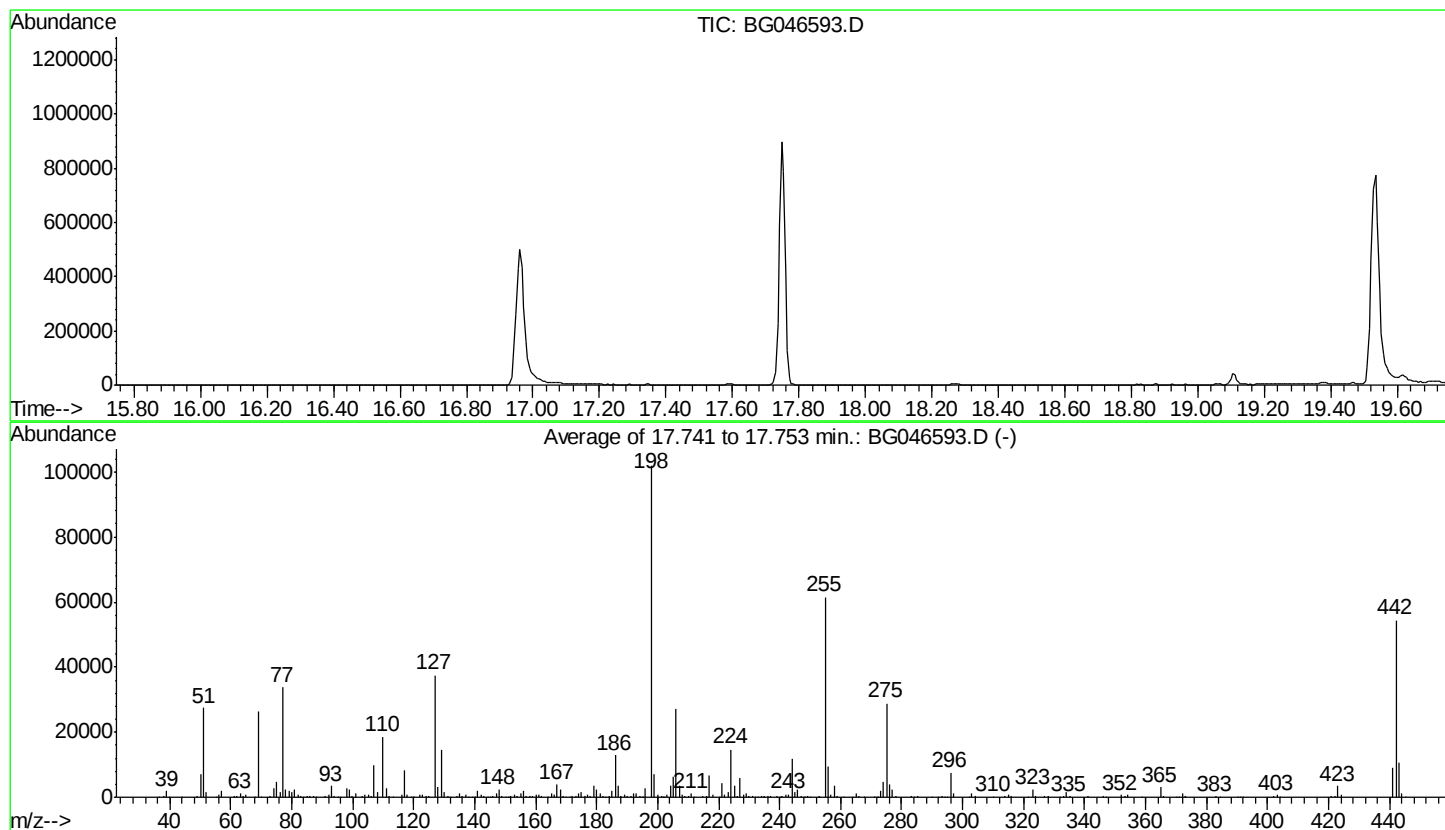

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	27474	PASS
68	69	0.00	2	0.6	155	PASS
69	198	0.00	100	25.8	26312	PASS
70	69	0.00	2	0.7	195	PASS
127	198	10	80	36.9	37570	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101906	PASS
199	198	5	9	6.9	7073	PASS
275	198	10	60	28.2	28720	PASS
365	198	1	100	3.0	3103	PASS
441	198	0.01	100	8.9	9029	PASS
442	198	50	100	53.4	54418	PASS
443	442	15	24	19.5	10590	PASS