
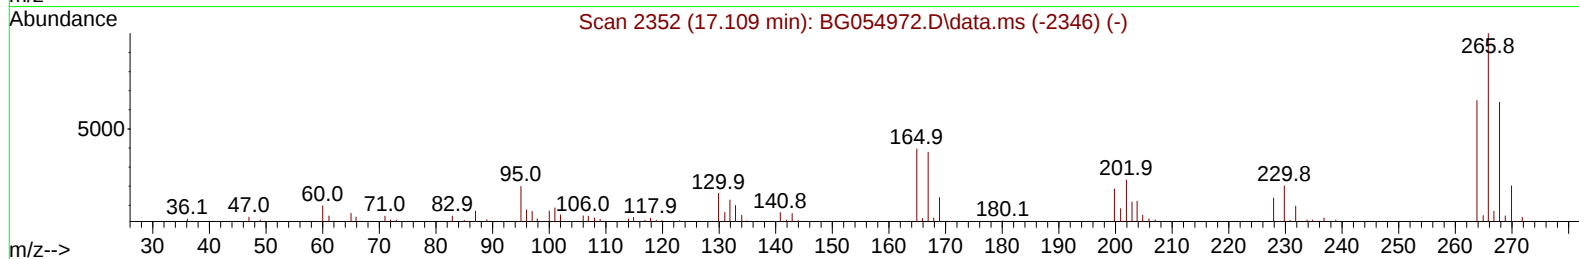
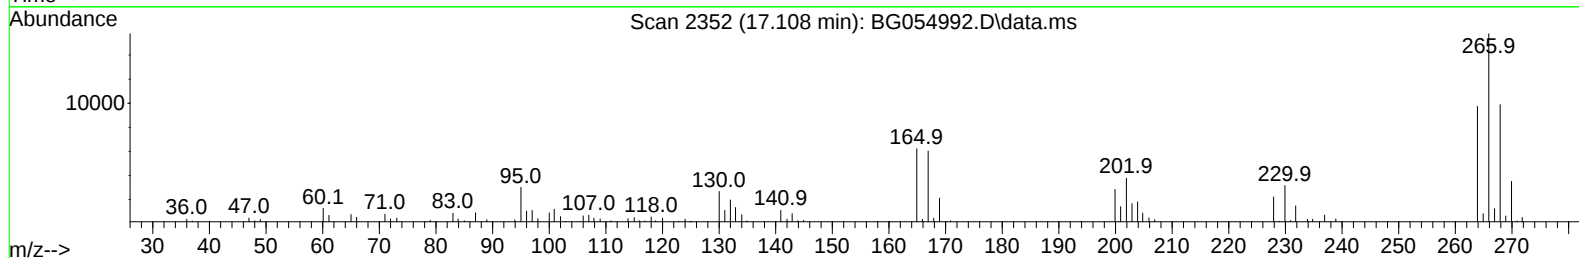


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG092122\  
Data File : BG054992.D  
Acq On : 21 Sep 2022 11:27  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 06:34:22 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 19 17:41:40 2022  
Response via : Initial Calibration

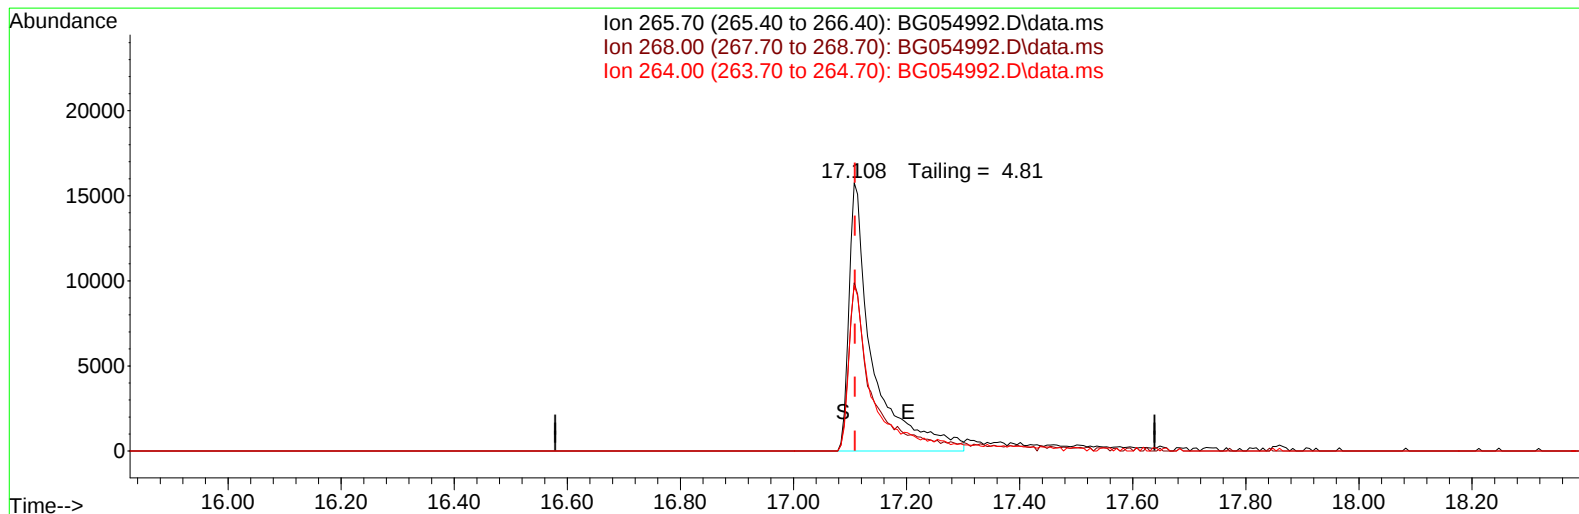

TIC: BG054992.D\data.ms

**(70) Pentachlorophenol (C)**




17.108min (-0.002) 2580.45 ng

response 45169

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.00  | 62.70  |
| 264.00 | 61.70  | 61.72  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG092122\  
Data File : BG054992.D  
Acq On : 21 Sep 2022 11:27  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 06:34:22 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG091922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Sep 19 17:41:40 2022  
Response via : Initial Calibration

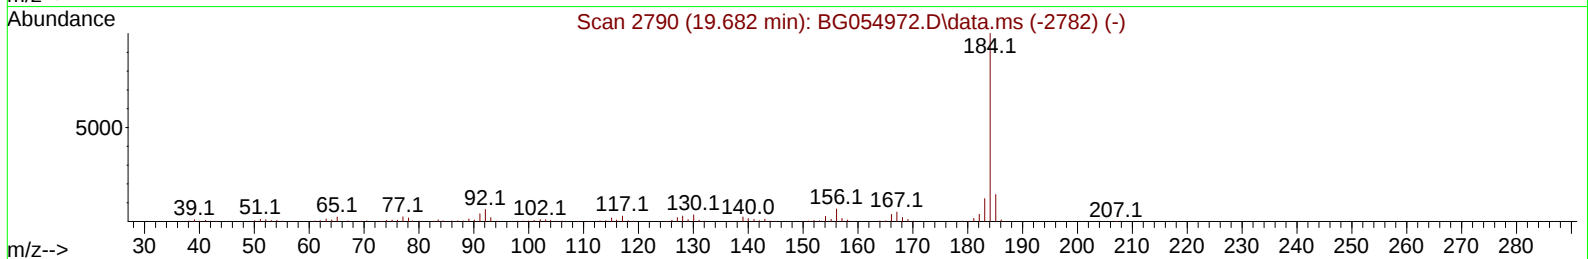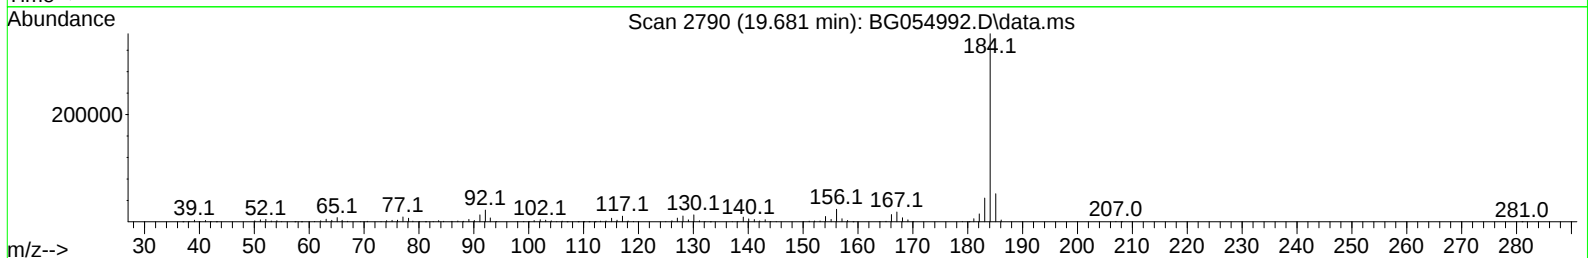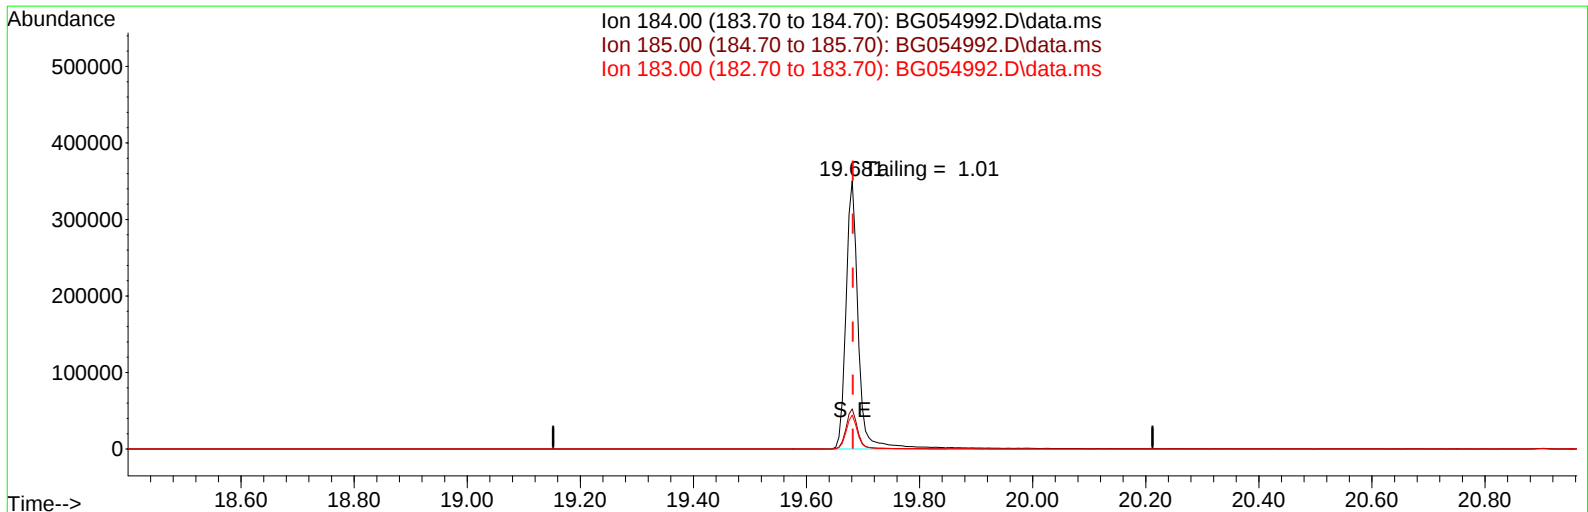

TIC: BG054992.D\data.ms

**(77) Benzidine**

19.681min (-0.001) 0.00 ng

response 529303

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.96  |
| 183.00 | 12.30  | 12.64  |
| 0.00   | 0.00   | 0.00   |