

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
 Data File : BG054995.D
 Acq On : 21 Sep 2022 15:52
 Operator : CG/JU
 Sample : N4723-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-13-COMP

Quant Time: Sep 22 04:40:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 17:41:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.053	152	40982	20.000	ng	0.00
21) Naphthalene-d8	10.879	136	159542	20.000	ng	# 0.00
39) Acenaphthene-d10	14.698	164	108732	20.000	ng	0.00
64) Phenanthrene-d10	17.448	188	264708	20.000	ng	0.00
76) Chrysene-d12	21.725	240	282088	20.000	ng	0.00
86) Perylene-d12	25.033	264	296094	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.591	112	258065	123.213	ng	0.00
7) Phenol-d6	7.213	99	325536	115.958	ng	0.00
23) Nitrobenzene-d5	9.228	82	186962	67.924	ng	-0.01
42) 2,4,6-Tribromophenol	16.191	330	148570	116.636	ng	0.00
45) 2-Fluorobiphenyl	13.324	172	502385	72.816	ng	0.00
79) Terphenyl-d14	20.051	244	972235	72.096	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
Data File : BG054995.D
Acq On : 21 Sep 2022 15:52
Operator : CG/JU
Sample : N4723-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-13-COMP

Quant Time: Sep 22 04:40:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration




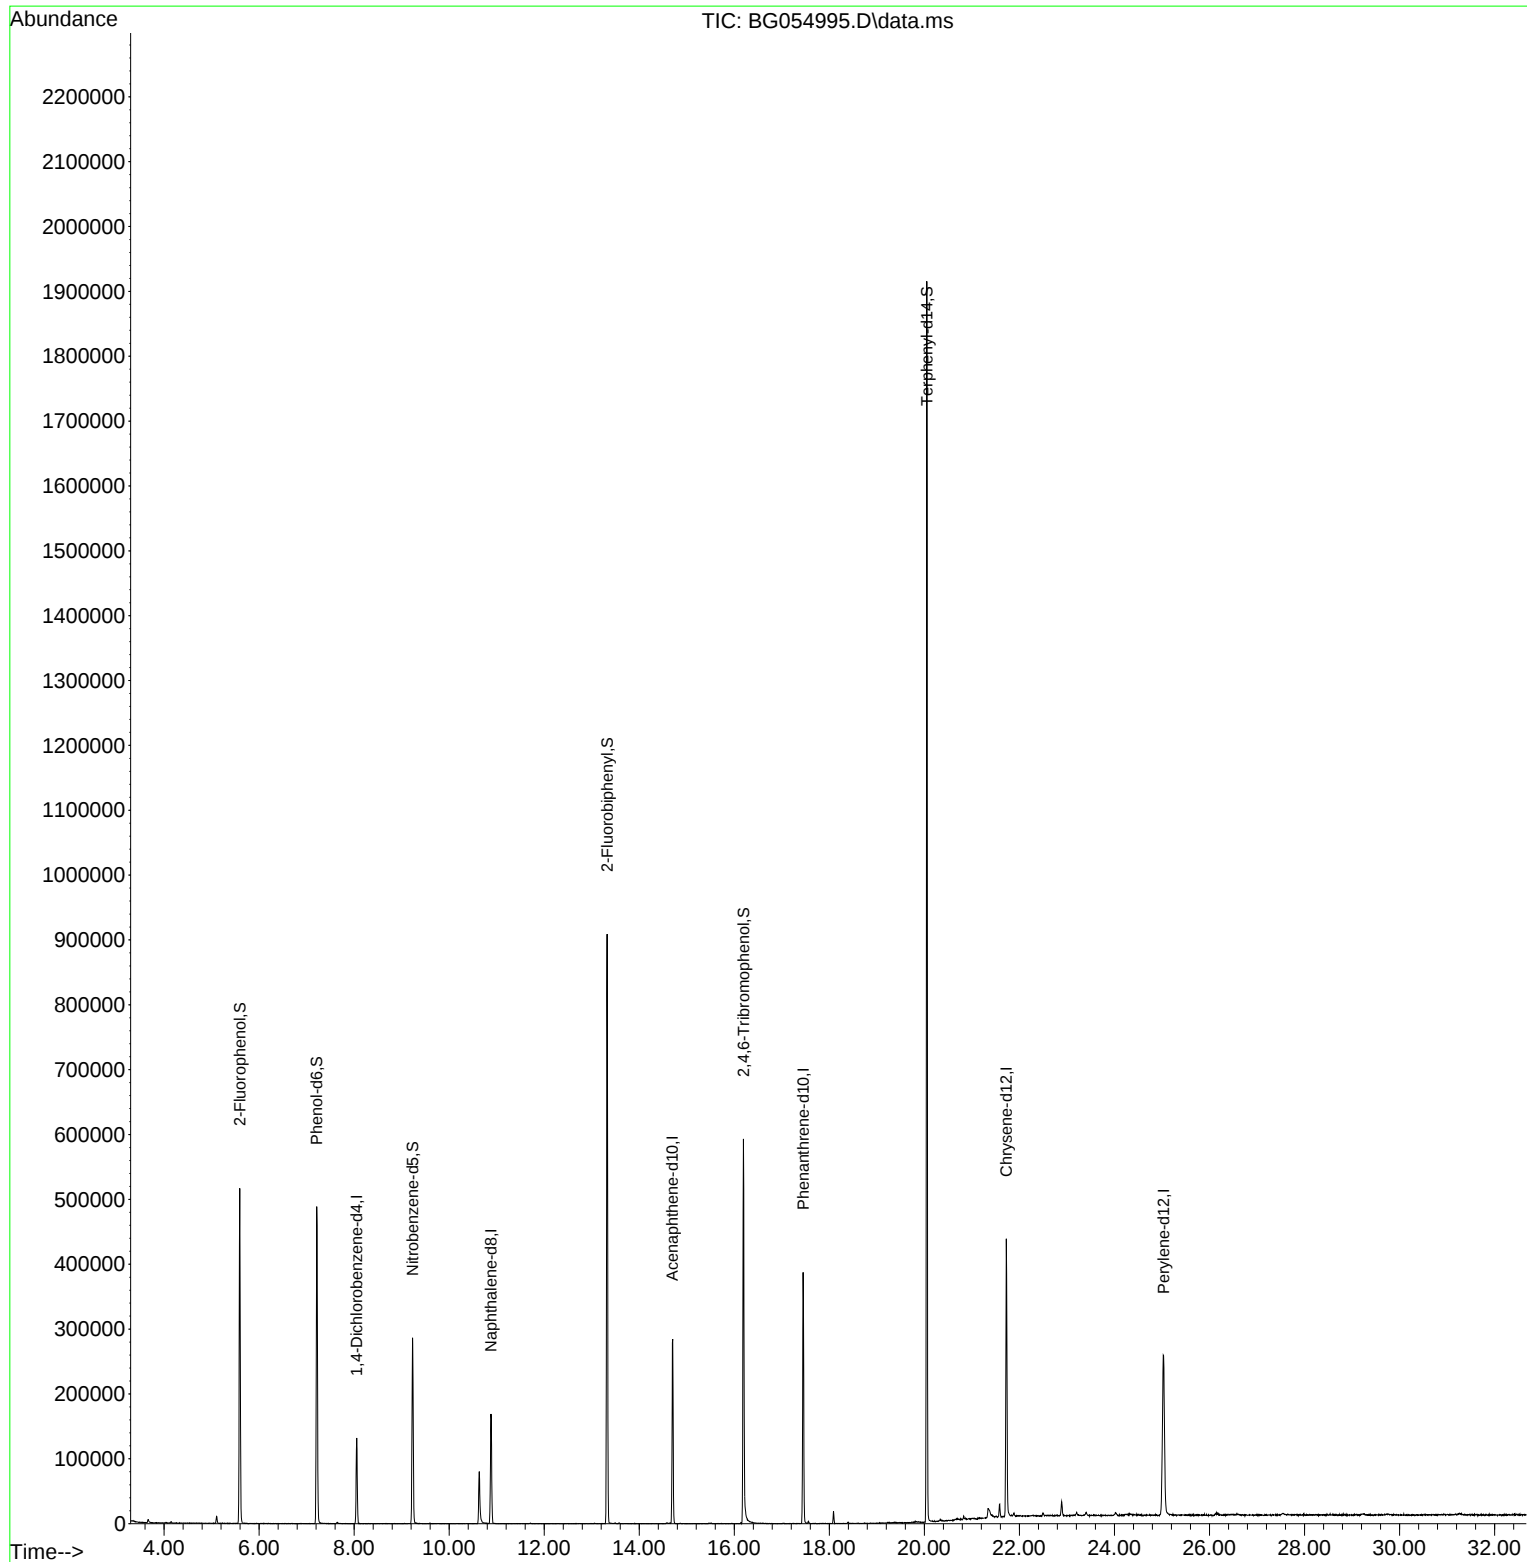


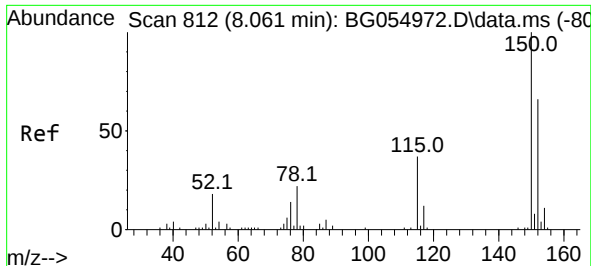

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.053 min Scan# 81
Delta R.T. -0.008 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52




Instrument :
BNA_G
ClientSampleId :
SB-13-COMP


Tgt Ion:152 Resp: 40982
Ion Ratio Lower Upper
152 100
150 155.6 125.2 187.8
115 55.3 47.9 71.9

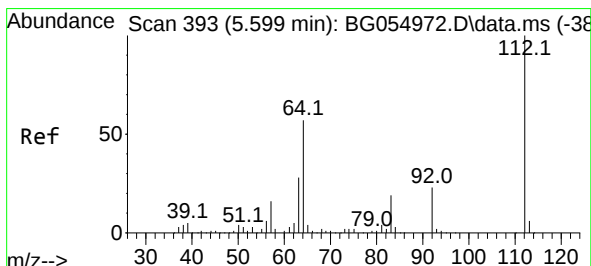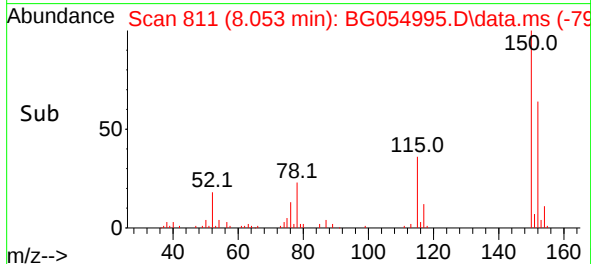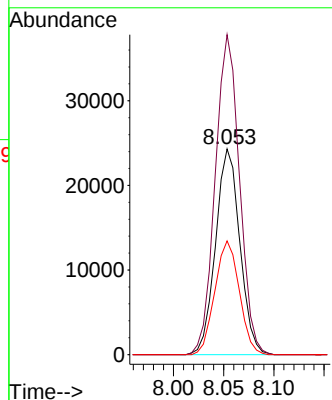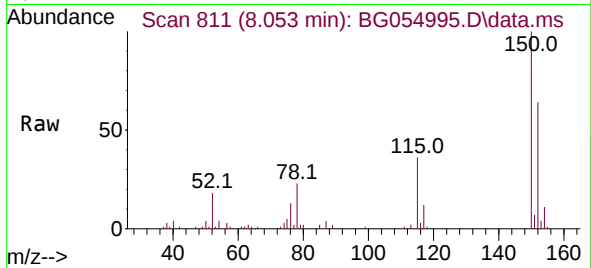

#5
2-Fluorophenol
Concen: 123.213 ng
RT: 5.591 min Scan# 392
Delta R.T. -0.007 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52

Tgt Ion:112 Resp: 258065
Ion Ratio Lower Upper
112 100
64 53.3 49.3 73.9
63 28.4 26.3 39.5


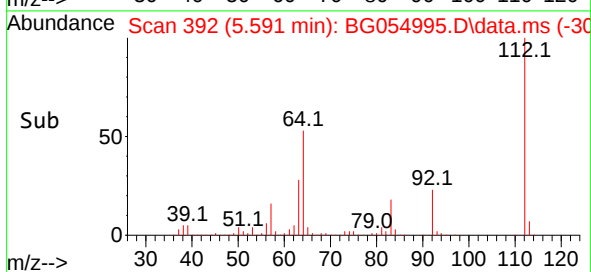
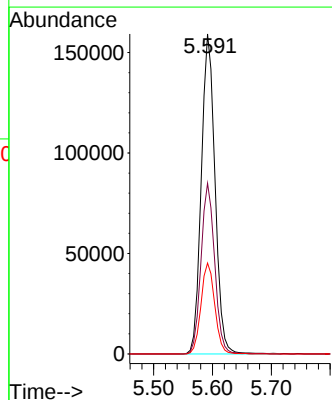
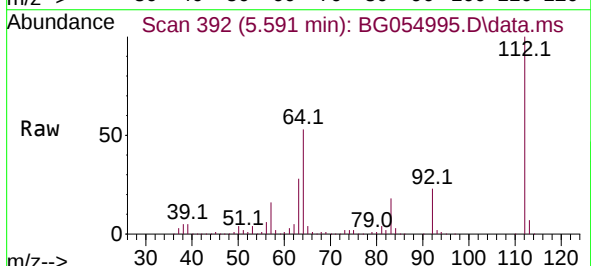


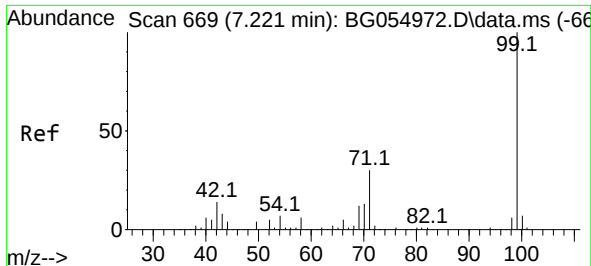

#7
Phenol-d6
Concen: 115.958 ng
RT: 7.213 min Scan# 668
Delta R.T. -0.007 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52




Instrument :
BNA_G
ClientSampleId :
SB-13-COMP


Tgt Ion: 99 Resp: 325536
Ion Ratio Lower Upper
99 100
42 14.7 14.6 22.0
71 30.2 24.6 37.0

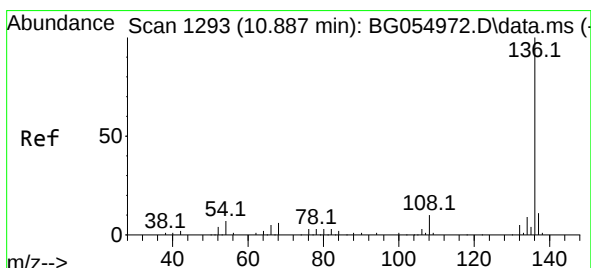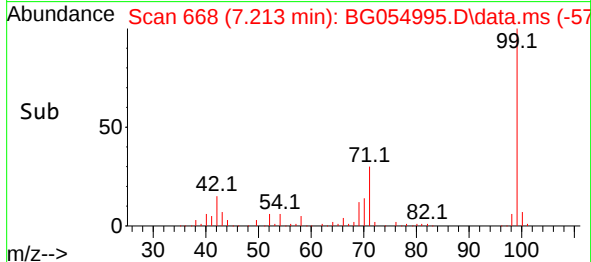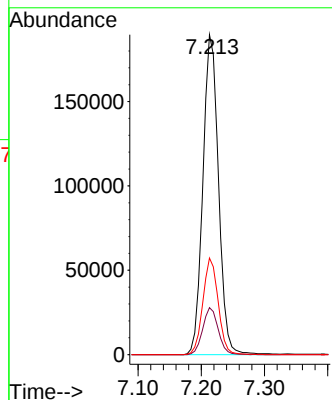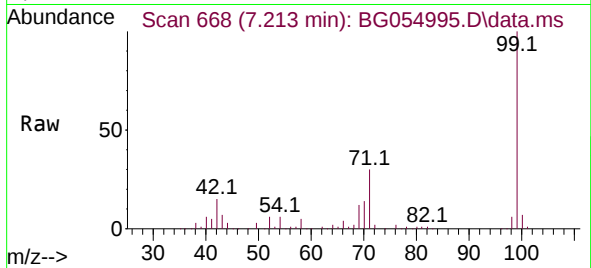

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.879 min Scan# 1292
Delta R.T. -0.007 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52

Tgt Ion: 136 Resp: 159542
Ion Ratio Lower Upper
136 100
137 11.3 9.2 13.8
54 6.5 7.7 11.5#
68 5.2 5.6 8.4#

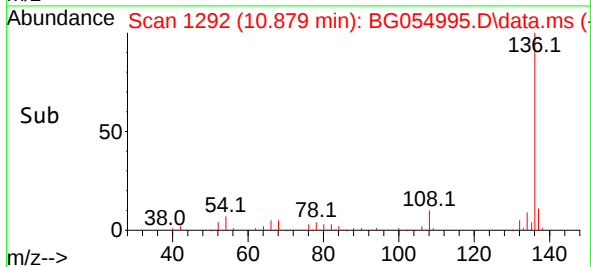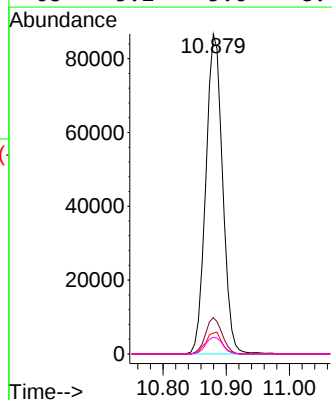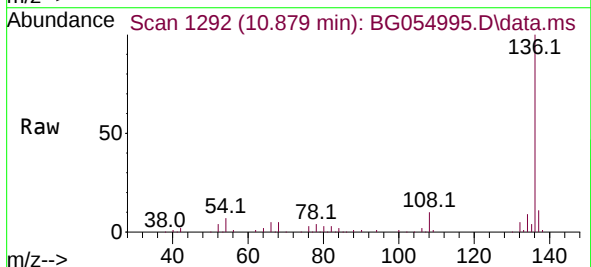

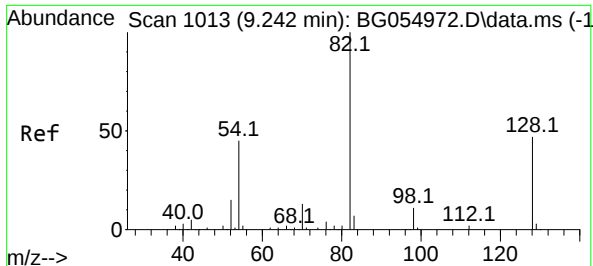

#23

Nitrobenzene-d5

Concen: 67.924 ng

RT: 9.228 min Scan# 1011

Delta R.T. -0.013 min

Lab File: BG054995.D

Acq: 21 Sep 2022 15:52

Instrument :

BNA_G

ClientSampleId :

SB-13-COMP





Tgt Ion: 82 Resp: 186962

Ion Ratio Lower Upper

82 100

128 47.7 32.2 48.2

54 45.8 41.4 62.0

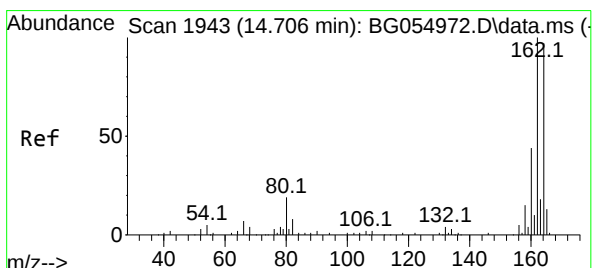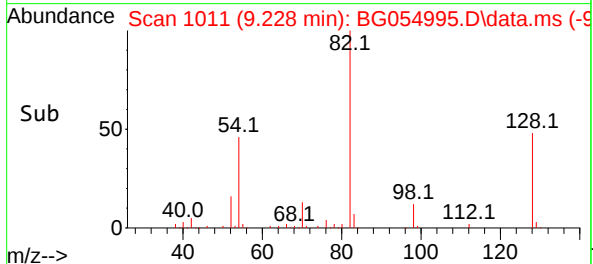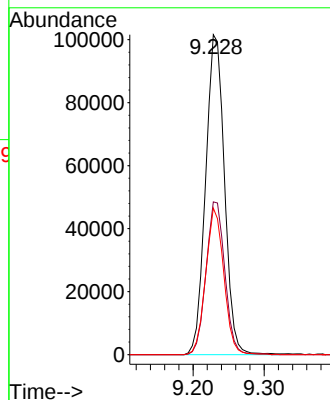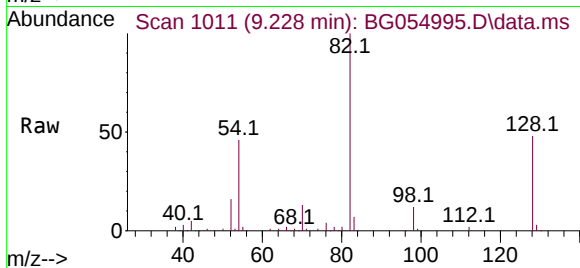

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.698 min Scan# 1942

Delta R.T. -0.008 min

Lab File: BG054995.D

Acq: 21 Sep 2022 15:52




Tgt Ion:164 Resp: 108732


Ion Ratio Lower Upper

164 100

162 98.8 83.0 124.4

160 44.0 38.0 57.0


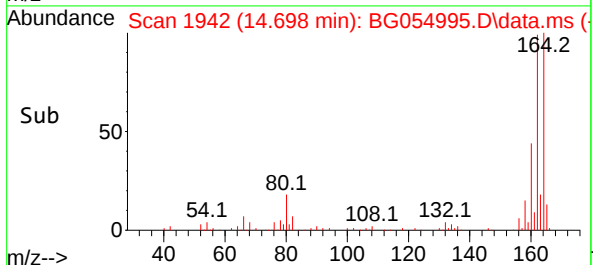
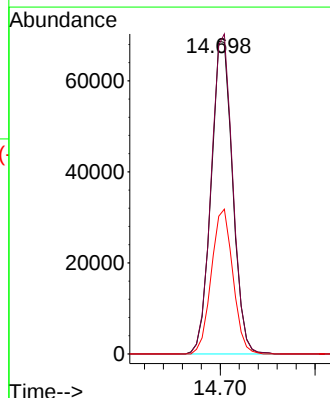
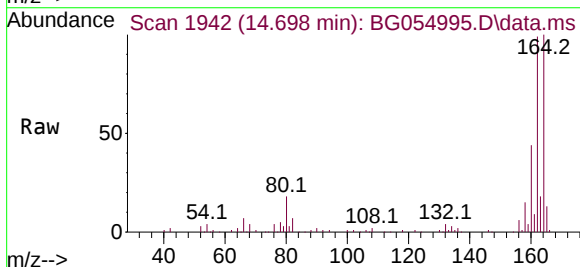


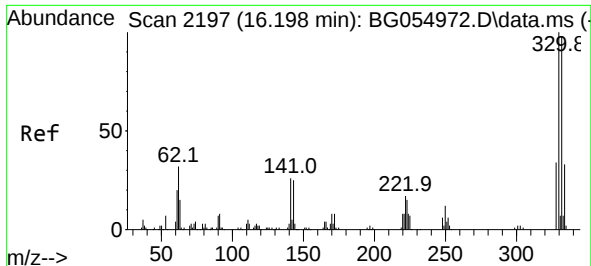

#42
2,4,6-Tribromophenol
Concen: 116.636 ng
RT: 16.191 min Scan# 2197
Delta R.T. -0.007 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52




Instrument :
BNA_G
ClientSampleId :
SB-13-COMP


Tgt Ion:330 Resp: 148570
Ion Ratio Lower Upper
330 100
332 96.6 79.8 119.6
141 27.8 26.8 40.2

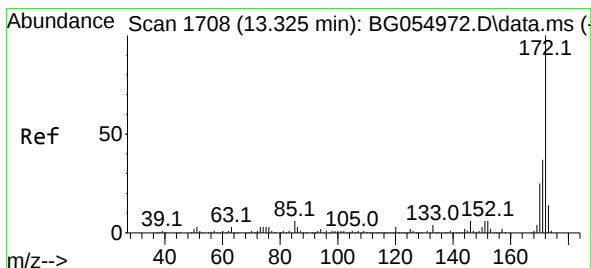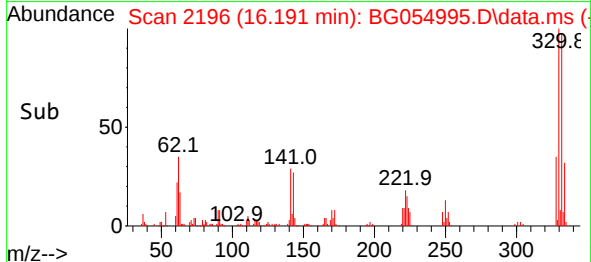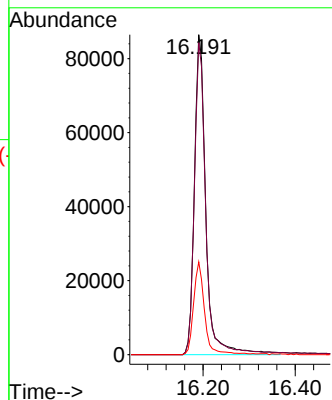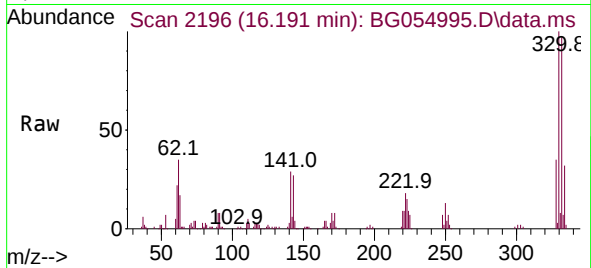

#45
2-Fluorobiphenyl
Concen: 72.816 ng
RT: 13.324 min Scan# 1708
Delta R.T. -0.002 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52

Tgt Ion:172 Resp: 502385
Ion Ratio Lower Upper
172 100
171 36.9 31.2 46.8
170 25.1 20.6 30.8


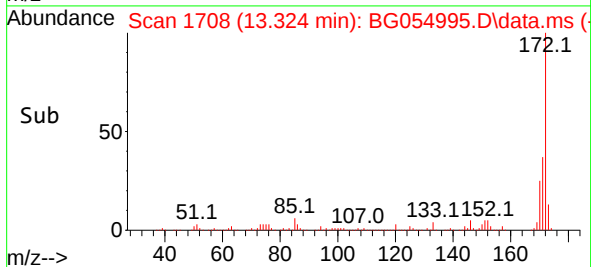
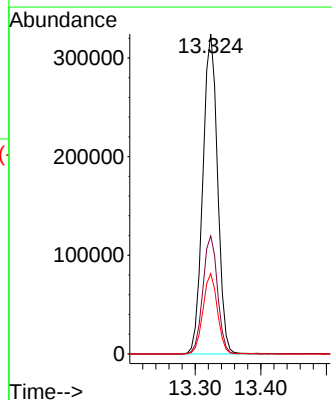
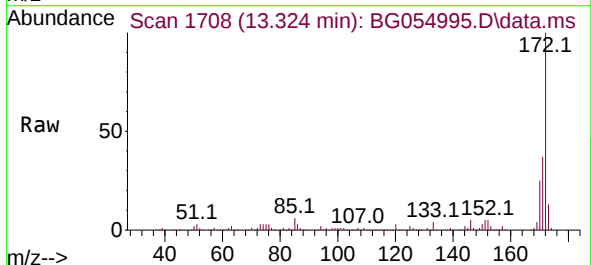


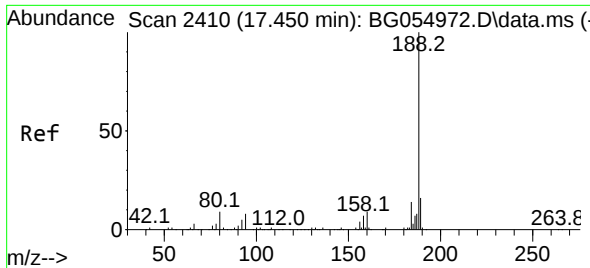

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.448 min Scan# 2410
Delta R.T. -0.002 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52




Instrument :
BNA_G
ClientSampleId :
SB-13-COMP


Tgt Ion:188 Resp: 264708
Ion Ratio Lower Upper
188 100
94 7.7 7.0 10.4
80 8.7 7.9 11.9

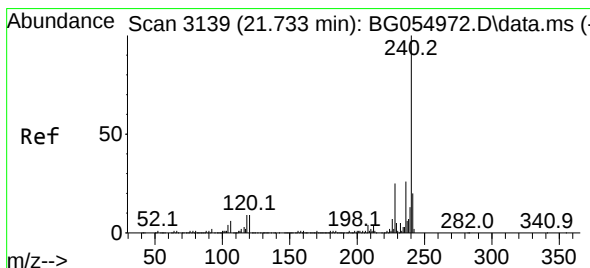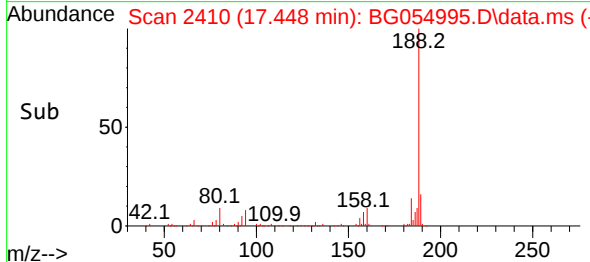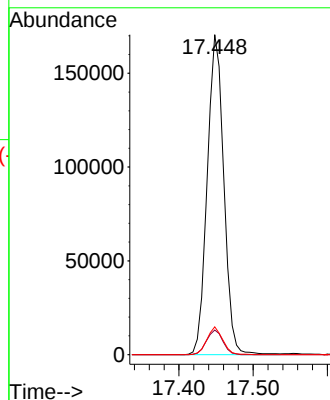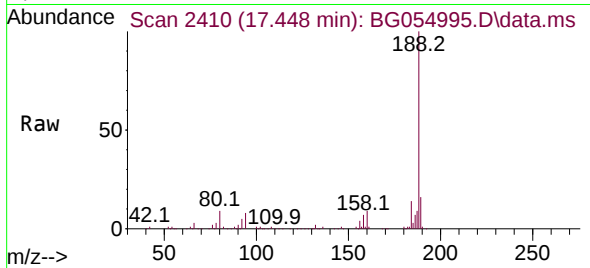

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.725 min Scan# 3138
Delta R.T. -0.007 min
Lab File: BG054995.D
Acq: 21 Sep 2022 15:52

Tgt Ion:240 Resp: 282088
Ion Ratio Lower Upper
240 100
120 8.5 8.2 12.4
236 25.1 21.2 31.8

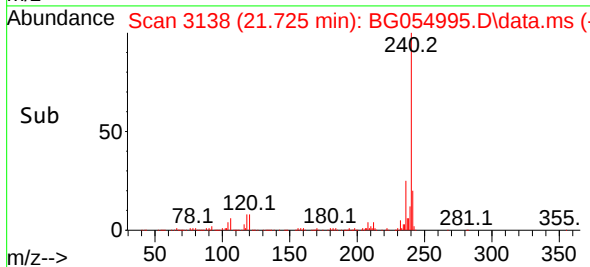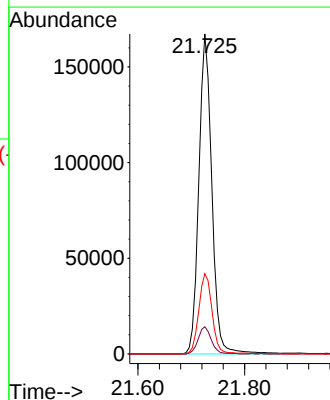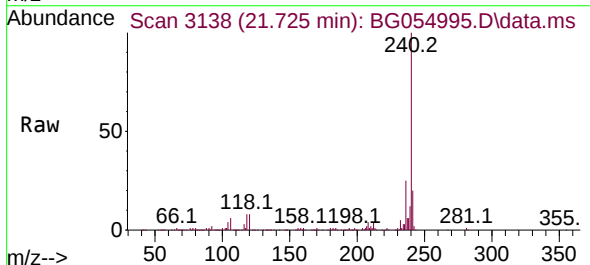

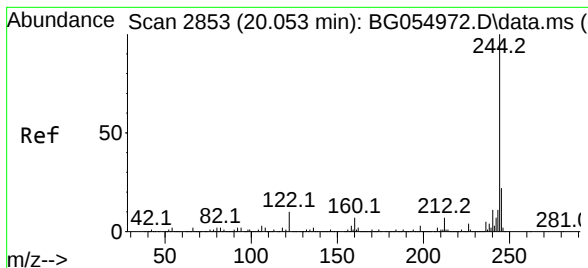

#79

Terphenyl-d14

Concen: 72.096 ng

RT: 20.051 min Scan# 2853

Delta R.T. -0.002 min

Lab File: BG054995.D

Acq: 21 Sep 2022 15:52

Instrument :

BNA_G

ClientSampleId :

SB-13-COMP





Tgt Ion:244 Resp: 972235

Ion Ratio Lower Upper

244 100

212 7.2 6.2 9.2

122 8.9 9.0 13.6#

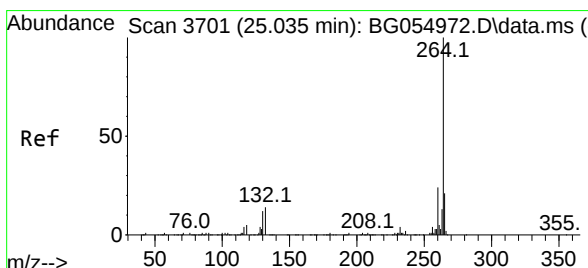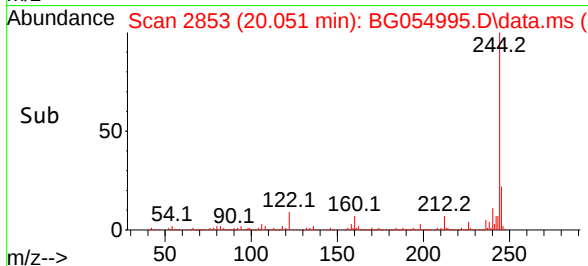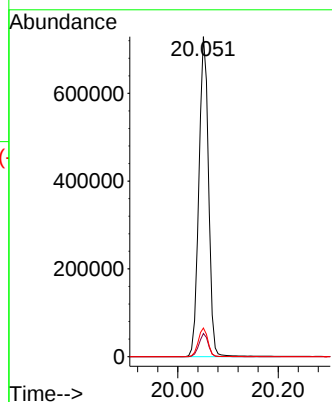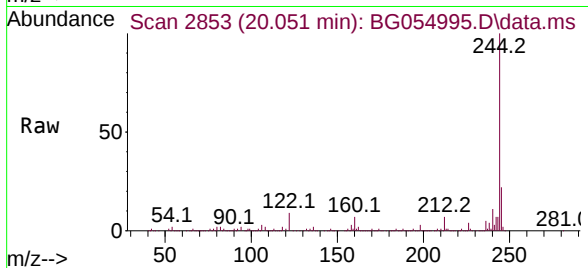

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.033 min Scan# 3701

Delta R.T. -0.002 min

Lab File: BG054995.D

Acq: 21 Sep 2022 15:52

Tgt Ion:264 Resp: 296094

Ion Ratio Lower Upper

264 100

260 23.7 19.9 29.9

265 21.6 16.9 25.3

