

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
 Data File : BG055003.D
 Acq On : 21 Sep 2022 21:28
 Operator : CG/JU
 Sample : N4723-18
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-28-COMP

Quant Time: Sep 22 04:45:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 17:41:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.058	152	38798	20.000	ng	0.00
21) Naphthalene-d8	10.885	136	154548	20.000	ng	# 0.00
39) Acenaphthene-d10	14.704	164	106888	20.000	ng	0.00
64) Phenanthrene-d10	17.447	188	258130	20.000	ng	# 0.00
76) Chrysene-d12	21.725	240	264465	20.000	ng	0.00
86) Perylene-d12	25.021	264	277088	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.597	112	261570	131.916	ng	0.00
7) Phenol-d6	7.218	99	334683	125.927	ng	0.00
23) Nitrobenzene-d5	9.234	82	193998	72.757	ng	0.00
42) 2,4,6-Tribromophenol	16.190	330	154025	123.005	ng	0.00
45) 2-Fluorobiphenyl	13.323	172	525718	77.513	ng	0.00
79) Terphenyl-d14	20.050	244	1016687	80.416	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
Data File : BG055003.D
Acq On : 21 Sep 2022 21:28
Operator : CG/JU
Sample : N4723-18
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-28-COMP


Quant Time: Sep 22 04:45:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

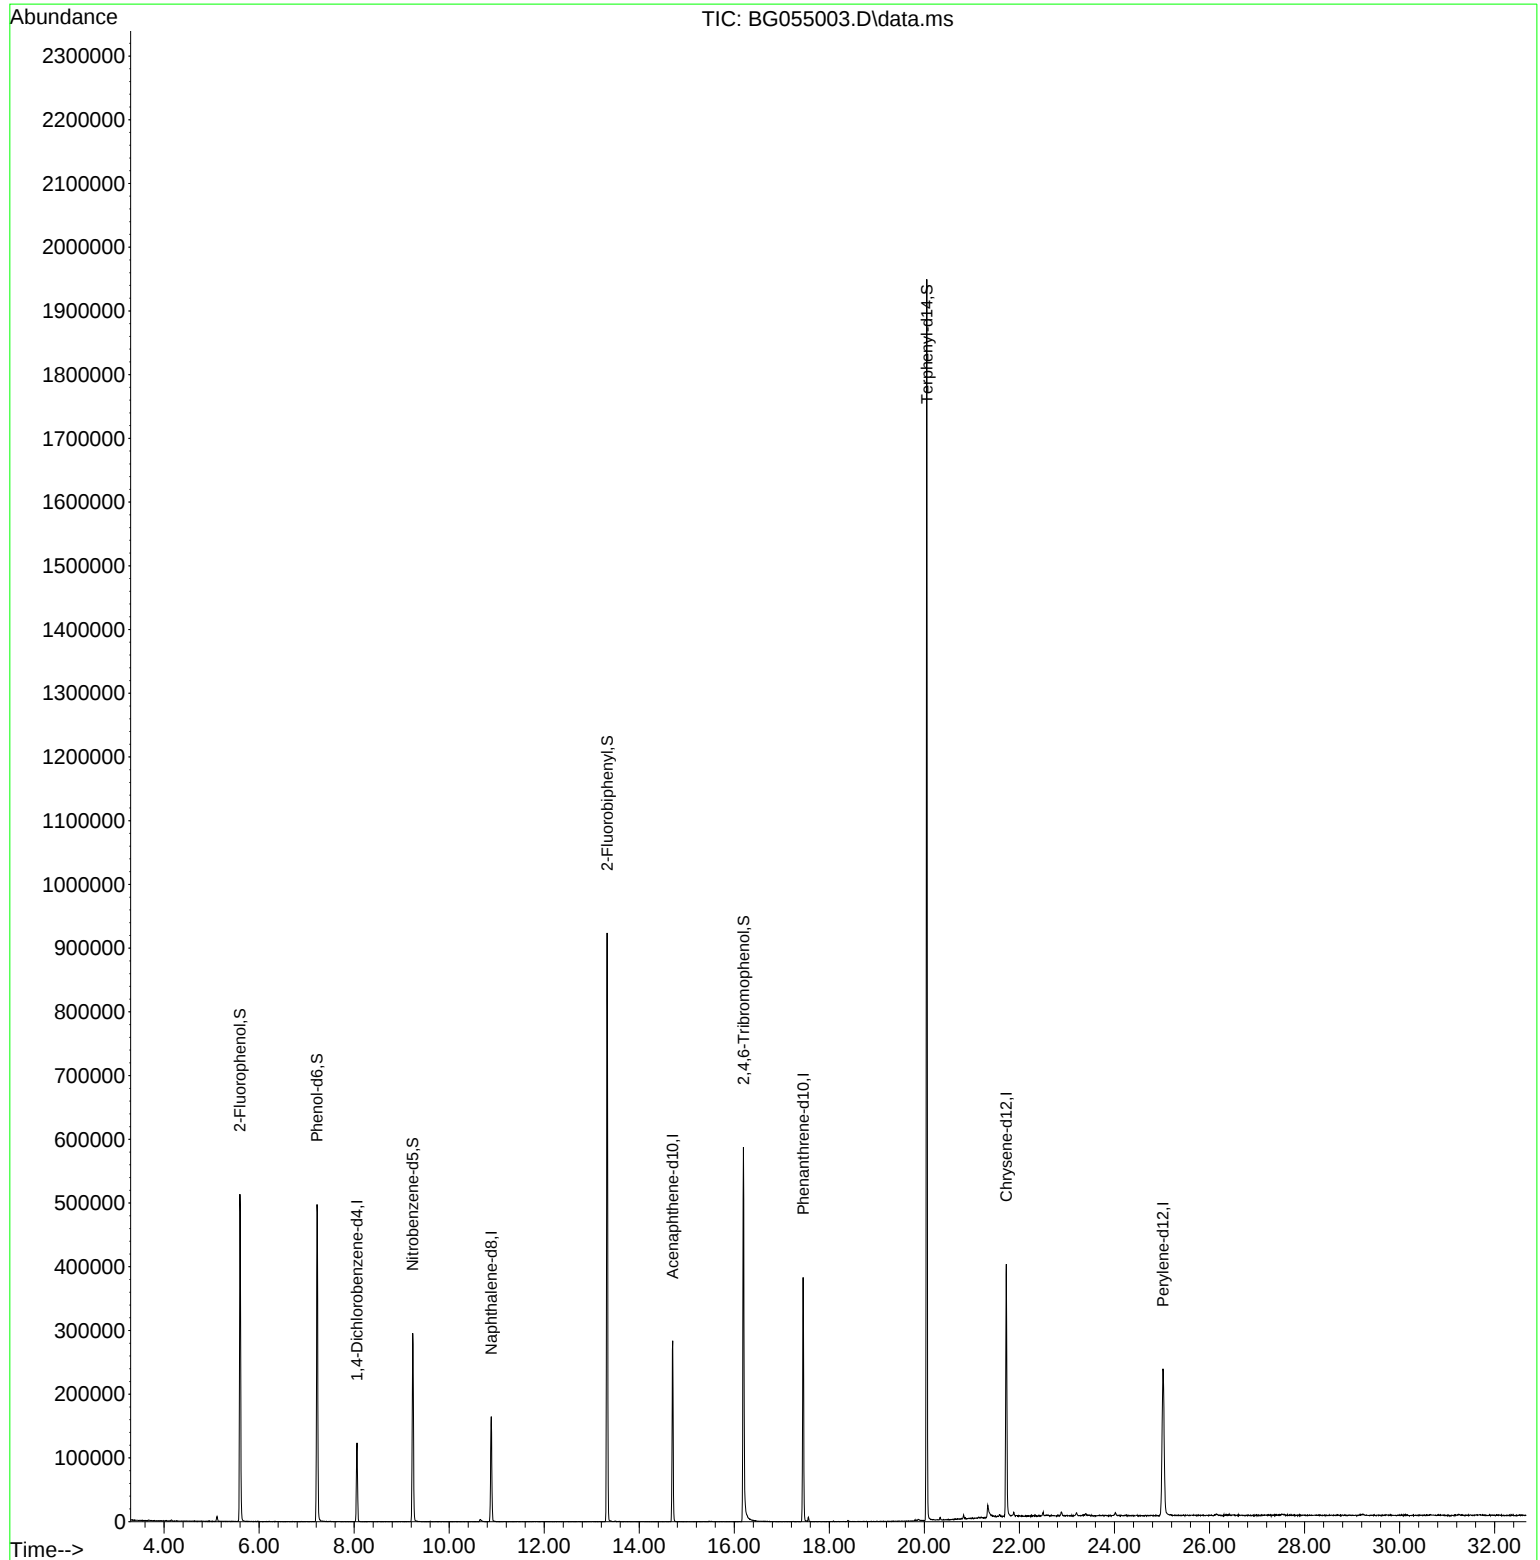



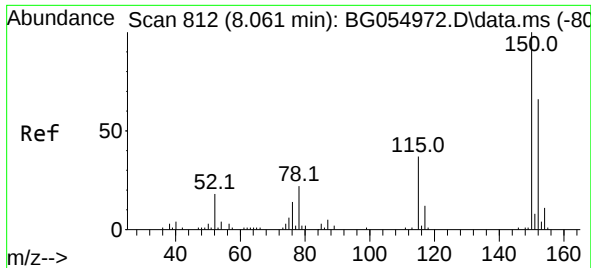


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.058 min Scan# 812
Delta R.T. -0.003 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28

Instrument :
BNA_G
ClientSampleId :
SB-28-COMP



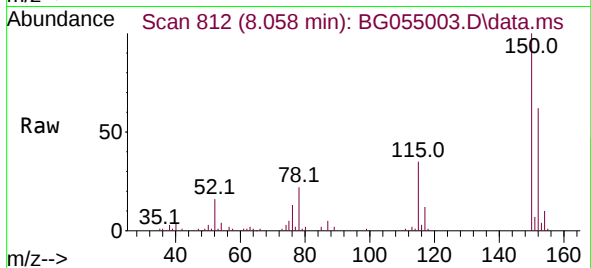



Tgt Ion:152 Resp: 38798
Ion Ratio Lower Upper
152 100
150 160.5 125.2 187.8
115 55.6 47.9 71.9

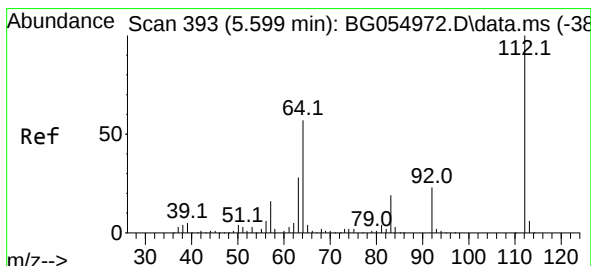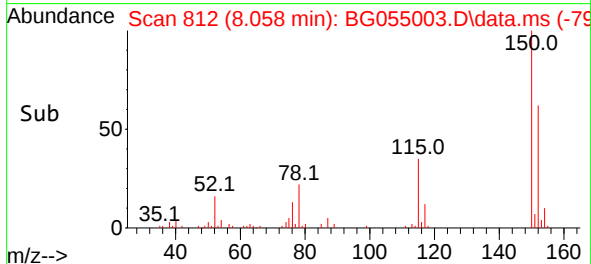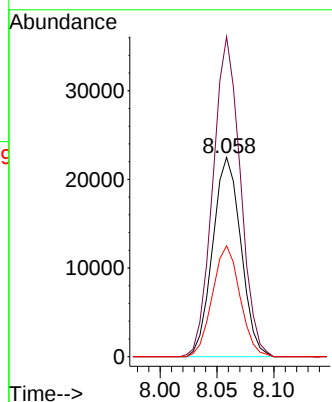

#5
2-Fluorophenol
Concen: 131.916 ng
RT: 5.597 min Scan# 393
Delta R.T. -0.002 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28

Tgt Ion:112 Resp: 261570
Ion Ratio Lower Upper
112 100
64 53.2 49.3 73.9
63 29.1 26.3 39.5


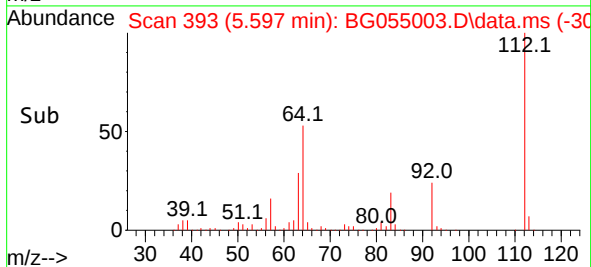
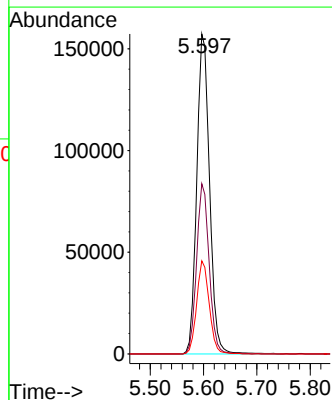
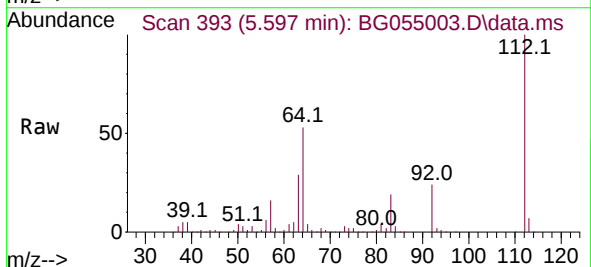


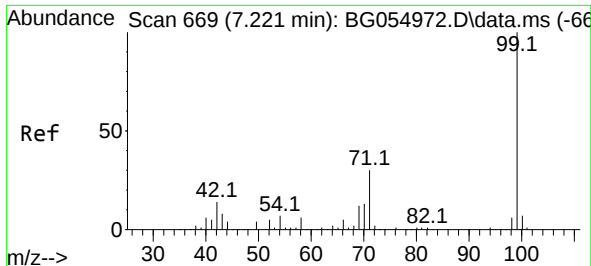

#7
Phenol-d6
Concen: 125.927 ng
RT: 7.218 min Scan# 669
Delta R.T. -0.002 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28




Instrument :
BNA_G
ClientSampleId :
SB-28-COMP


Tgt Ion: 99 Resp: 334683
Ion Ratio Lower Upper
99 100
42 15.0 14.6 22.0
71 29.6 24.6 37.0

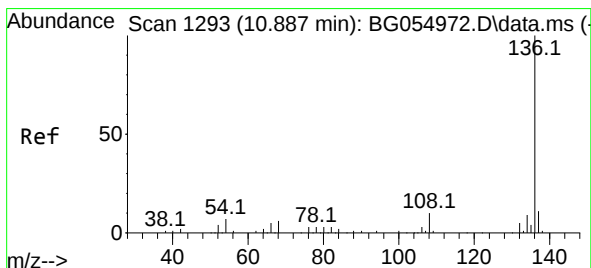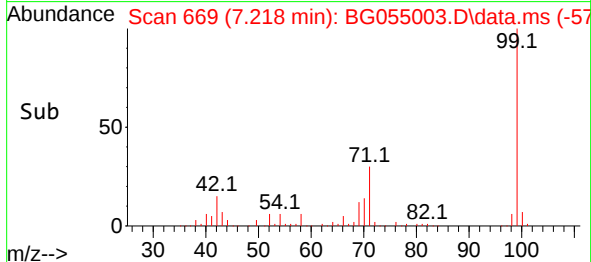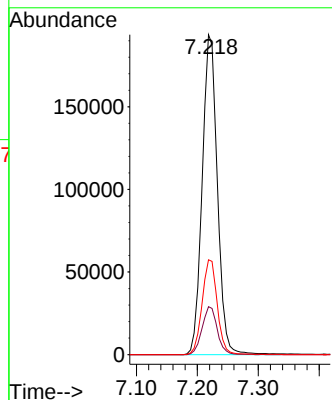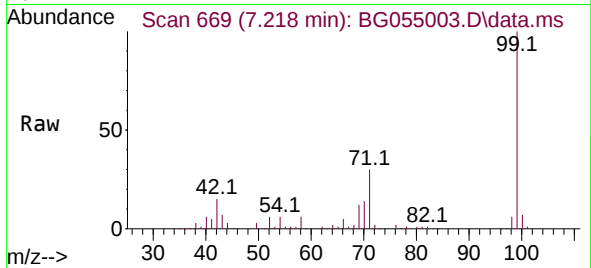

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.885 min Scan# 1293
Delta R.T. -0.002 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28

Tgt Ion: 136 Resp: 154548
Ion Ratio Lower Upper
136 100
137 10.4 9.2 13.8
54 6.3 7.7 11.5#
68 5.4 5.6 8.4#

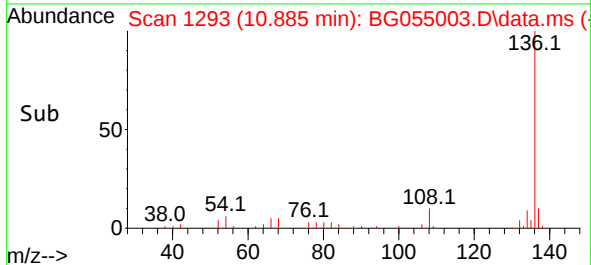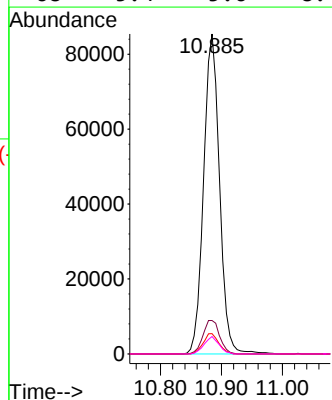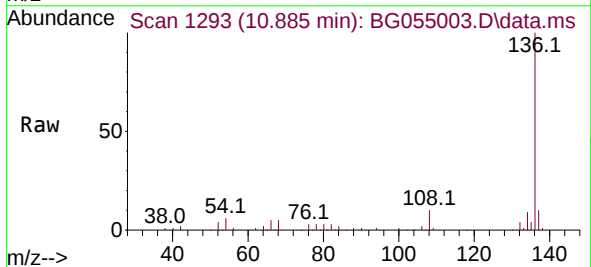

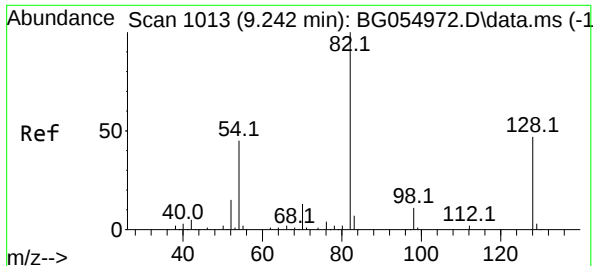

#23

Nitrobenzene-d5

Concen: 72.757 ng

RT: 9.234 min Scan# 1013

Delta R.T. -0.008 min

Lab File: BG055003.D

Acq: 21 Sep 2022 21:28

Instrument :

BNA_G

ClientSampleId :

SB-28-COMP





Tgt Ion: 82 Resp: 193998

Ion Ratio Lower Upper

82 100

128 47.4 32.2 48.2

54 43.6 41.4 62.0

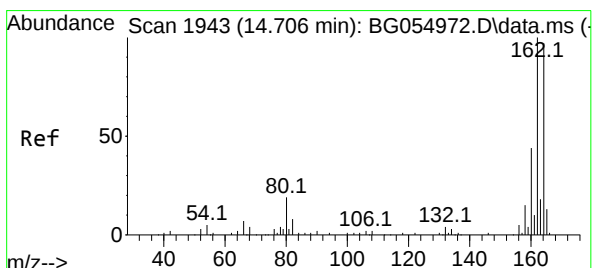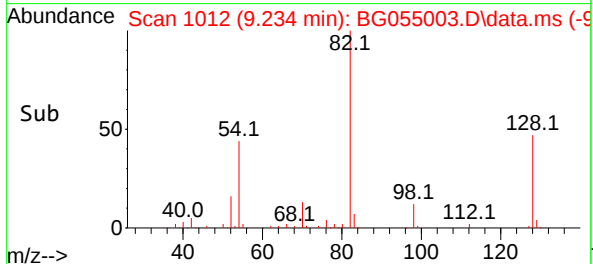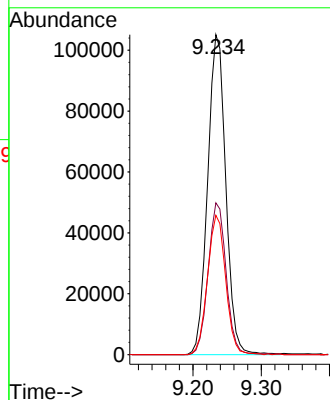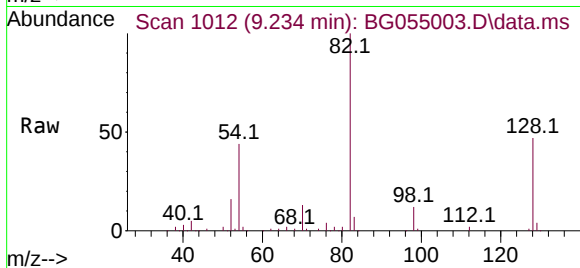

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.704 min Scan# 1943

Delta R.T. -0.002 min

Lab File: BG055003.D

Acq: 21 Sep 2022 21:28




Tgt Ion:164 Resp: 106888


Ion Ratio Lower Upper

164 100

162 102.3 83.0 124.4

160 46.5 38.0 57.0

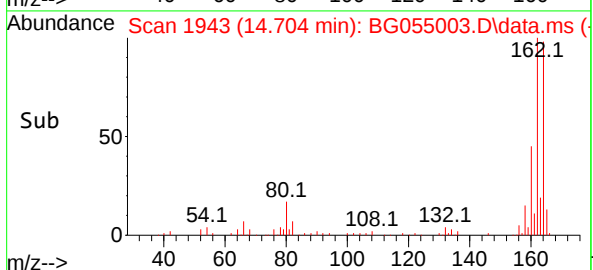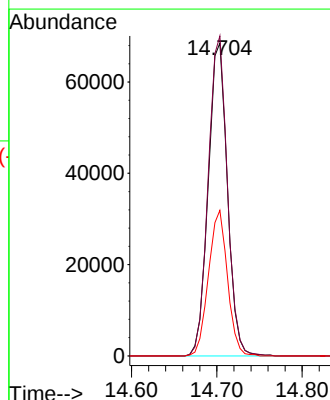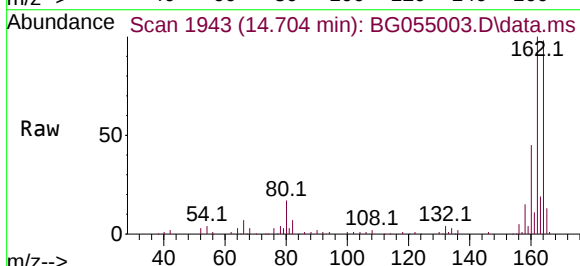

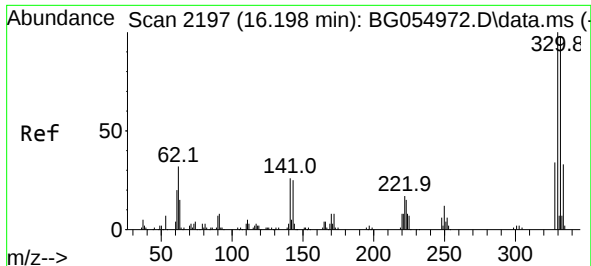

#42

2,4,6-Tribromophenol

Concen: 123.005 ng

RT: 16.190 min Scan# 21

Delta R.T. -0.008 min

Lab File: BG055003.D

Acq: 21 Sep 2022 21:28

Instrument :

BNA_G

ClientSampleId :

SB-28-COMP





Tgt Ion:330 Resp: 154025

Ion Ratio Lower Upper

330 100

332 96.5 79.8 119.6

141 28.2 26.8 40.2

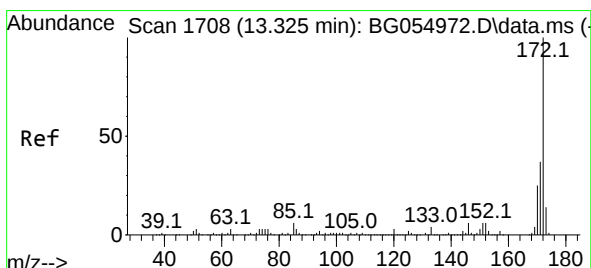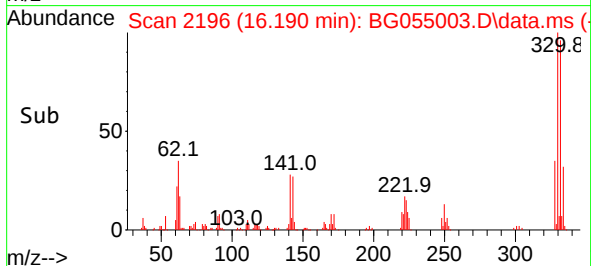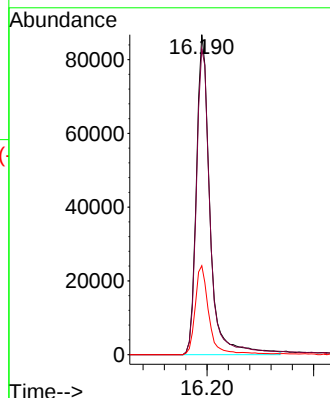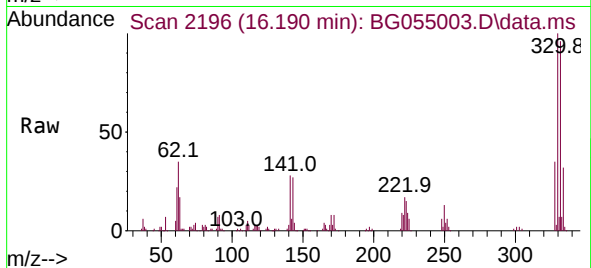

#45

2-Fluorobiphenyl

Concen: 77.513 ng

RT: 13.323 min Scan# 1708

Delta R.T. -0.002 min

Lab File: BG055003.D

Acq: 21 Sep 2022 21:28




Tgt Ion:172 Resp: 525718


Ion Ratio Lower Upper

172 100

171 36.5 31.2 46.8

170 24.4 20.6 30.8


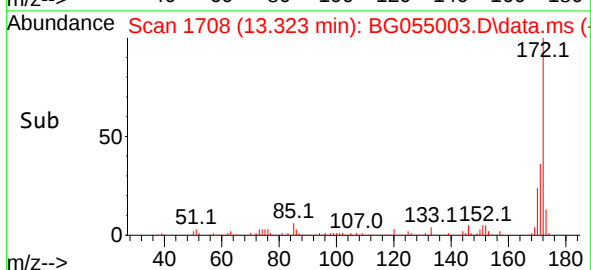
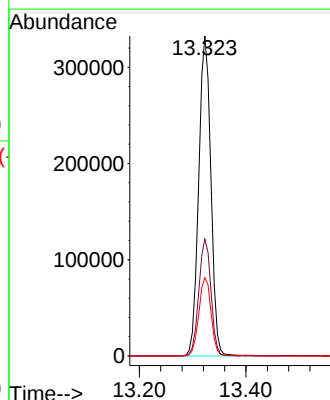
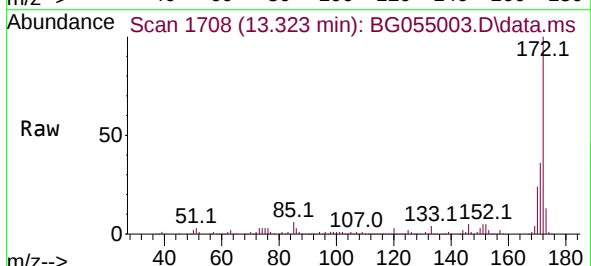


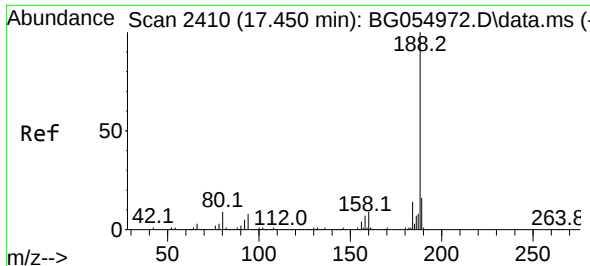

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.447 min Scan# 2410
Delta R.T. -0.003 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28




Instrument :
BNA_G
ClientSampleId :
SB-28-COMP


Tgt Ion:188 Resp: 258130
Ion Ratio Lower Upper
188 100
94 7.7 7.0 10.4
80 7.6 7.9 11.9#

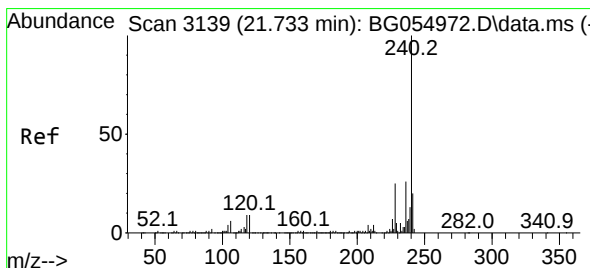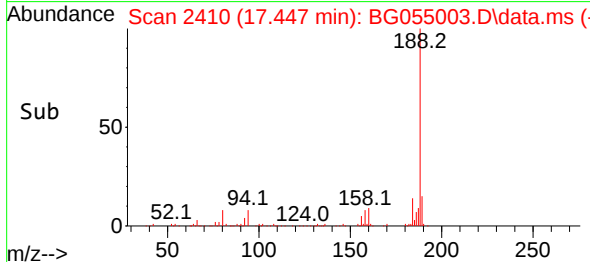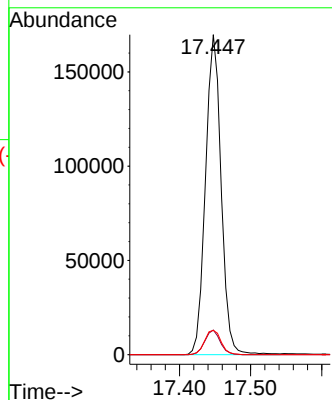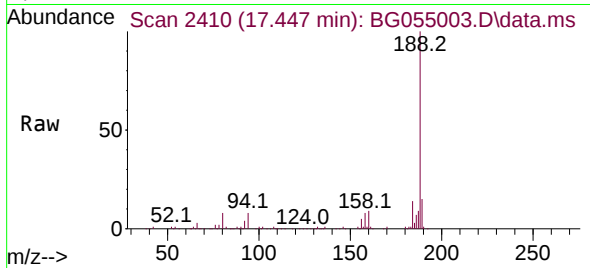

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.725 min Scan# 3138
Delta R.T. -0.008 min
Lab File: BG055003.D
Acq: 21 Sep 2022 21:28

Tgt Ion:240 Resp: 264465
Ion Ratio Lower Upper
240 100
120 8.6 8.2 12.4
236 26.2 21.2 31.8


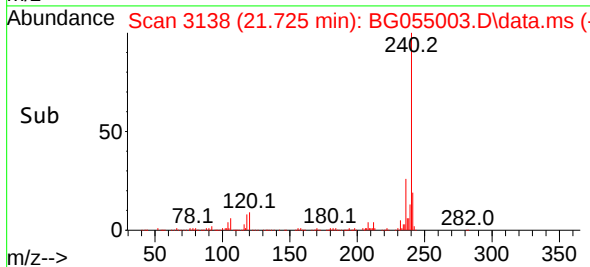
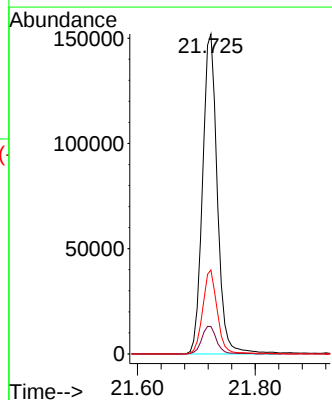
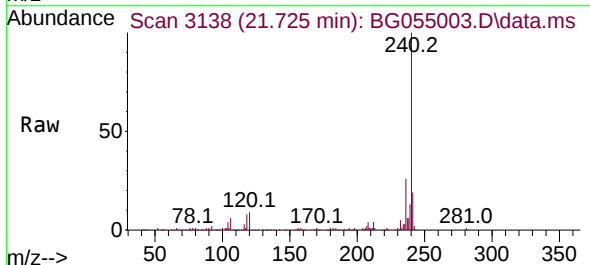


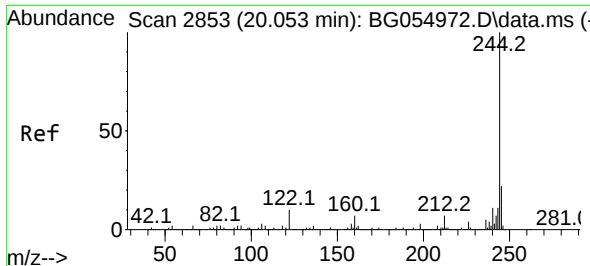

#79
 Terphenyl-d14
 Concen: 80.416 ng
 RT: 20.050 min Scan# 21
 Delta R.T. -0.002 min
 Lab File: BG055003.D
 Acq: 21 Sep 2022 21:28

Instrument :
 BNA_G
 ClientSampleId :
 SB-28-COMP

Tgt Ion:244 Resp: 1016687
 Ion Ratio Lower Upper
 244 100
 212 7.1 6.2 9.2
 122 8.7 9.0 13.6#

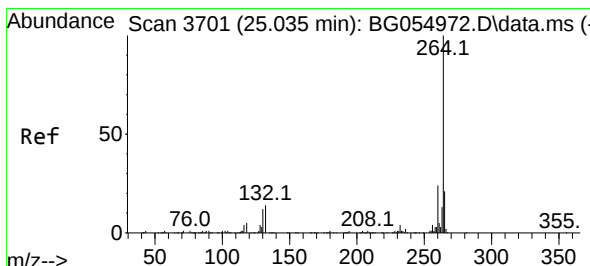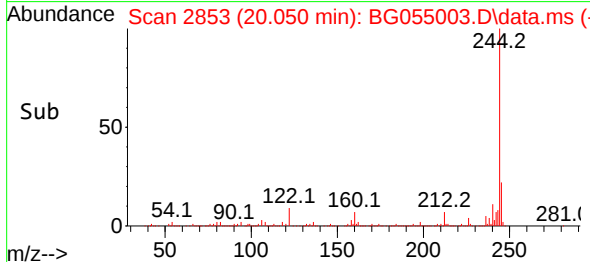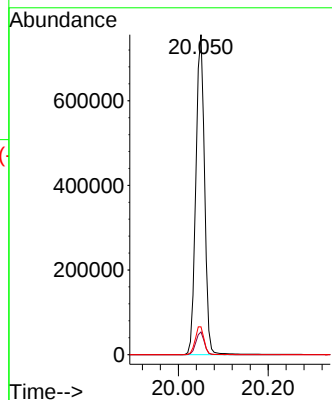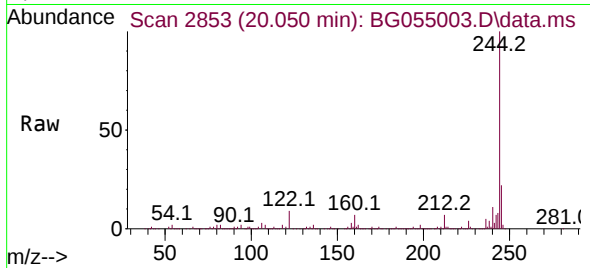

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.021 min Scan# 3699
 Delta R.T. -0.014 min
 Lab File: BG055003.D
 Acq: 21 Sep 2022 21:28

Tgt Ion:264 Resp: 277088
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.9 29.9
 265 20.8 16.9 25.3

