


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
 Data File : BG054992.D
 Acq On : 21 Sep 2022 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 17:41:40 2022

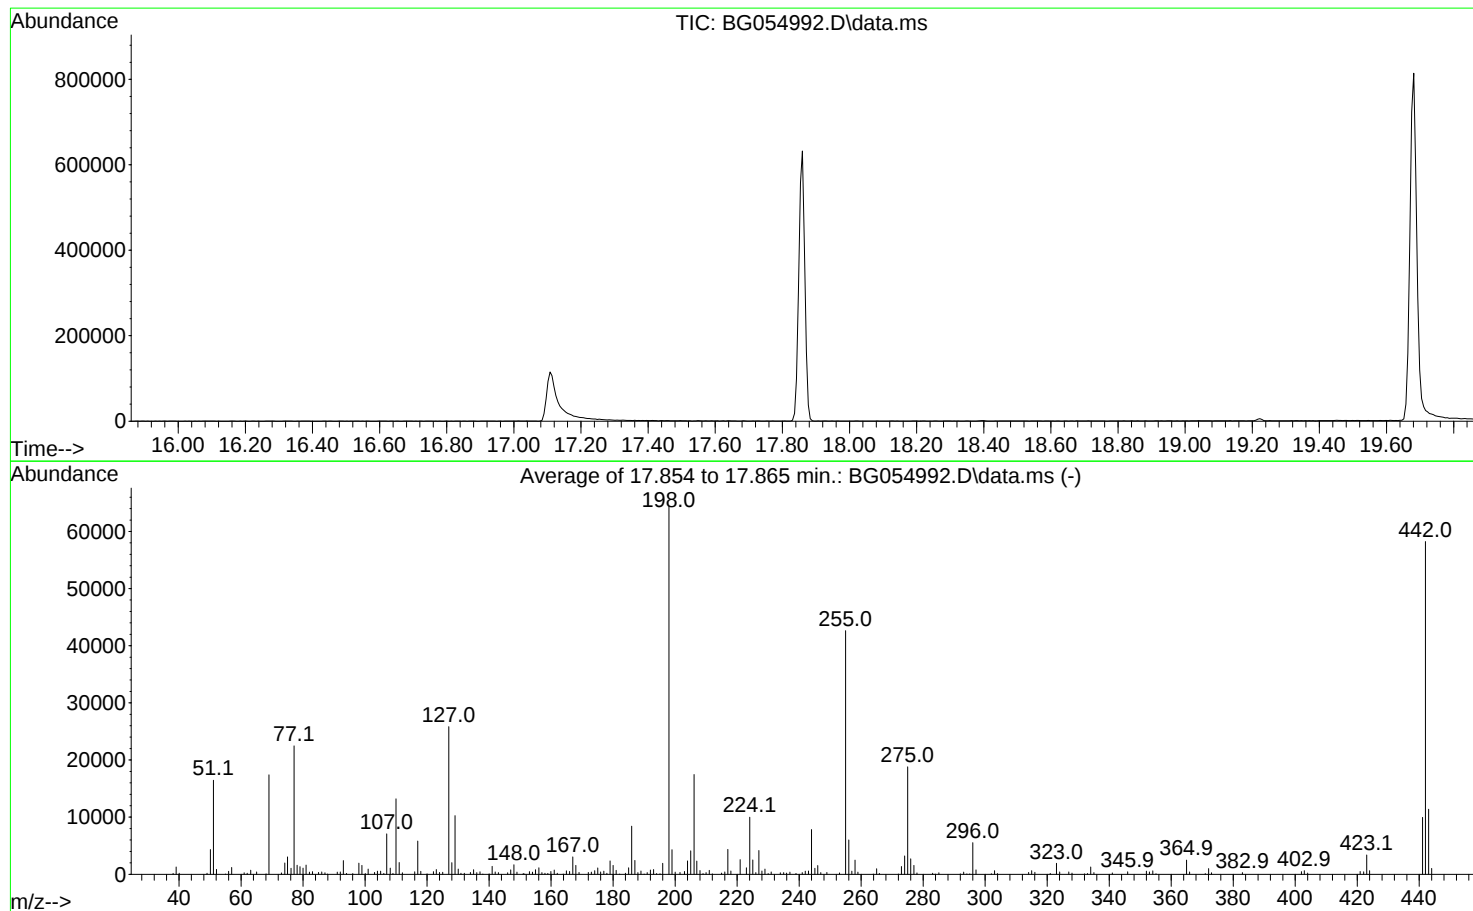




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	16454	PASS
68	69	0.00	2	0.5	80	PASS
69	198	0.00	100	27.0	17406	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.1	25845	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64384	PASS
199	198	5	9	6.7	4315	PASS
275	198	10	60	29.2	18818	PASS
365	198	1	100	3.9	2492	PASS
441	198	0.01	100	15.5	9963	PASS
442	442	50	100	100.0	58229	PASS
443	442	15	24	19.5	11376	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
Data File : BG054992.D
Acq On : 21 Sep 2022 11:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Sep 22 06:34:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 17:41:40 2022
Response via : Initial Calibration

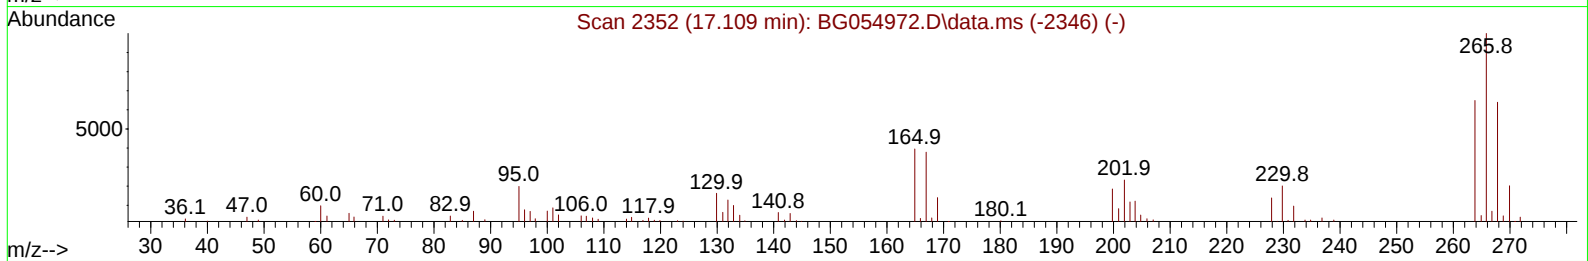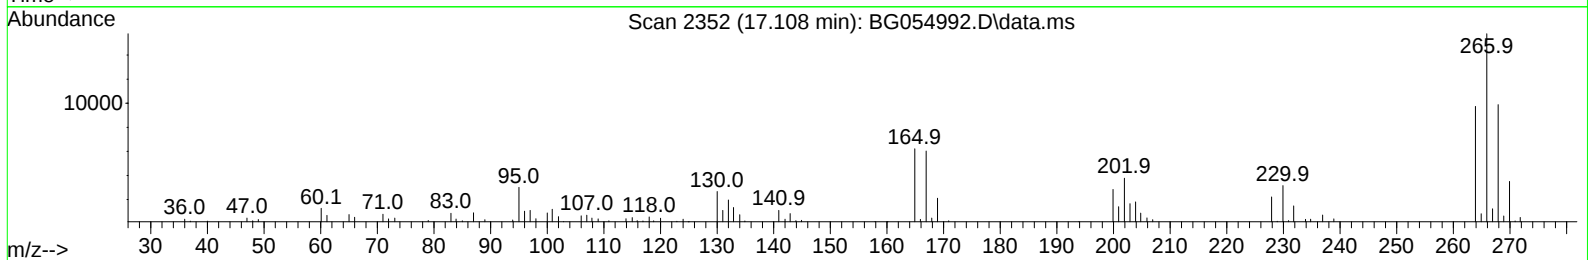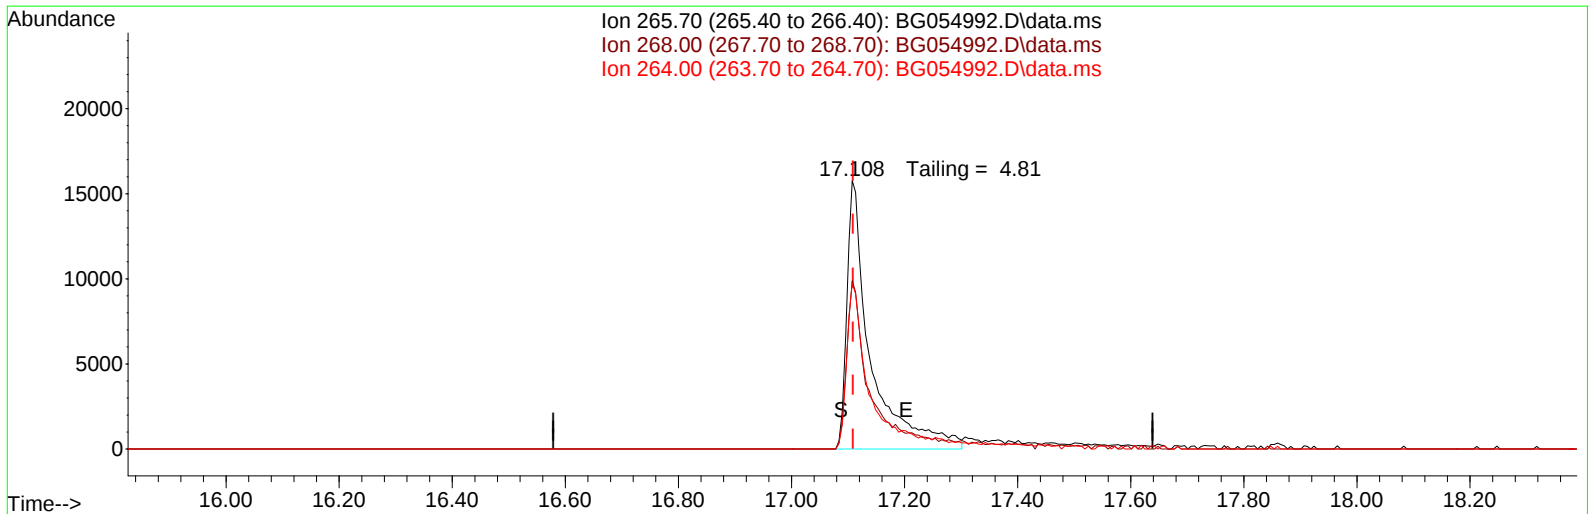

TIC: BG054992.D\data.ms

(70) Pentachlorophenol (C)

17.108min (-0.002) 2580.45 ng




response 45169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	62.70
264.00	61.70	61.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092122\
 Data File : BG054992.D
 Acq On : 21 Sep 2022 11:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 06:34:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG091922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 17:41:40 2022
 Response via : Initial Calibration

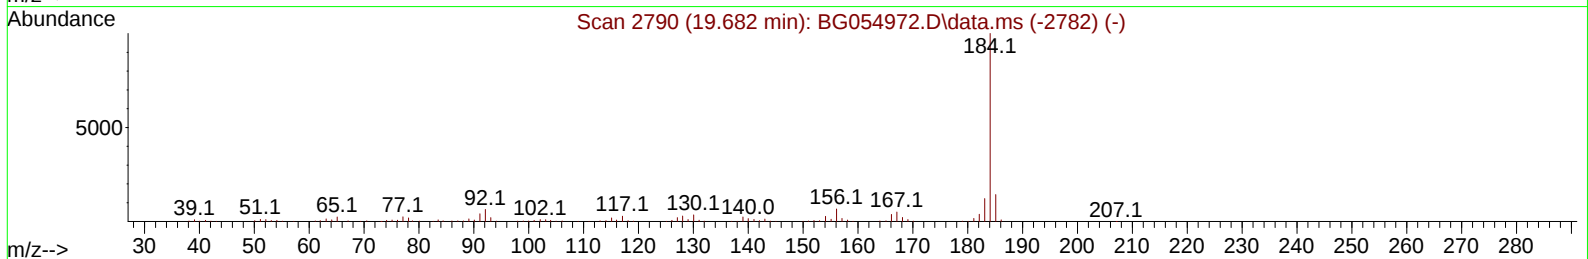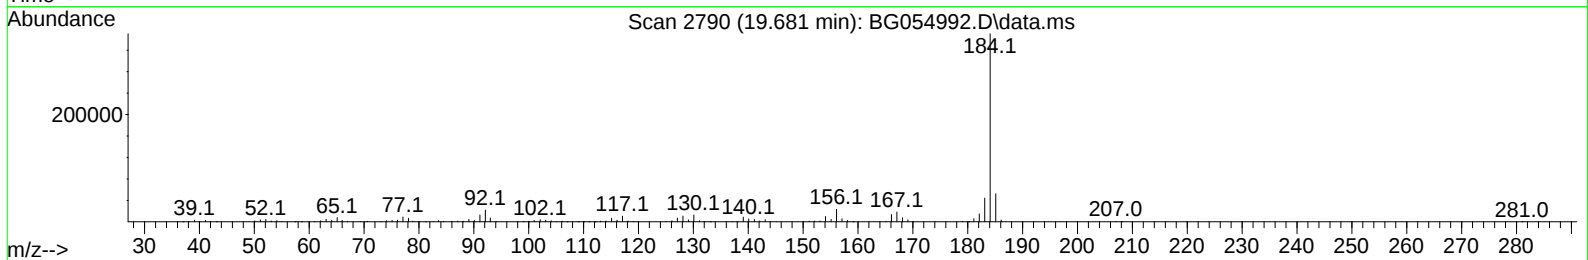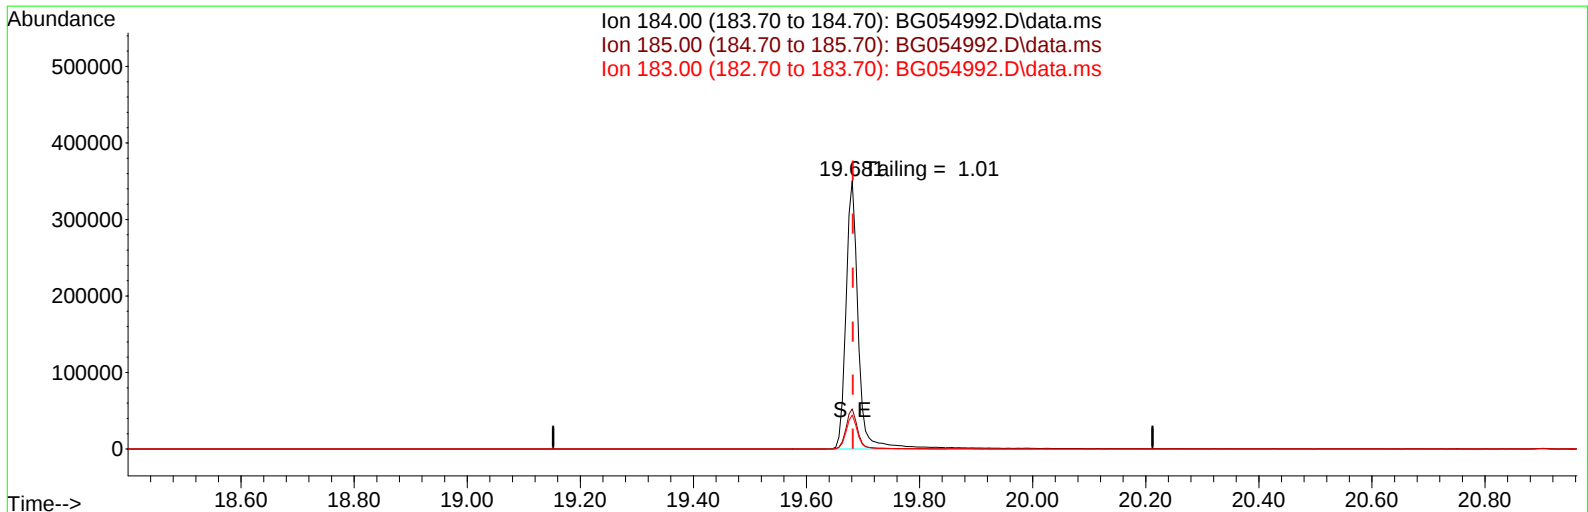

TIC: BG054992.D\data.ms

(77) Benzidine

19.681min (-0.001) 0.00 ng

response 529303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.96
183.00	12.30	12.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/21/2022	BNA_G	BG054992.D
Compound Name	Response	Retention Time
DDT	249913	20.903
DDD	8575	20.462
DDE	0	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8575	258488	3.32

Instrument :
BNA_G
ClientSampleId :
DFTPP