

Instrument :
BNA_G
LabSampleId :
SSTDCCC020

mohammad
9/29/2021 12:54:00 PM

[illegible]




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050311.D
 Acq On : 29 Sep 2021 9:17
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 9/29/2021 12:54:00 PM

Quant Time: Sep 29 10:57:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 29 10:57:11 2021
 Response via : Initial Calibration

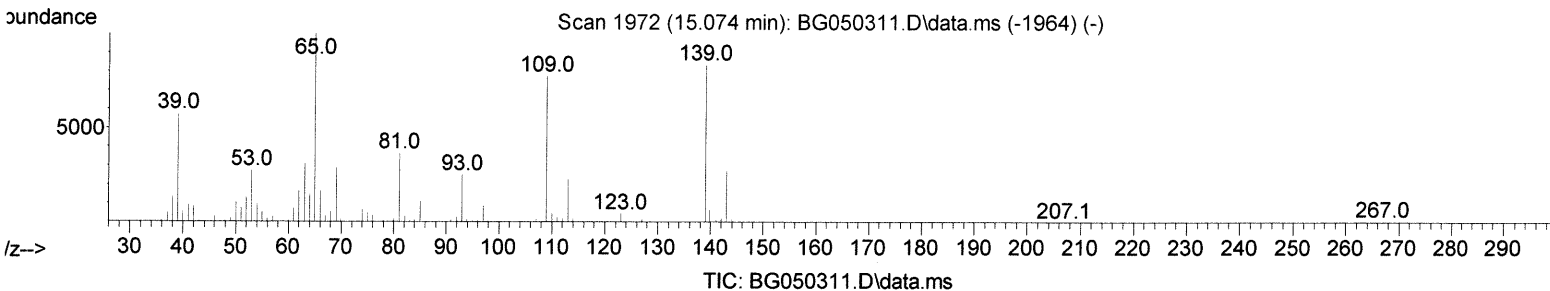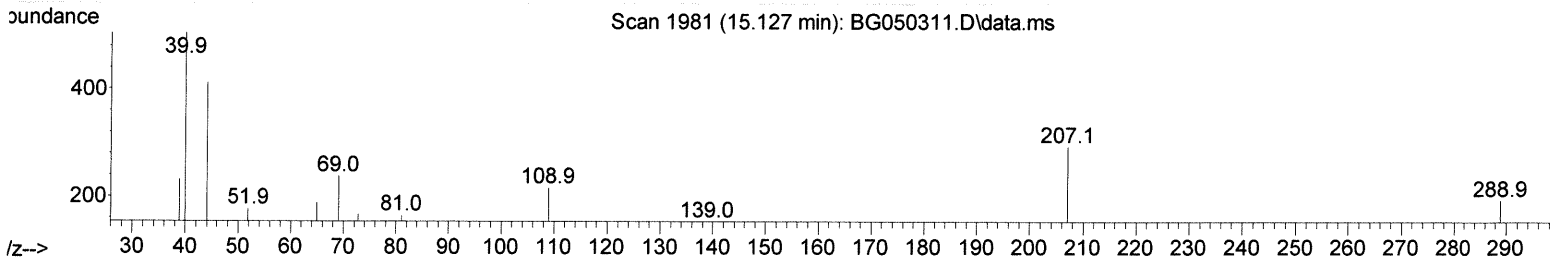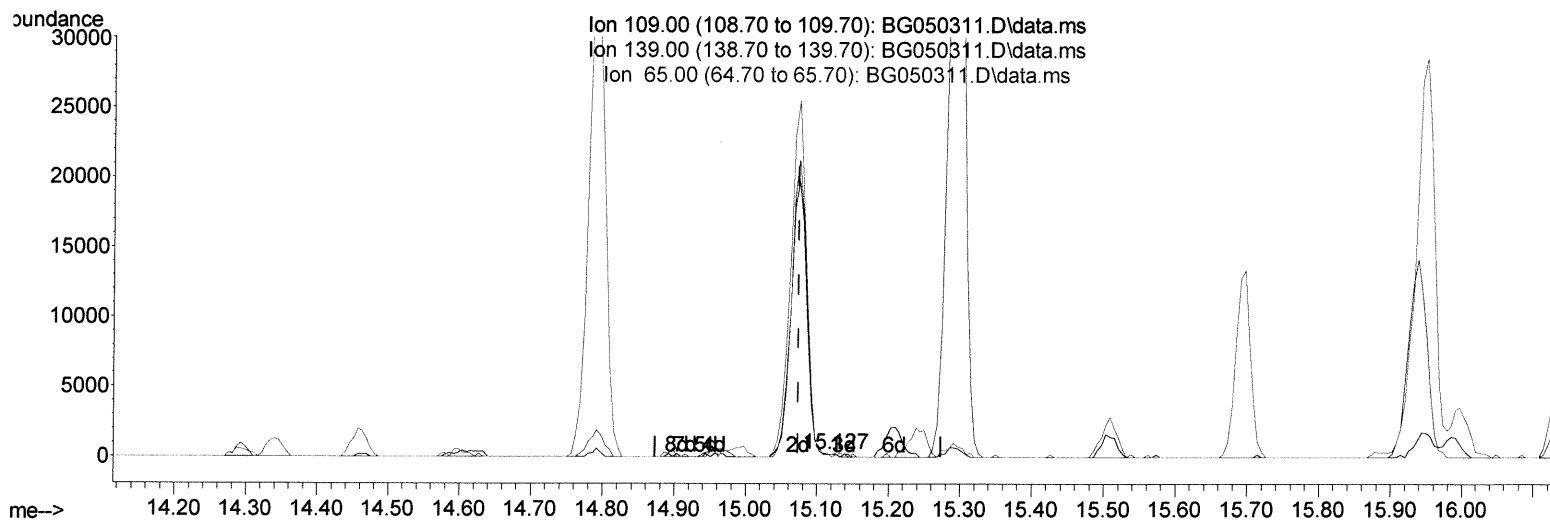

TIC: BG050311.D\data.ms

(55) 4-Nitrophenol

15.127min (+ 0.053) 0.09 ng/ul

response 140

Ion	Exp%	Act%
109.00	100.00	100.00
139.00	76.70	71.16
65.00	95.60	86.98
0.00	0.00	0.00

Instrument :
BNA_G
LabSampleId :
SSTDCCC020


mohammad
9/29/2021 12:54:00 PM

undance

Ion 109.00 (108.70 to 109.70): BG050311.D\data.ms
Ion 139.00 (138.70 to 139.70): BG050311.D\data.ms
Ion 65.00 (64.70 to 65.70): BG050311.D\data.ms

30000
20000
10000
0

15.074
15.054
15.034
15.014
14.994
14.974
14.954
14.934
14.914
14.894
14.874
14.854
14.834
14.814
14.794
14.774
14.754
14.734
14.714
14.694
14.674
14.654
14.634
14.614
14.594
14.574
14.554
14.534
14.514
14.494
14.474
14.454
14.434
14.414
14.394
14.374
14.354
14.334
14.314
14.294
14.274
14.254
14.234
14.214
14.194
14.174
14.154
14.134
14.114
14.094
14.074
14.054
14.034
14.014
13.994
13.974
13.954
13.934
13.914
13.894
13.874
13.854
13.834
13.814
13.794
13.774
13.754
13.734
13.714
13.694
13.674
13.654
13.634
13.614
13.594
13.574
13.554
13.534
13.514
13.494
13.474
13.454
13.434
13.414
13.394
13.374
13.354
13.334
13.314
13.294
13.274
13.254
13.234
13.214
13.194
13.174
13.154
13.134
13.114
13.094
13.074
13.054
13.034
13.014
12.994
12.974
12.954
12.934
12.914
12.894
12.874
12.854
12.834
12.814
12.794
12.774
12.754
12.734
12.714
12.694
12.674
12.654
12.634
12.614
12.594
12.574
12.554
12.534
12.514
12.494
12.474
12.454
12.434
12.414
12.394
12.374
12.354
12.334
12.314
12.294
12.274
12.254
12.234
12.214
12.194
12.174
12.154
12.134
12.114
12.094
12.074
12.054
12.034
12.014
11.994
11.974
11.954
11.934
11.914
11.894
11.874
11.854
11.834
11.814
11.794
11.774
11.754
11.734
11.714
11.694
11.674
11.654
11.634
11.614
11.594
11.574
11.554
11.534
11.514
11.494
11.474
11.454
11.434
11.414
11.394
11.374
11.354
11.334
11.314
11.294
11.274
11.254
11.234
11.214
11.194
11.174
11.154
11.134
11.114
11.094
11.074
11.054
11.034
11.014
10.994
10.974
10.954
10.934
10.914
10.894
10.874
10.854
10.834
10.814
10.794
10.774
10.754
10.734
10.714
10.694
10.674
10.654
10.634
10.614
10.594
10.574
10.554
10.534
10.514
10.494
10.474
10.454
10.434
10.414
10.394
10.374
10.354
10.334
10.314
10.294
10.274
10.254
10.234
10.214
10.194
10.174
10.154
10.134
10.114
10.094
10.074
10.054
10.034
10.014
9.994
9.974
9.954
9.934
9.914
9.894
9.874
9.854
9.834
9.814
9.794
9.774
9.754
9.734
9.714
9.694
9.674
9.654
9.634
9.614
9.594
9.574
9.554
9.534
9.514
9.494
9.474
9.454
9.434
9.414
9.394
9.374
9.354
9.334
9.314
9.294
9.274
9.254
9.234
9.214
9.194
9.174
9.154
9.134
9.114
9.094
9.074
9.054
9.034
9.014
8.994
8.974
8.954
8.934
8.914
8.894
8.874
8.854
8.834
8.814
8.794
8.774
8.754
8.734
8.714
8.694
8.674
8.654
8.634
8.614
8.594
8.574
8.554
8.534
8.514
8.494
8.474
8.454
8.434
8.414
8.394
8.374
8.354
8.334
8.314
8.294
8.274
8.254
8.234
8.214
8.194
8.174
8.154
8.134
8.114
8.094
8.074
8.054
8.034
8.014
7.994
7.974
7.954
7.934
7.914
7.894
7.874
7.854
7.834
7.814
7.794
7.774
7.754
7.734
7.714
7.694
7.674
7.654
7.634
7.614
7.594
7.574
7.554
7.534
7.514
7.494
7.474
7.454
7.434
7.414
7.394
7.374
7.354
7.334
7.314
7.294
7.274
7.254
7.234
7.214
7.194
7.174
7.154
7.134
7.114
7.094
7.074
7.054
7.034
7.014
6.994
6.974
6.954
6.934
6.914
6.894
6.874
6.854
6.834
6.814
6.794
6.774
6.754
6.734
6.714
6.694
6.674
6.654
6.634
6.614
6.594
6.574
6.554
6.534
6.514
6.494
6.474
6.454
6.434
6.414
6.394
6.374
6.354
6.334
6.314
6.294
6.274
6.254
6.234
6.214
6.194
6.174
6.154
6.134
6.114
6.094
6.074
6.054
6.034
6.014
5.994
5.974
5.954
5.934
5.914
5.894
5.874
5.854
5.834
5.814
5.794
5.774
5.754
5.734
5.714
5.694
5.674
5.654
5.634
5.614
5.594
5.574
5.554
5.534
5.514
5.494
5.474
5.454
5.434
5.414
5.394
5.374
5.354
5.334
5.314
5.294
5.274
5.254
5.234
5.214
5.194
5.174
5.154
5.134
5.114
5.094
5.074
5.054
5.034
5.014
4.994
4.974
4.954
4.934
4.914
4.894
4.874
4.854
4.834
4.814
4.794
4.774
4.754
4.734
4.714
4.694
4.674
4.654
4.634
4.614
4.594
4.574
4.554
4.534
4.5

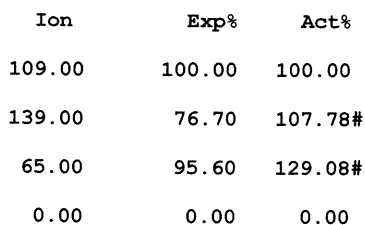

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050311.D
 Acq On : 29 Sep 2021 9:17
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 9/29/2021 12:54:00 PM

Quant Time: Sep 29 10:57:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Wed Sep 29 10:57:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.282	152	45639	20.000	ng/ul	0.00
20) Naphthalene-d8	11.108	136	189454	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.898	164	127216	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.642	188	291340	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.948	240	293732	20.000	ng/ul	# 0.00
88) Perylene-d12	25.386	264	310162	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.652	96	9766	10.348	ng/uL	0.00
4) Pyridine-d5	4.081	84	72298	25.418	ng/ul	0.00
7) Phenol-d5	7.412	99	77257	21.320	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.595	67	48541	23.079	ng/ul	0.00
11) 2-Chlorophenol-d4	7.806	132	56323	21.385	ng/ul	0.00
15) 4-Methylphenol-d8	8.969	113	58372	20.448	ng/ul	0.00
21) Nitrobenzene-d5	9.451	128	26902	22.986	ng/ul	0.00
24) 2-Nitrophenol-d4	10.174	143	29657	22.942	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.714	165	57889	19.197	ng/ul	0.00
31) 4-Chloroaniline-d4	11.232	131	75082	18.953	ng/ul	0.00
46) Dimethylphthalate-d6	14.293	166	171485	19.834	ng/ul	0.00
49) Acenaphthylene-d8	14.592	160	218194	20.076	ng/ul	0.00
54) 4-Nitrophenol-d4	15.062	143	31418	21.537	ng/ul	0.00
60) Fluorene-d10	15.885	176	151982	19.199	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.985	200	28881	23.399	ng/ul	0.00
73) Anthracene-d10	17.742	188	245550	19.788	ng/ul	0.00
81) Pyrene-d10	20.015	212	293711	18.469	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.145	264	309970	19.602	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.687	88	11188	9.397	ng/ul#	91
5) Pyridine	4.099	79	72809	24.683	ng/ul	93
6) Benzaldehyde	7.412	77	58976	25.641	ng/ul	95
8) Phenol	7.436	94	80996	22.065	ng/ul	95
10) Bis(2-Chloroethyl)ether	7.694	93	60965	22.347	ng/ul	96
12) 2-Chlorophenol	7.841	128	57333	20.655	ng/ul#	78
13) 2-Methylphenol	8.705	108	59148	20.652	ng/ul	96
14) 2,2'-oxybis(1-Chloropr...	8.811	45	87344	24.200	ng/ul#	91
16) Acetophenone	9.110	105	94193	21.600	ng/ul	97
17) N-Nitroso-di-n-propyla...	9.087	70	53666	21.648	ng/ul	98
18) 4-Methylphenol	9.034	108	62020	21.260	ng/ul	86
19) Hexachloroethane	9.375	117	25023	21.010	ng/ul	97
22) Nitrobenzene	9.492	77	79287	23.613	ng/ul	100
23) Isophorone	10.021	82	143119	20.208	ng/ul#	94
25) 2-Nitrophenol	10.209	139	31925	23.646	ng/ul#	85
26) 2,4-Dimethylphenol	10.250	107	71059	19.683	ng/ul	89
27) Bis(2-Chloroethoxy)met...	10.497	93	80418	20.800	ng/ul	97
29) 2,4-Dichlorophenol	10.738	162	55661	19.157	ng/ul	98
30) Naphthalene	11.155	128	191105	19.666	ng/ul	97
32) 4-Chloroaniline	11.255	127	77237	19.523	ng/ul	91
33) Hexachlorobutadiene	11.437	225	42780	17.748	ng/ul	96
34) Caprolactam	12.025	113	18533	20.228	ng/ul#	75
35) 4-Chloro-3-methylphenol	12.348	107	62737	19.910	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050311.D
 Acq On : 29 Sep 2021 9:17
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 LabSampleId :
 SSTDCCC020

Manual Integrations
 APPROVED

mohammad
 9/29/2021 12:54:00 PM

Quant Time: Sep 29 10:57:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 Last Update : Wed Sep 29 10:57:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.742	142	127524	18.949	ng/ul	97
37) 1-Methylnaphthalene	12.959	142	127981	18.835	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	13.100	216	78382	19.570	ng/ul	93
40) Hexachlorocyclopentadiene	13.076	237	52680	19.068	ng/ul	95
41) 2,4,6-Trichlorophenol	13.335	196	49001	20.747	ng/ul	87
42) 2,4,5-Trichlorophenol	13.400	196	52463	20.646	ng/ul	92
43) 1,1'-Biphenyl	13.734	154	174879	20.264	ng/ul#	96
44) 2-Chloronaphthalene	13.781	162	136254	19.954	ng/ul	100
45) 2-Nitroaniline	13.975	65	43573	26.801	ng/ul	96
47) Dimethylphthalate	14.340	163	171498	19.691	ng/ul	99
48) 2,6-Dinitrotoluene	14.463	165	33910	24.595	ng/ul	91
50) Acenaphthylene	14.622	152	223196	20.328	ng/ul	97
51) 3-Nitroaniline	14.792	138	35624	23.110	ng/ul	86
52) Acenaphthene	14.962	153	144517	20.104	ng/ul	98
53) 2,4-Dinitrophenol	14.992	184	20005	22.917	ng/ul#	84
55) 4-Nitrophenol	15.074	109	31028m	20.697	ng/ul	93
56) Dibenzofuran	15.291	168	215444	20.027	ng/ul	93
57) 2,4-Dinitrotoluene	15.244	165	48040	24.587	ng/ul#	98
58) 2,3,4,6-Tetrachlorophenol	15.509	232	45598	19.946	ng/ul#	93
59) Diethylphthalate	15.697	149	176659	19.730	ng/ul	98
61) Fluorene	15.938	166	166534	19.760	ng/ul	97
62) 4-Chlorophenyl-phenyle...	15.926	204	90896	19.159	ng/ul	95
63) 4-Nitroaniline	15.950	138	36432	22.959	ng/ul#	81
66) 4,6-Dinitro-2-methylph...	16.002	198	28728	23.168	ng/ul	98
67) N-Nitrosodiphenylamine	16.138	169	147305	19.996	ng/ul	98
68) 4-Bromophenyl-phenylether	16.825	248	56655	18.754	ng/ul	97
69) Hexachlorobenzene	16.942	284	63759	19.049	ng/ul	96
70) Atrazine	17.078	200	62401	19.198	ng/ul	93
71) Pentachlorophenol	17.277	266	40603	19.012	ng/ul	96
72) Phenanthrene	17.683	178	286051	19.783	ng/ul	98
74) Anthracene	17.777	178	288202	20.013	ng/ul	95
75) 1,2,3,4-Tetrachloroben...	13.705	216	82123	19.829	ng/ul	90
76) Pentachlorobenzene	15.209	250	77939	19.517	ng/ul	98
77) Carbazole	18.035	167	263375	20.672	ng/ul	98
78) Di-n-butylphthalate	18.582	149	310591	21.143	ng/ul	98
80) Fluoranthene	19.680	202	370302	18.366	ng/ul#	91
82) Pyrene	20.039	202	364618	18.391	ng/ul#	89
83) Butylbenzylphthalate	20.920	149	134035	20.068	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.831	252	127038	20.195	ng/ul#	93
85) Benzo(a)anthracene	21.925	228	351047	19.846	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.813	149	193781	20.326	ng/ul	98
87) Chrysene	21.995	228	337255	19.667	ng/ul	94
89) Di-n-octyl phthalate	23.106	149	328228	21.588	ng/ul	100
90) Benzo(b)fluoranthene	24.281	252	358193	19.729	ng/ul#	98
91) Benzo(k)fluoranthene	24.357	252	334294	19.609	ng/ul#	97
93) Benzo(a)pyrene	25.221	252	340858	19.766	ng/ul#	98
94) Indeno(1,2,3-cd)pyrene	29.328	276	393954	19.550	ng/ul#	93
95) Dibenzo(a,h)anthracene	29.404	278	335341	19.308	ng/ul#	97
96) Benzo(g,h,i)perylene	30.562	276	327500	18.995	ng/ul#	96

29/10/04/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed