

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050306.D
 Acq On : 29 Sep 2021 5:54
 Operator : CG/JU
 Sample : M3755-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AL2

Quant Time: Sep 29 07:06:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 27 03:10:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.282	152	46782	20.000	ng/ul	0.00
20) Naphthalene-d8	11.109	136	188701	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.898	164	125630	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.642	188	285924	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.943	240	289184	20.000	ng/ul	#-0.01
88) Perylene-d12	25.386	264	293948	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.658	96	2888	2.985	ng/uL	0.00
4) Pyridine-d5	4.087	84	26922	9.234	ng/ul	0.00
7) Phenol-d5	7.413	99	51243	13.796	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.595	67	33894	15.721	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.807	132	38244	14.166	ng/ul	0.00
15) 4-Methylphenol-d8	8.970	113	39089	13.359	ng/ul	-0.01
21) Nitrobenzene-d5	9.452	128	19029	16.324	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.174	143	20064	15.583	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.709	165	36674	12.210	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.232	131	48361	12.257	ng/ul	-0.01
46) Dimethylphthalate-d6	14.293	166	125280	14.673	ng/ul	-0.01
49) Acenaphthylene-d8	14.593	160	153381	14.291	ng/ul	-0.01
54) 4-Nitrophenol-d4	15.057	143	17461	12.121	ng/ul	-0.01
60) Fluorene-d10	15.885	176	111412	14.252	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.985	200	15333	12.658	ng/ul	0.00
73) Anthracene-d10	17.736	188	179546	14.743	ng/ul	-0.01
81) Pyrene-d10	20.010	212	235039	15.012	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.145	264	225464	15.044	ng/ul	-0.02
Target Compounds						
80) Fluoranthene	19.681	202	19949	1.005	ng/ul#	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050306.D
Acq On : 29 Sep 2021 5:54
Operator : CG/JU
Sample : M3755-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AL2

Quant Time: Sep 29 07:06:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 27 03:10:48 2021
Response via : Initial Calibration

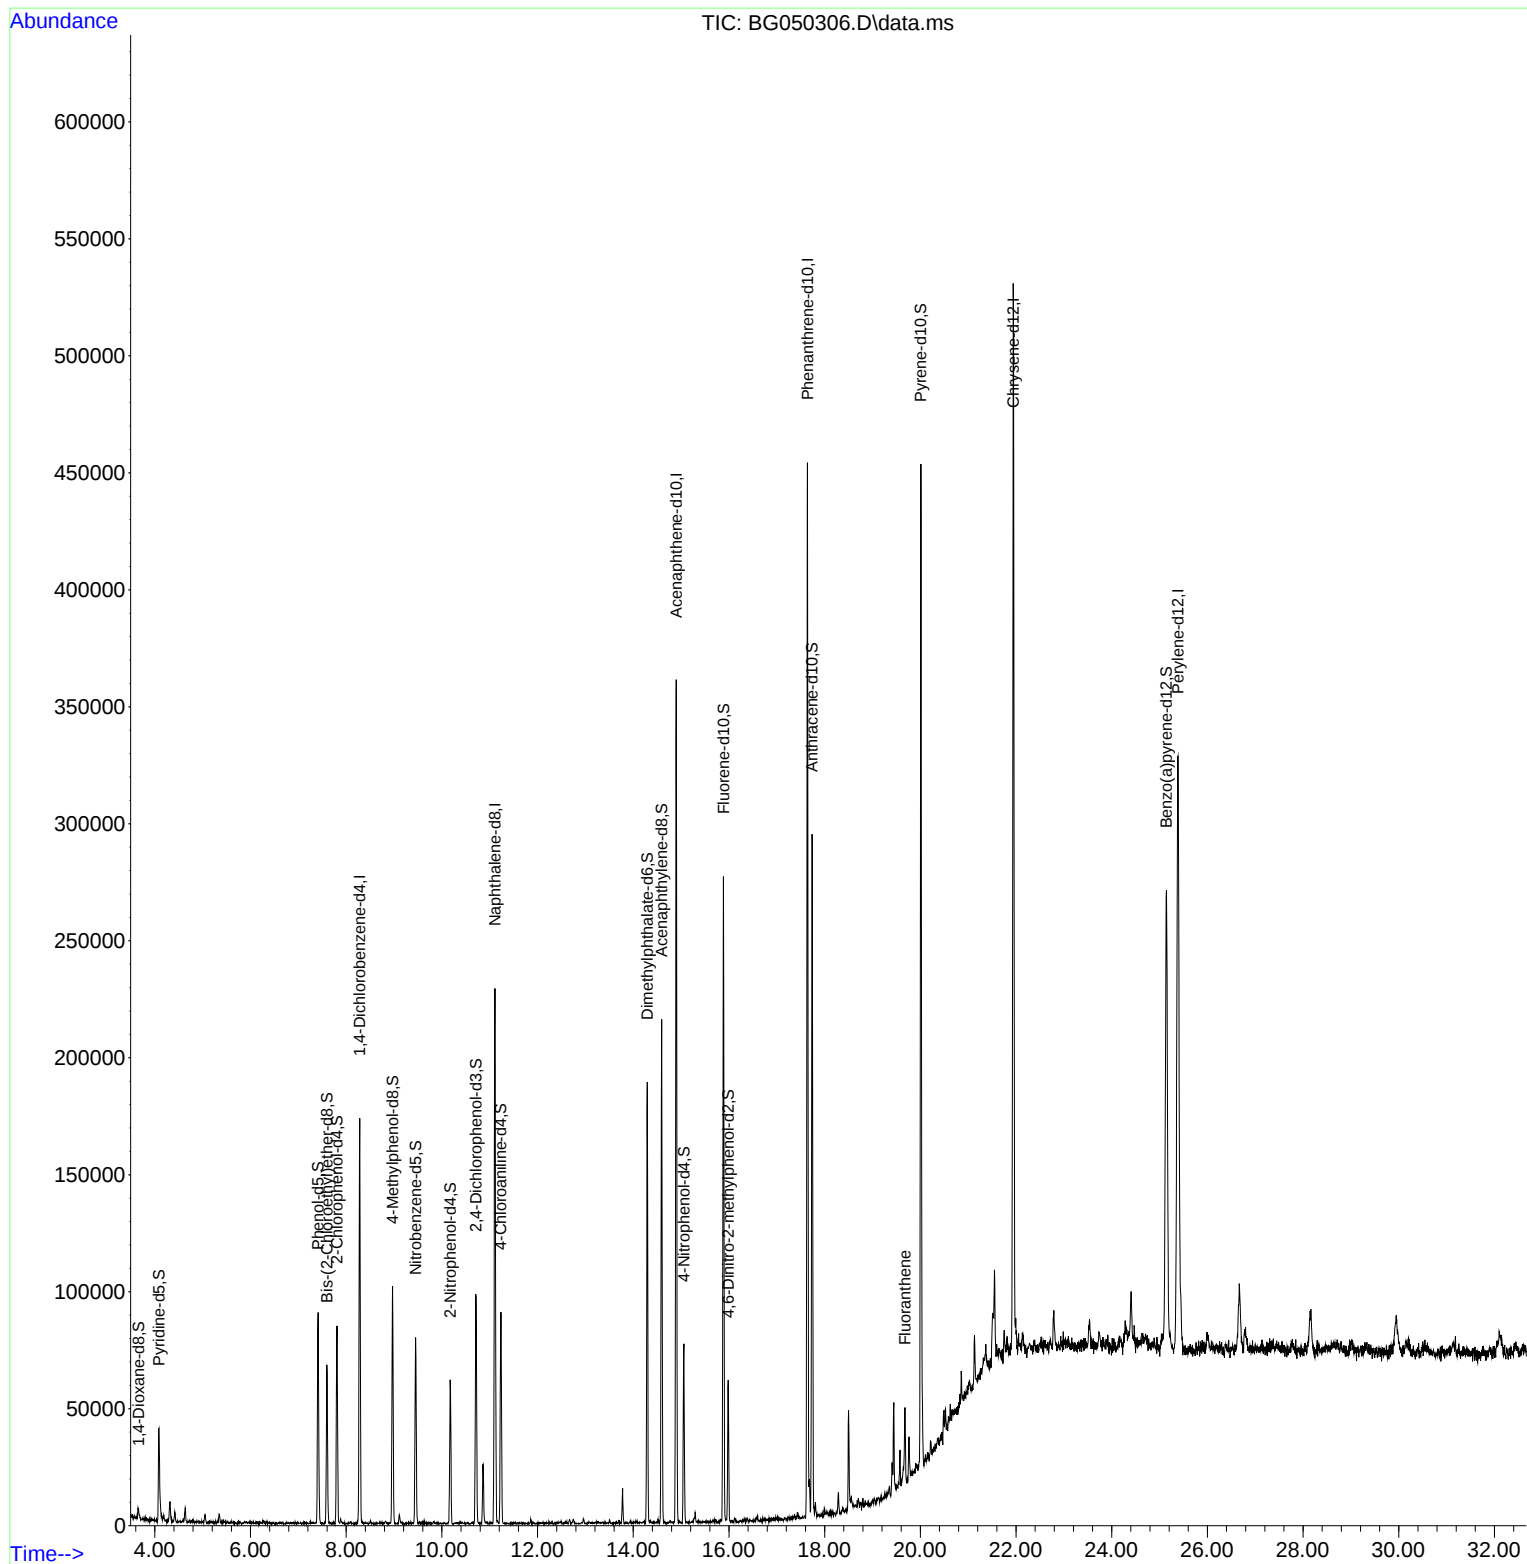

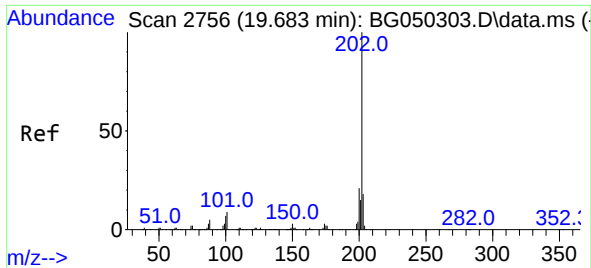

#80
Fluoranthene
Concen: 1.005 ng/ul
RT: 19.681 min Scan# 2756
Delta R.T. -0.009 min
Lab File: BG050306.D
Acq: 29 Sep 2021 5:54

Instrument :
BNA_G
ClientSampleId :
C0AL2

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.2	4.3	6.5#
100	5.5	3.5	5.3#

