

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050312.D
 Acq On : 29 Sep 2021 10:20
 Operator : CG/JU
 Sample : PB138259BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.518	3	5	8	rVB3	1392	1233	0.10%	0.009%
2	3.547	8	10	13	rVB2	1807	1637	0.13%	0.013%
3	3.577	13	15	18	rBV3	1997	2015	0.17%	0.015%
4	3.653	23	28	34	rBV2	11325	21141	1.74%	0.162%
5	3.753	44	45	51	rVB3	1121	1733	0.14%	0.013%
6	3.800	51	53	56	rVV2	1408	1651	0.14%	0.013%
7	3.888	65	68	70	rVB3	1149	1233	0.10%	0.009%
8	4.029	88	92	94	rBV3	1483	2125	0.18%	0.016%
9	4.082	96	101	117	rVV	152272	302708	24.95%	2.323%
10	4.358	143	148	149	rBV3	965	1342	0.11%	0.010%
11	4.411	155	157	163	rVB5	2724	5339	0.44%	0.041%
12	4.746	212	214	219	rVV4	1141	1825	0.15%	0.014%
13	5.116	272	277	279	rVB2	1219	1763	0.15%	0.014%
14	5.151	279	283	285	rVV2	1062	1234	0.10%	0.009%
15	5.821	394	397	401	rBV2	1394	1575	0.13%	0.012%
16	6.579	522	526	530	rVV2	1120	1625	0.13%	0.012%
17	7.413	658	668	676	rBV	210927	362956	29.91%	2.786%
18	7.595	692	699	709	rBV	149308	261605	21.56%	2.008%
19	7.807	727	735	744	rBV	191952	343384	28.30%	2.635%
20	8.283	809	816	823	rBV	172779	296911	24.47%	2.279%
21	8.970	925	933	942	rBV2	241527	415696	34.26%	3.190%
22	9.452	1001	1015	1023	rVV	185943	335345	27.63%	2.574%
23	10.181	1130	1139	1147	rVB	146974	263564	21.72%	2.023%
24	10.715	1223	1230	1239	rBV	223266	407351	33.57%	3.126%
25	11.109	1289	1297	1305	rBV	220159	412752	34.01%	3.168%
26	11.232	1310	1318	1326	rBV	233040	421961	34.77%	3.238%
27	12.672	1559	1563	1570	rBV4	4301	6840	0.56%	0.052%
28	13.647	1724	1729	1731	rBV3	1164	1339	0.11%	0.010%
29	14.293	1832	1839	1846	rBV	425113	613094	50.52%	4.705%
30	14.599	1883	1891	1897	rBV	449648	734004	60.49%	5.633%
31	14.899	1935	1942	1950	rVB	361113	578807	47.70%	4.442%
32	15.057	1962	1969	1977	rBV	207843	324977	26.78%	2.494%
33	15.886	2103	2110	2118	rVB	582454	911808	75.14%	6.998%
34	15.986	2121	2127	2134	rBV	171915	255947	21.09%	1.964%
35	16.127	2146	2151	2155	rVV3	3389	5915	0.49%	0.045%
36	16.461	2202	2208	2211	rVB5	822	1617	0.13%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050312.D
 Acq On : 29 Sep 2021 10:20
 Operator : CG/JU
 Sample : PB138259BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK259

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

37	16.555	2219	2224	2227	rBV3	805	1518	0.13%	0.012%
38	16.661	2239	2242	2247	rBV3	1570	2375	0.20%	0.018%
39	16.743	2253	2256	2259	rVB4	1387	1471	0.12%	0.011%
40	17.425	2369	2372	2374	rBV5	2133	2661	0.22%	0.020%
41	17.642	2401	2409	2416	rBV	469827	726046	59.83%	5.572%
42	17.742	2419	2426	2434	rVB	657711	1019501	84.01%	7.824%
43	18.060	2479	2480	2485	rBV3	1121	1578	0.13%	0.012%
44	18.365	2529	2532	2534	rVB4	1230	1548	0.13%	0.012%
45	18.565	2563	2566	2569	rBV4	1764	2152	0.18%	0.017%
46	18.653	2579	2581	2583	rVB3	2152	1398	0.12%	0.011%
47	18.671	2583	2584	2587	rBV3	1206	1257	0.10%	0.010%
48	18.741	2592	2596	2599	rVB4	1333	2174	0.18%	0.017%
49	18.847	2613	2614	2618	rVB2	2250	1787	0.15%	0.014%
50	18.988	2636	2638	2639	rBV	1560	1302	0.11%	0.010%
51	19.117	2659	2660	2663	rBV3	2372	2284	0.19%	0.018%
52	19.176	2669	2670	2673	rVV3	2230	1869	0.15%	0.014%
53	19.399	2706	2708	2711	rBV3	1833	1363	0.11%	0.010%
54	19.581	2735	2739	2742	rBV5	6535	9218	0.76%	0.071%
55	19.652	2747	2751	2755	rVB2	9384	13327	1.10%	0.102%
56	19.728	2762	2764	2766	rBV2	2298	1864	0.15%	0.014%
57	19.899	2789	2793	2794	rBV4	4821	6664	0.55%	0.051%
58	20.016	2806	2813	2820	rBV	846668	1213481	100.00%	9.313%
59	21.949	3135	3142	3149	rBV	449526	781260	64.38%	5.996%
60	25.151	3676	3687	3698	rVB2	384169	1133224	93.39%	8.697%
61	25.386	3717	3727	3744	rVB2	253679	792518	65.31%	6.082%




Sum of corrected areas: 13029892

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050312.D
Acq On : 29 Sep 2021 10:20
Operator : CG/JU
Sample : PB138259BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK259

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

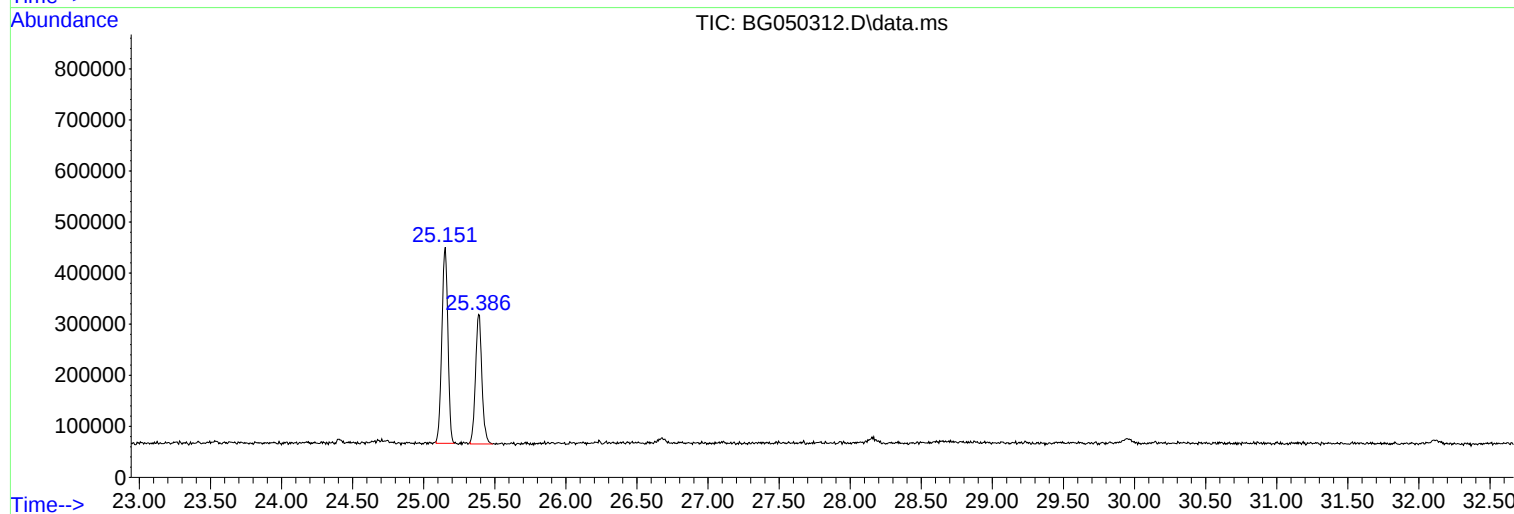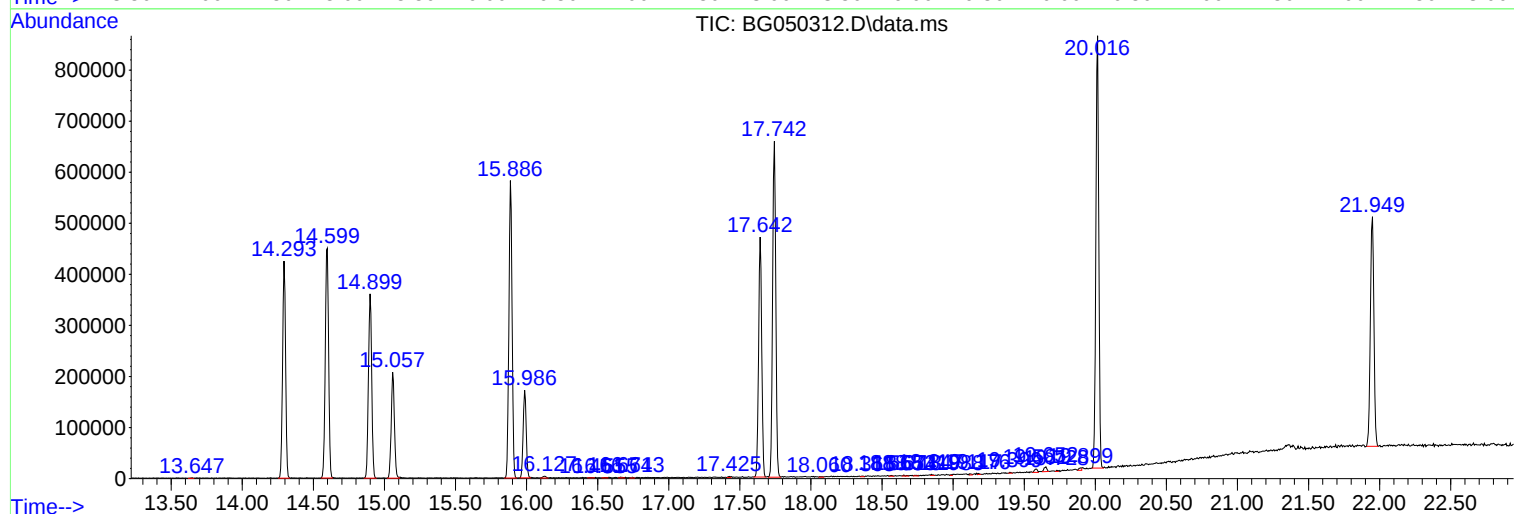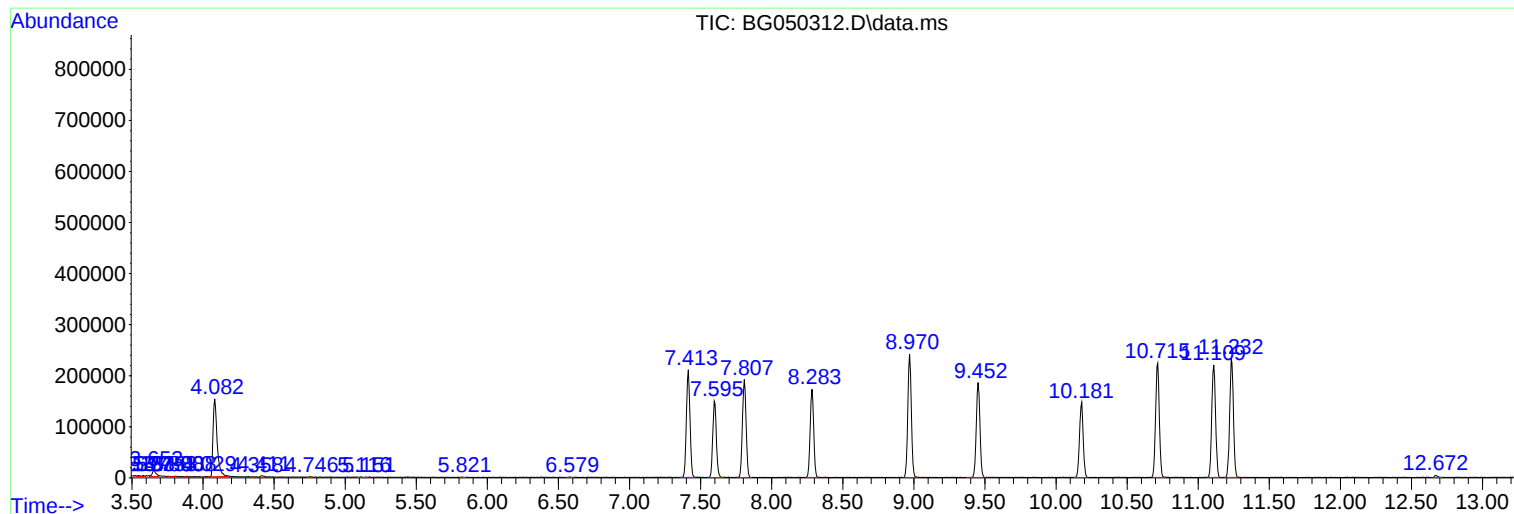

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050312.D
Acq On : 29 Sep 2021 10:20
Operator : CG/JU
Sample : PB138259BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK259

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050312.D
Acq On : 29 Sep 2021 10:20
Operator : CG/JU
Sample : PB138259BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK259

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
