

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050314.D
 Acq On : 29 Sep 2021 16:12
 Operator : CG/JU
 Sample : PB139036BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	14	17	19	rVB2	1517	1764	0.15%	0.014%
2	3.617	19	22	24	rBV3	1315	1484	0.13%	0.012%
3	3.652	24	28	36	rVB2	11146	18784	1.62%	0.153%
4	4.081	95	101	116	rBV	144374	284960	24.60%	2.323%
5	4.416	154	158	165	rVB3	2677	5432	0.47%	0.044%
6	6.607	527	531	533	rBV2	998	1367	0.12%	0.011%
7	7.160	623	625	632	rVB3	1201	1501	0.13%	0.012%
8	7.412	660	668	678	rVB2	194273	340837	29.43%	2.778%
9	7.595	693	699	710	rVV	137998	243050	20.98%	1.981%
10	7.806	727	735	743	rBV	184529	318702	27.52%	2.598%
11	8.282	809	816	823	rBV	157739	275148	23.76%	2.243%
12	8.969	925	933	941	rBV	225352	389773	33.65%	3.177%
13	9.451	1007	1015	1024	rVV	172185	316609	27.33%	2.581%
14	9.516	1024	1026	1033	rVB2	741	1339	0.12%	0.011%
15	10.180	1131	1139	1147	rBV	136821	250443	21.62%	2.041%
16	10.714	1223	1230	1240	rBV	219627	391889	33.83%	3.194%
17	11.108	1288	1297	1307	rBV	209753	388078	33.50%	3.163%
18	11.237	1309	1319	1328	rBV	212921	395128	34.11%	3.221%
19	12.677	1558	1564	1568	rVB4	3737	6479	0.56%	0.053%
20	14.293	1833	1839	1847	rVB	385193	571030	49.30%	4.655%
21	14.598	1883	1891	1900	rVB	424359	681302	58.82%	5.554%
22	14.898	1934	1942	1949	rVB	330256	534508	46.15%	4.357%
23	15.056	1960	1969	1980	rBV	191752	307119	26.52%	2.503%
24	15.544	2050	2052	2054	rBV2	939	1164	0.10%	0.009%
25	15.885	2102	2110	2119	rBV	564166	848492	73.26%	6.916%
26	15.985	2121	2127	2134	rVV	158282	241058	20.81%	1.965%
27	16.126	2147	2151	2158	rVB5	3182	5424	0.47%	0.044%
28	16.484	2209	2212	2213	rBV3	962	1292	0.11%	0.011%
29	16.590	2227	2230	2233	rBV3	926	1164	0.10%	0.009%
30	17.430	2368	2373	2377	rBV3	2346	4391	0.38%	0.036%
31	17.642	2403	2409	2415	rVV	440583	671773	58.00%	5.476%
32	17.741	2418	2426	2433	rBV2	610565	946879	81.75%	7.718%
33	17.818	2436	2439	2444	rBV5	2022	3897	0.34%	0.032%
34	17.929	2457	2458	2462	rBV4	1122	1465	0.13%	0.012%
35	18.053	2478	2479	2481	rBV2	1583	1439	0.12%	0.012%
36	18.141	2490	2494	2496	rVV3	1585	1654	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
 Data File : BG050314.D
 Acq On : 29 Sep 2021 16:12
 Operator : CG/JU
 Sample : PB139036BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK036

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
 Title : SVOA CALIBRATION

37	18.282	2516	2518	2520	rBV3	1200	1165	0.10%	0.009%
38	18.347	2526	2529	2530	rBV3	1162	1168	0.10%	0.010%
39	18.452	2545	2547	2549	rBV2	1568	1344	0.12%	0.011%
40	18.570	2565	2567	2570	rVB3	1795	1799	0.16%	0.015%
41	18.758	2598	2599	2603	rVB3	1660	1493	0.13%	0.012%
42	18.834	2608	2612	2613	rBV4	1252	1212	0.10%	0.010%
43	18.981	2635	2637	2640	rVB4	2669	3028	0.26%	0.025%
44	19.228	2676	2679	2680	rBV3	1537	1305	0.11%	0.011%
45	19.363	2699	2702	2703	rBV3	2089	1921	0.17%	0.016%
46	19.580	2736	2739	2745	rBV8	5936	9788	0.85%	0.080%
47	19.651	2747	2751	2755	rBV3	9511	13115	1.13%	0.107%
48	19.757	2767	2769	2770	rBV2	2821	1636	0.14%	0.013%
49	20.015	2806	2813	2819	rBV	795385	1158271	100.00%	9.442%
50	21.948	3135	3142	3149	rBV2	412182	741557	64.02%	6.045%
51	25.145	3677	3686	3699	rVB2	376674	1114749	96.24%	9.087%
52	25.385	3718	3727	3742	rVB2	240739	757294	65.38%	6.173%




Sum of corrected areas: 12267663

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050314.D
Acq On : 29 Sep 2021 16:12
Operator : CG/JU
Sample : PB139036BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

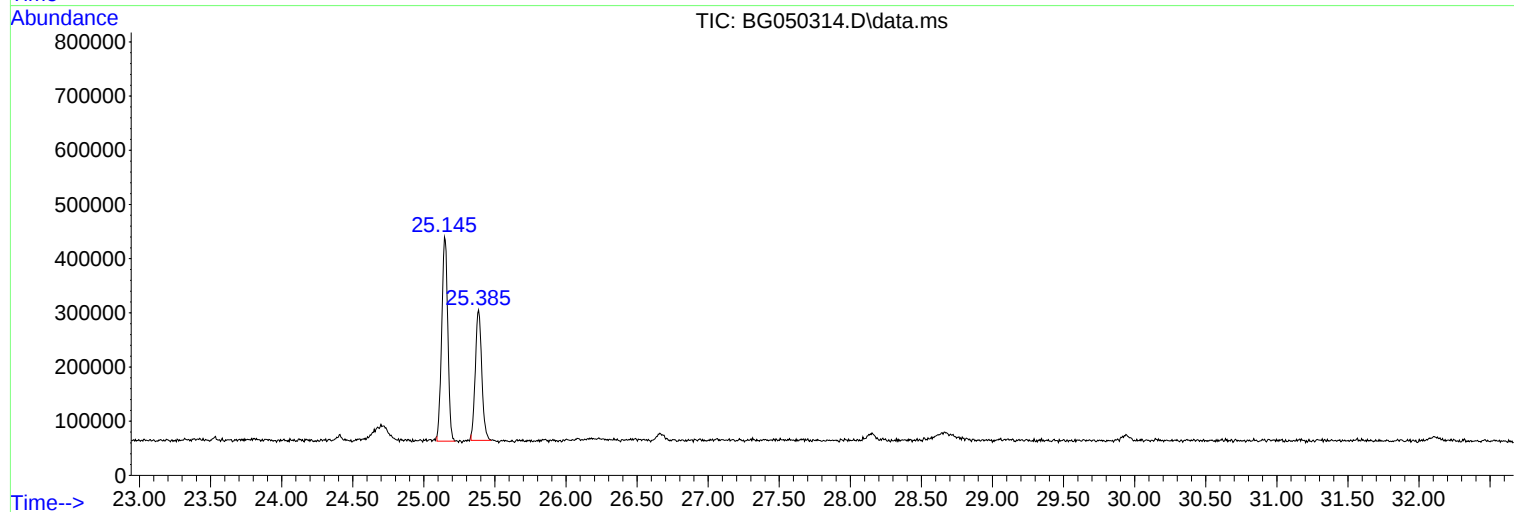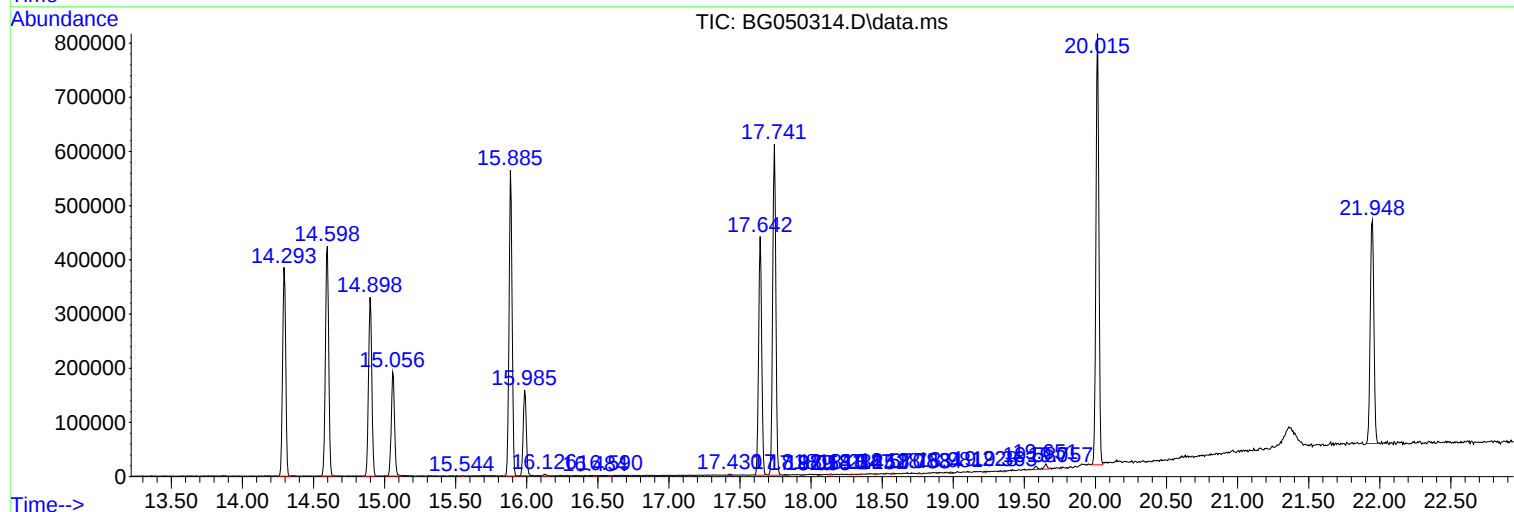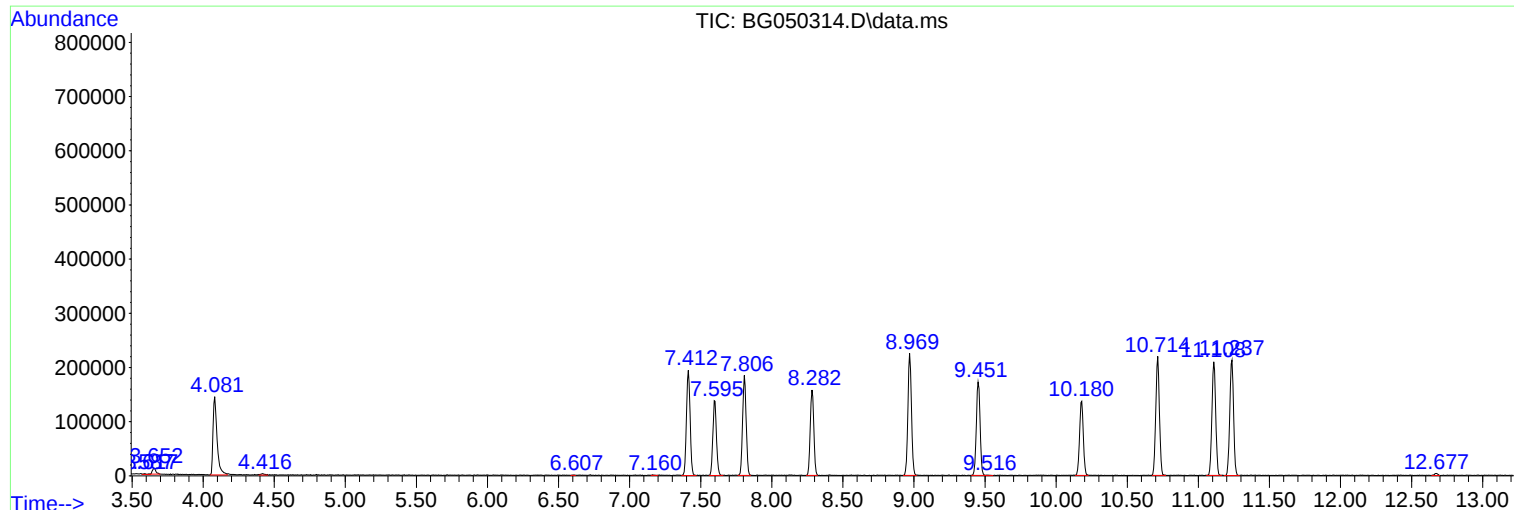

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050314.D
Acq On : 29 Sep 2021 16:12
Operator : CG/JU
Sample : PB139036BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG092821\
Data File : BG050314.D
Acq On : 29 Sep 2021 16:12
Operator : CG/JU
Sample : PB139036BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK036

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG092521.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
