
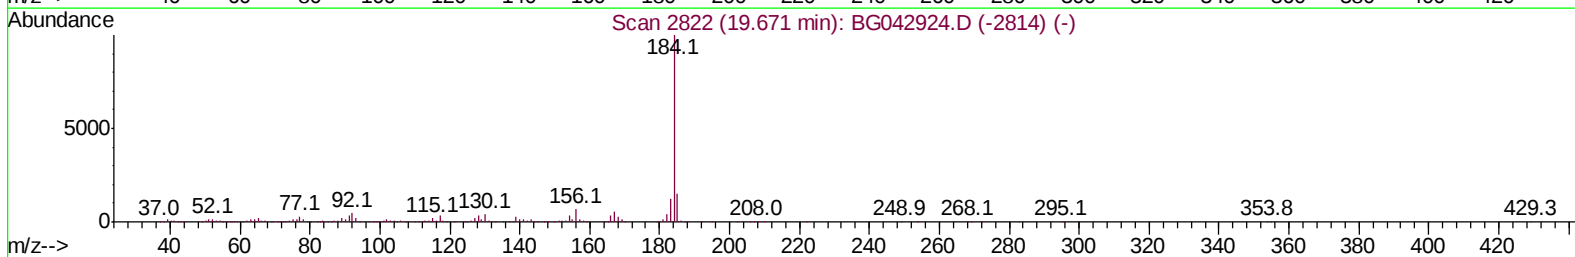
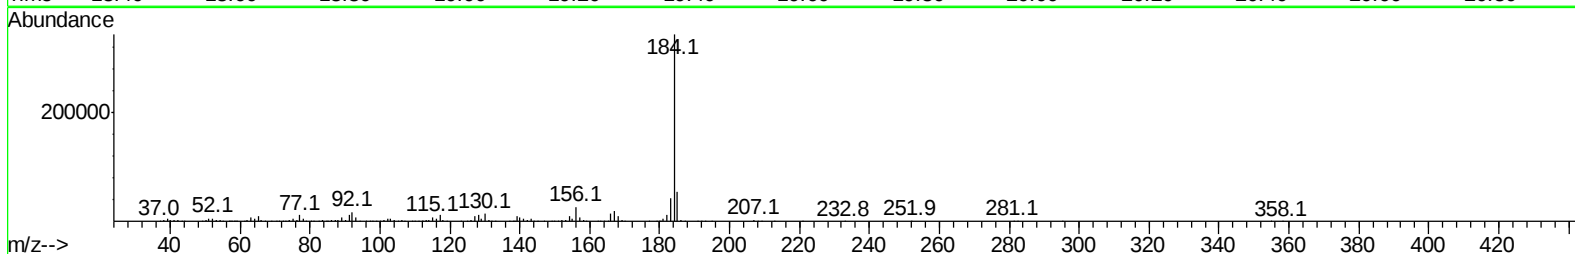


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100519\
Data File : BG043046.D
Acq On : 5 Oct 2019 9:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 09:27:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

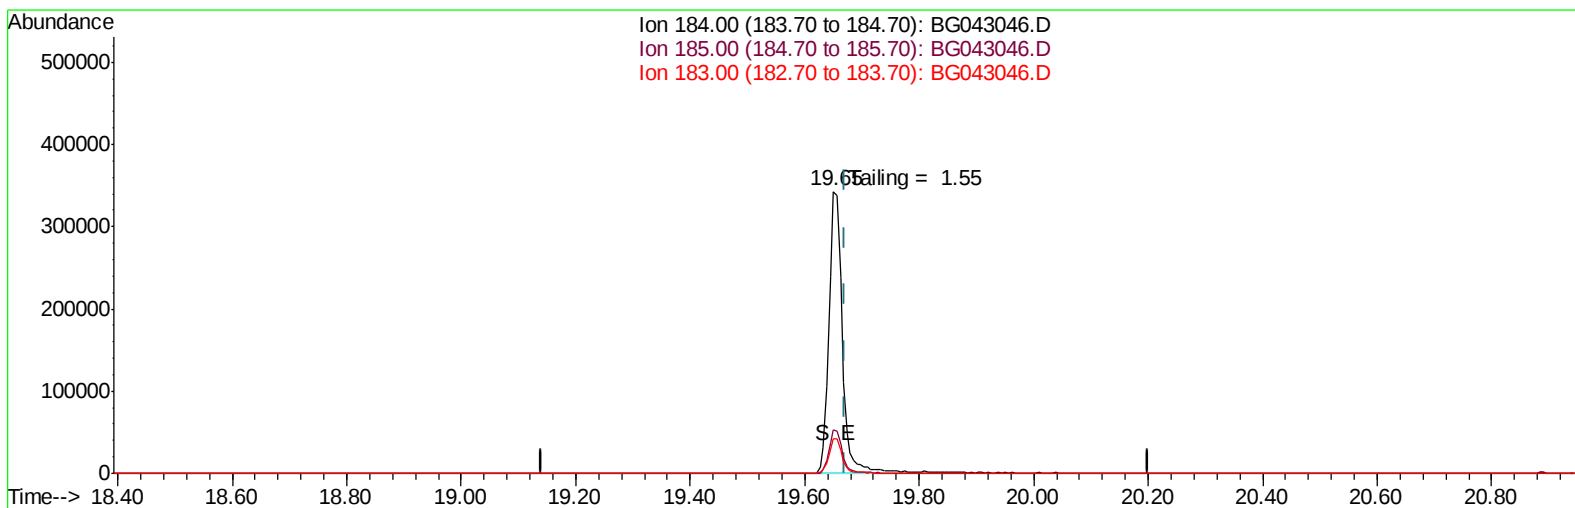

TIC: BG043046.D

(77) Benzidine




19.651min (-0.020) 21382.46ng

response 561094

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.61
183.00	12.60	12.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100519\
Data File : BG043046.D
Acq On : 5 Oct 2019 9:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 09:27:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

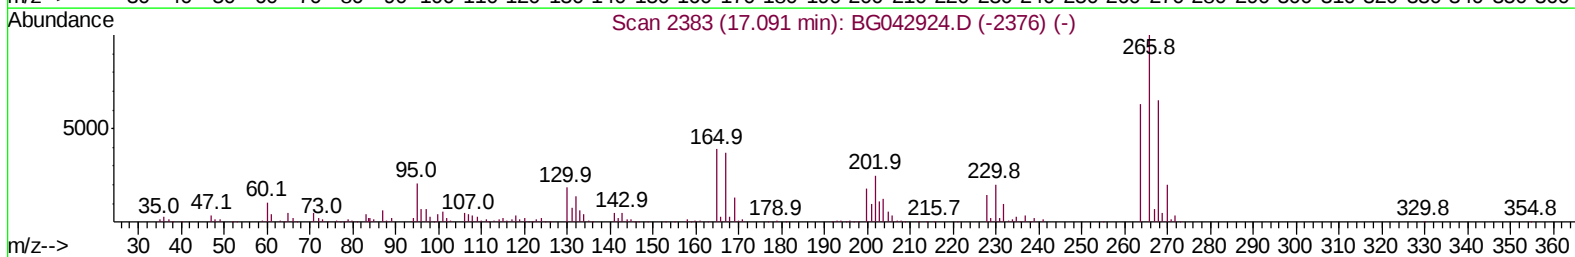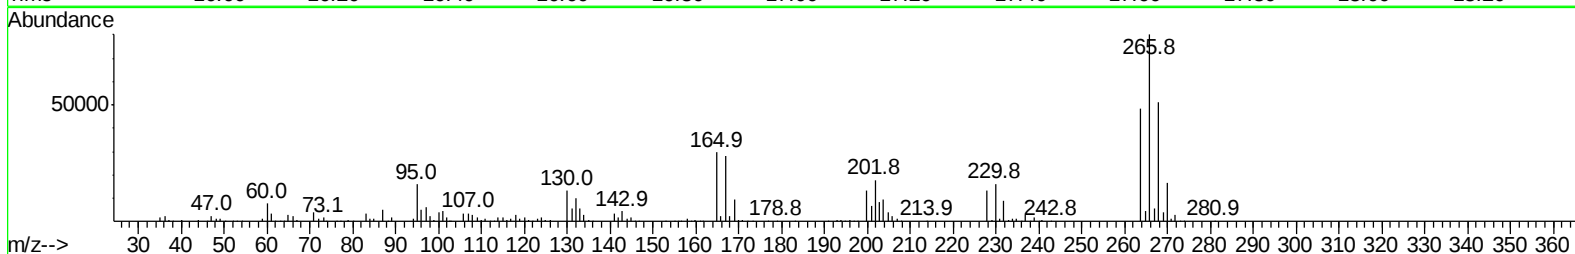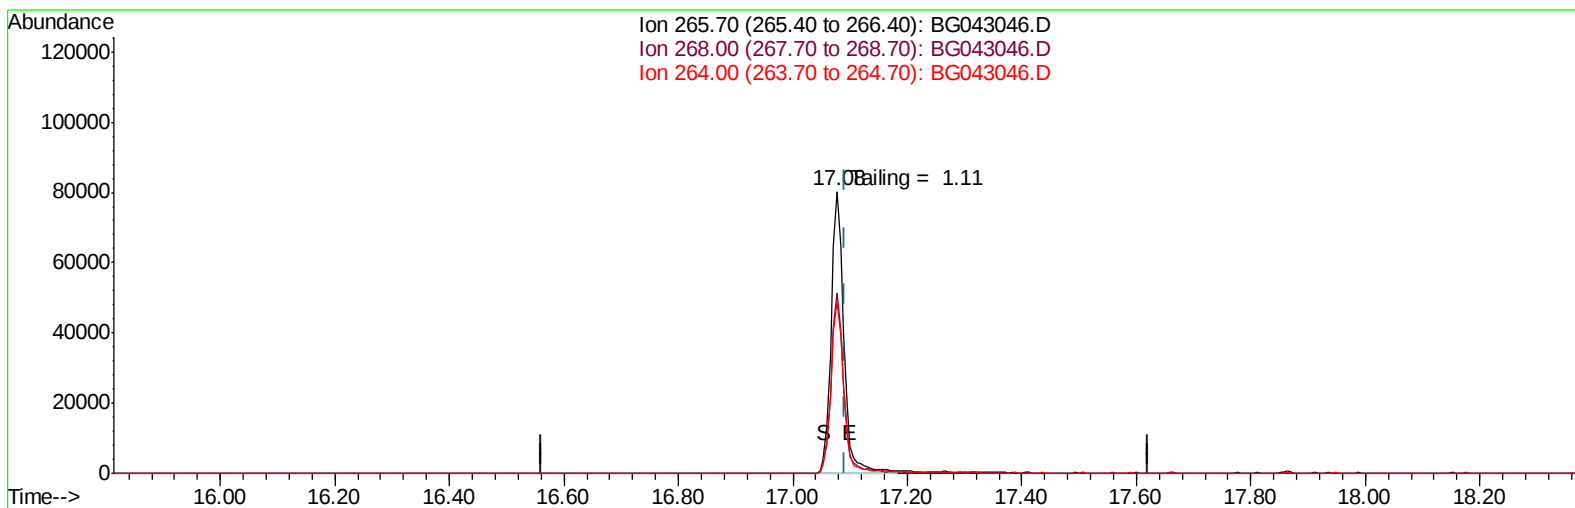

TIC: BG043046.D

(70) Pentachlorophenol (C)

17.077min (-0.014) 228795.55ng

response 121766

Ion	Exp%	Act%
265.70	100	100
268.00	65.20	63.92
264.00	63.40	60.70
0.00	0.00	0.00