

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100519\
 Data File : BG043050.D
 Acq On : 5 Oct 2019 11:43
 Operator : JU
 Sample : PB123594BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB123594BL

Quant Time: Oct 07 08:45:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 25 15:35:52 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	67690	20.00	ng	-0.01
21) Naphthalene-d8	10.86	136	249462	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	178153	20.00	ng	-0.01
64) Phenanthrene-d10	17.42	188	411983	20.00	ng	-0.01
76) Chrysene-d12	21.69	240	445799	20.00	ng	-0.03
87) Perylene-d12	24.90	264	514613	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	450169	118.69	ng	0.00
7) Phenol-d6	7.24	99	656777	120.24	ng	0.00
23) Nitrobenzene-d5	9.22	82	407977	79.49	ng	-0.01
42) 2,4,6-Tribromophenol	16.17	330	404748	132.12	ng	-0.01
45) 2-Fluorobiphenyl	13.30	172	1067371	86.86	ng	-0.02
79) Terphenyl-d14	20.03	244	2007863	95.97	ng	-0.01
Target Compounds						
50) Dimethylphthalate	14.13	163	71715	5.373	ng	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100519\
Data File : BG043050.D
Acq On : 5 Oct 2019 11:43
Operator : JU
Sample : PB123594BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB123594BL

Quant Time: Oct 07 08:45:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 25 15:35:52 2019
Response via : Initial Calibration

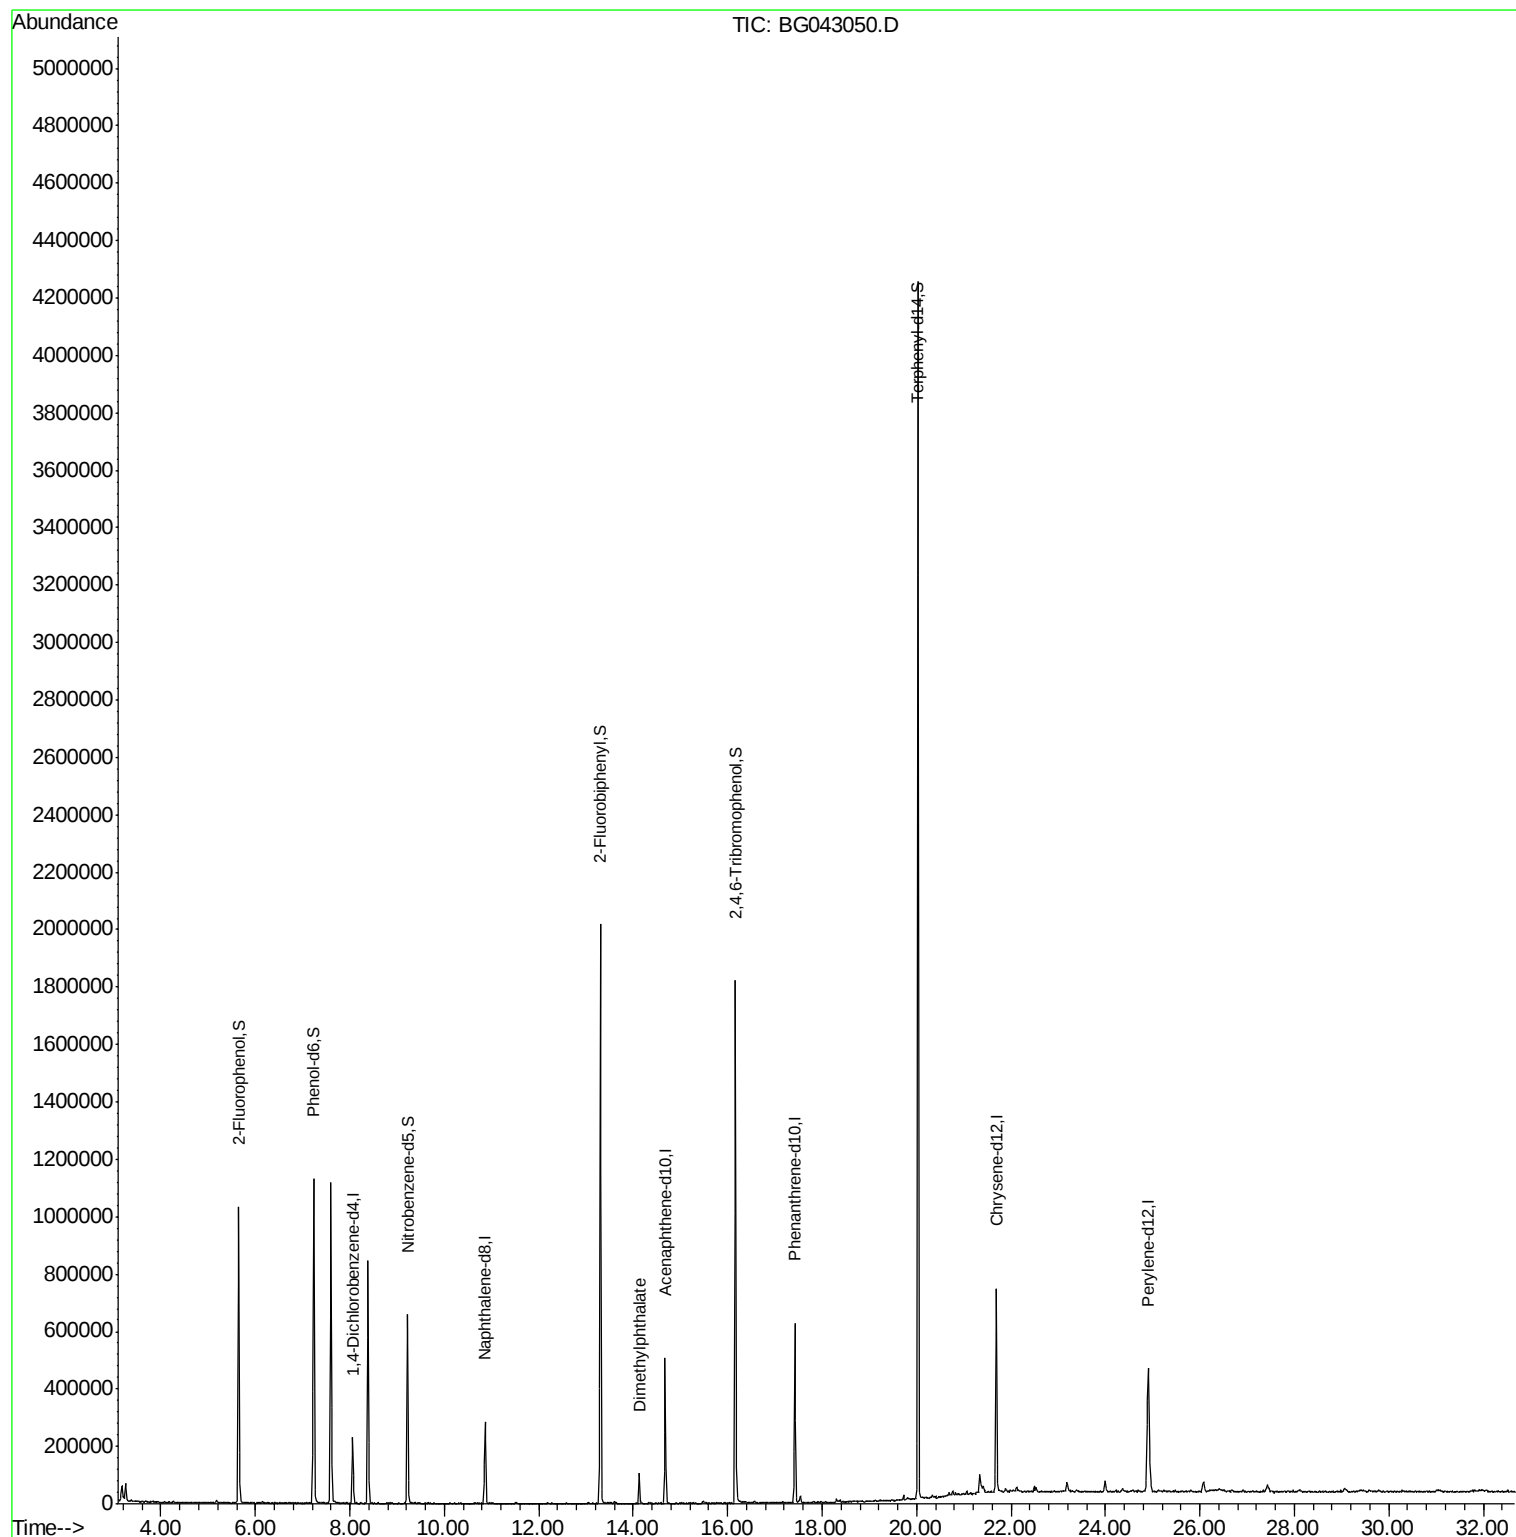

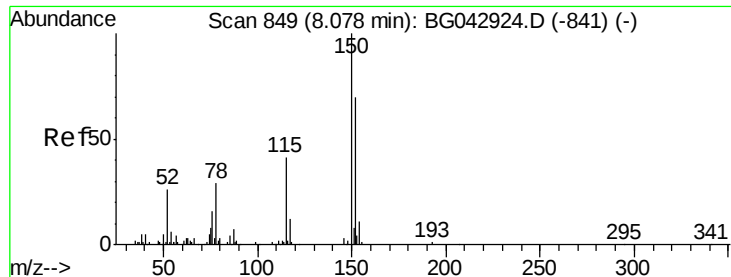


#1


1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.06 min Scan# 847
Delta R.T. -0.01 min
Lab File: BG043050.D
Acq: 5 Oct 2019 11:43

Instrument :
BNA_G
ClientSampleId :
PB123594BL



Tgt Ion	Ratio	Lower	Upper
152	100		
150	139.9	115.0	172.4
115	55.4	47.0	70.6

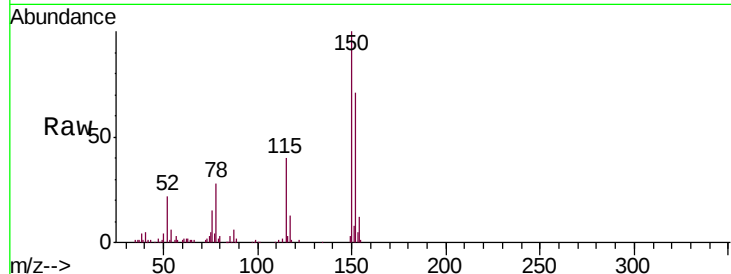

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

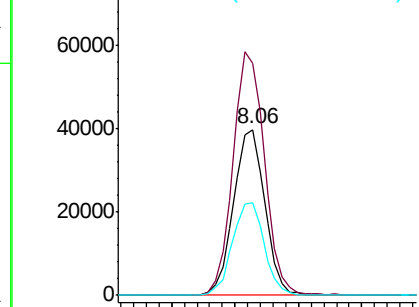


Time-->

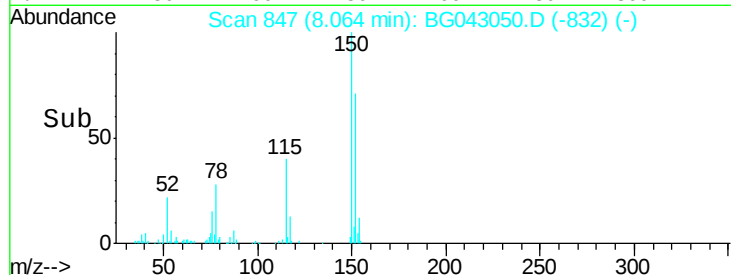


#5

2-Fluorophenol
Concen: 118.685 ng
RT: 5.65 min Scan# 436
Delta R.T. -0.01 min
Lab File: BG043050.D
Acq: 5 Oct 2019 11:43


Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.0	56.6	84.8
63	35.5	35.1	52.7




Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

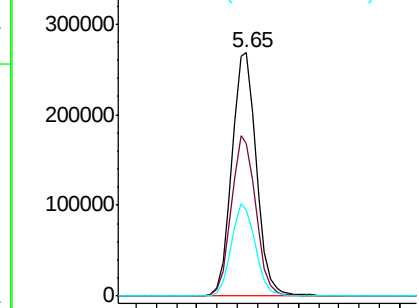

Time-->

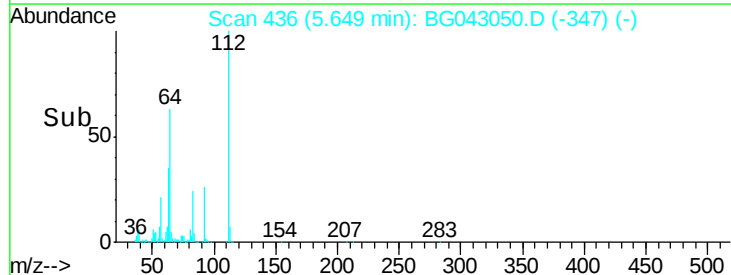

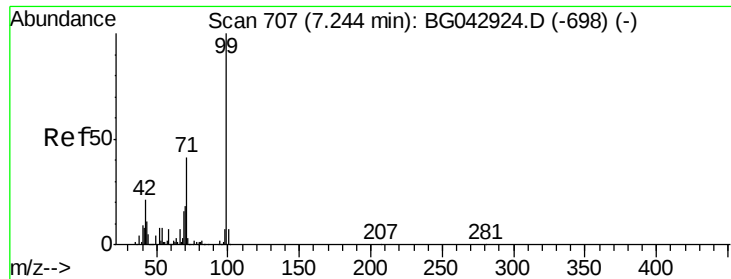

#7

Phenol-d6

Concen: 120.243 ng

RT: 7.24 min Scan# 706

Delta R.T. -0.01 min

Lab File: BG043050.D

Acq: 5 Oct 2019 11:43

Instrument :

BNA_G

ClientSampleId :

PB123594BL


Tgt Ion: 99 Resp: 656777

Ion Ratio Lower Upper




99 100

42 19.3 17.2 25.8

71 40.5 33.1 49.7



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

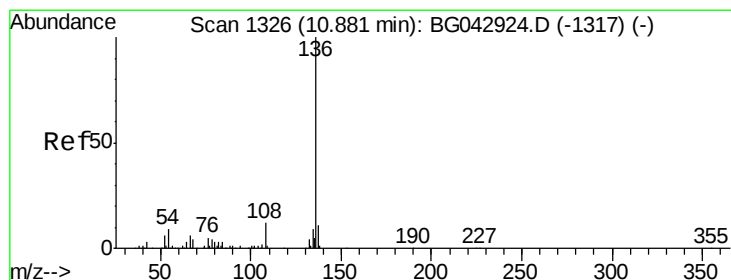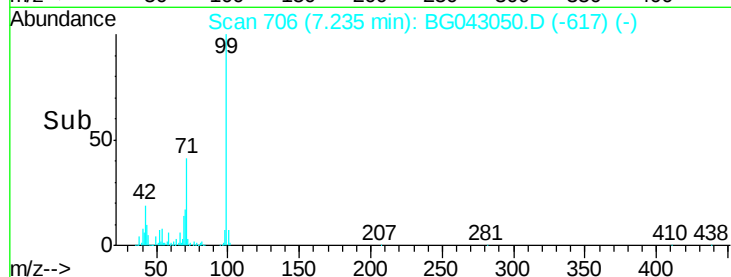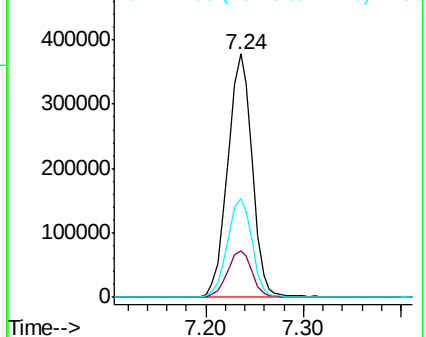

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.86 min Scan# 1323

Delta R.T. -0.02 min

Lab File: BG043050.D

Acq: 5 Oct 2019 11:43

Tgt Ion: 136 Resp: 249462


Ion Ratio Lower Upper

136 100



137 10.5 8.5 12.7


54 9.1 7.4 11.2

68 4.0 3.6 5.4



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



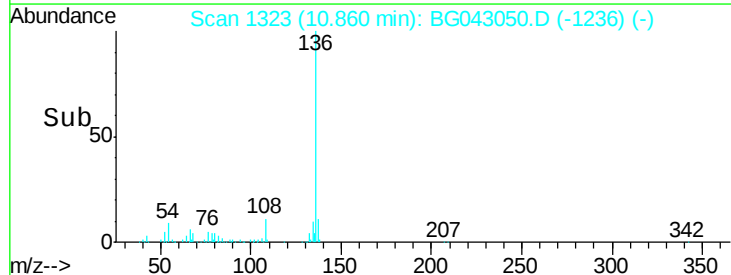
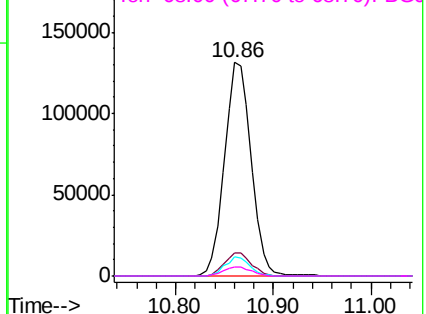


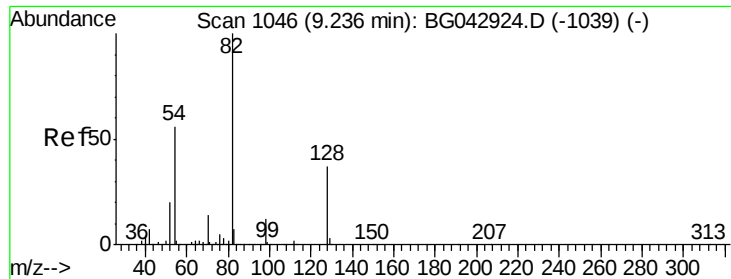

#23
 Nitrobenzene-d5
 Concen: 79.490 ng
 RT: 9.22 min Scan# 1044
 Delta R.T. -0.01 min
 Lab File: BG043050.D
 Acq: 5 Oct 2019 11:43




Instrument :
 BNA_G
 ClientSampleId :
 PB123594BL


Tgt Ion	Ratio	Lower	Upper
82	100		
128	40.5	29.5	44.3
54	53.5	44.6	67.0

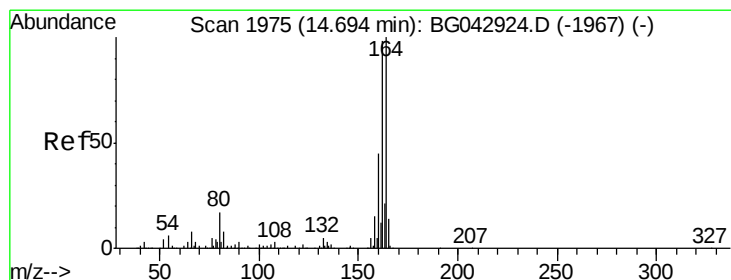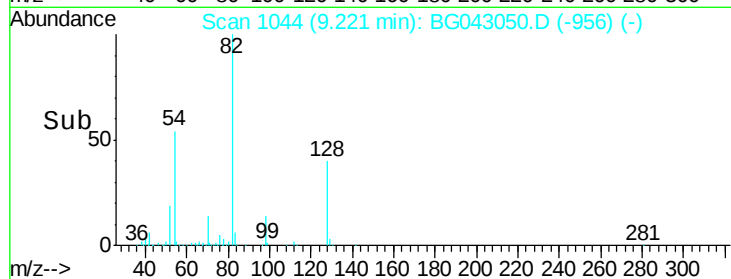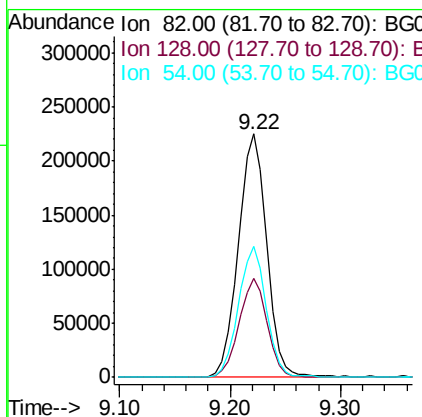

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.68 min Scan# 1973
 Delta R.T. -0.01 min
 Lab File: BG043050.D
 Acq: 5 Oct 2019 11:43

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.3	78.5	117.7
160	49.6	35.9	53.9

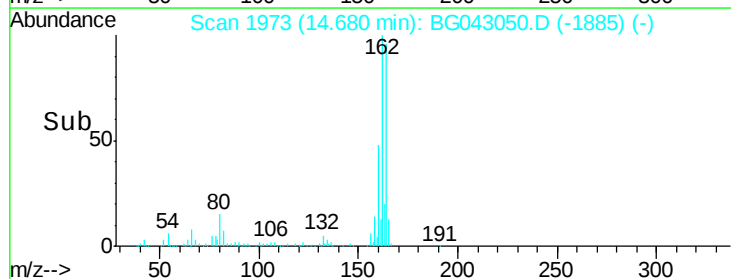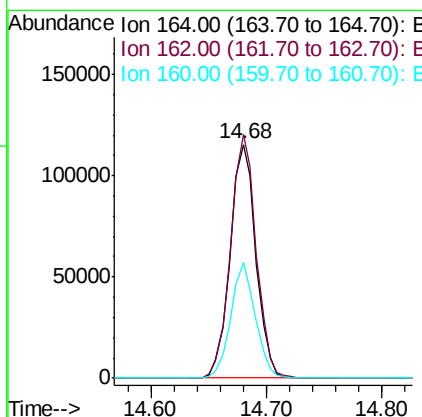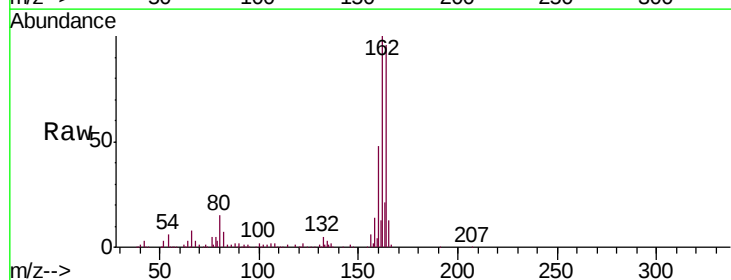


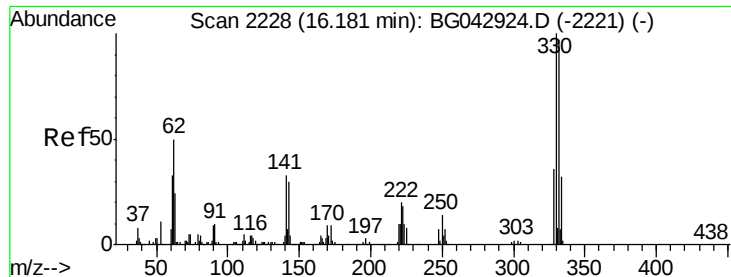




#42
 2,4,6-Tribromophenol
 Concen: 132.121 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.01 min
 Lab File: BG043050.D
 Acq: 5 Oct 2019 11:43

Instrument :
 BNA_G
 ClientSampleId :
 PB123594BL

Tgt Ion:330 Resp: 404748
 Ion Ratio Lower Upper
 330 100
 332 96.6 78.2 117.2
 141 29.5 26.0 39.0

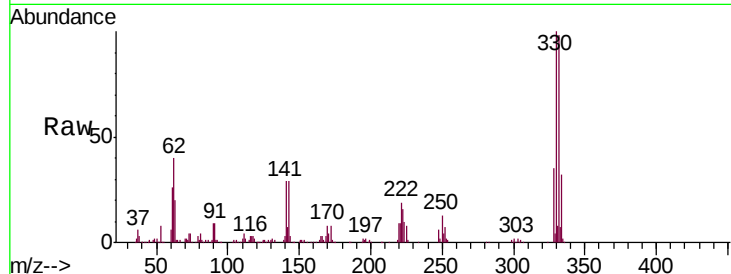


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

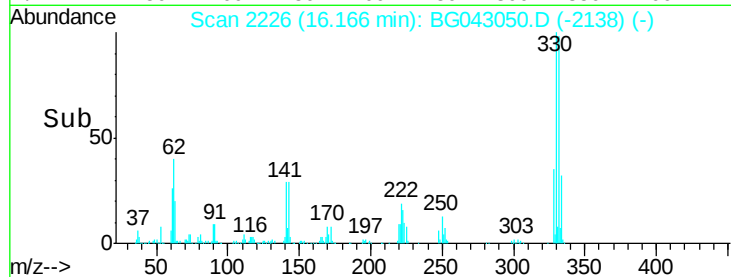
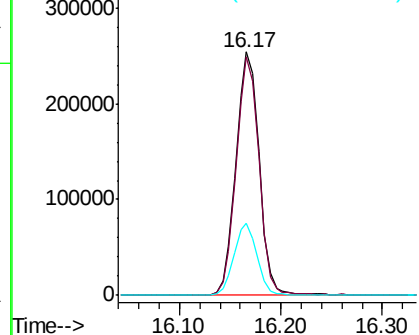



#45
 2-Fluorobiphenyl
 Concen: 86.856 ng
 RT: 13.30 min Scan# 1739
 Delta R.T. -0.02 min
 Lab File: BG043050.D
 Acq: 5 Oct 2019 11:43

Tgt Ion:172 Resp: 1067371
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.6 44.4
 170 24.5 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

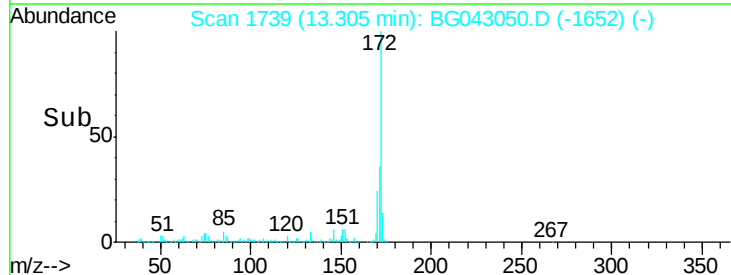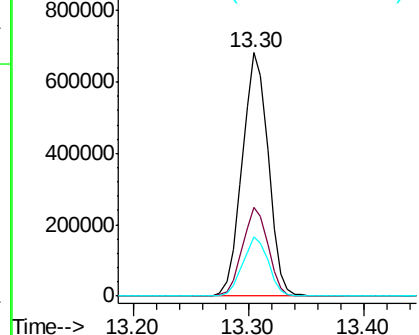

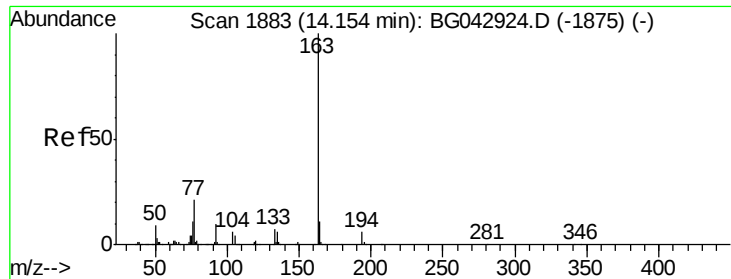

#50

Dimethylphthalate

Concen: 5.373 ng

RT: 14.13 min Scan# 1879

Delta R.T. -0.03 min

Lab File: BG043050.D

Acq: 5 Oct 2019 11:43

Instrument :

BNA_G

ClientSampleId :

PB123594BL


Tgt Ion:163 Resp: 71715

Ion Ratio Lower Upper

163 100

194 4.5 4.4 6.6




164 9.2 8.6 12.8

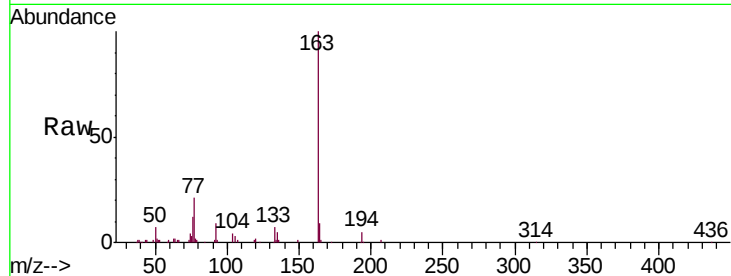

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

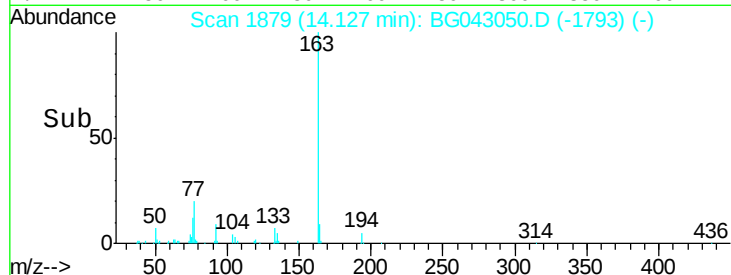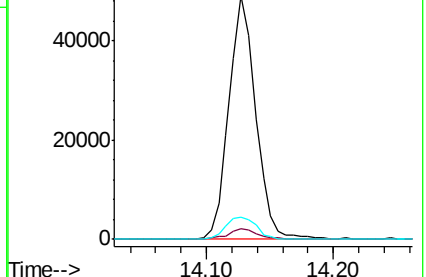

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.42 min Scan# 2440

Delta R.T. -0.01 min

Lab File: BG043050.D

Acq: 5 Oct 2019 11:43


Tgt Ion:188 Resp: 411983

Ion Ratio Lower Upper

188 100

94 6.2 5.7 8.5



80 6.3 6.5 9.7#




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC



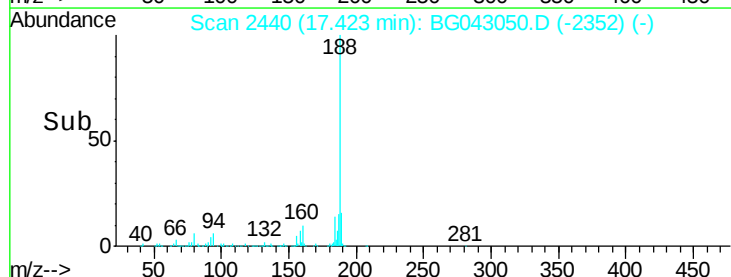
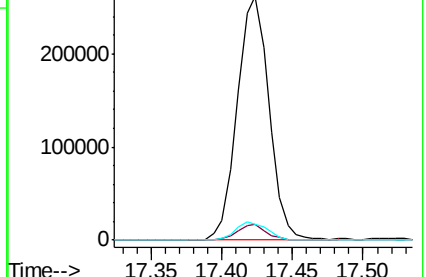


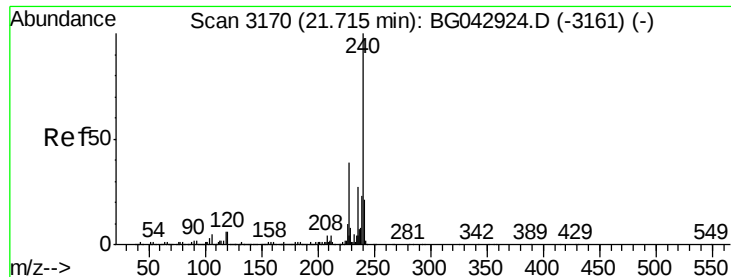

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.69 min Scan# 3166
Delta R.T. -0.03 min
Lab File: BG043050.D
Acq: 5 Oct 2019 11:43




Instrument :
BNA_G
ClientSampleId :
PB123594BL


Tgt Ion:240 Resp: 445799
Ion Ratio Lower Upper
240 100
120 5.9 4.8 7.2
236 27.1 21.4 32.0

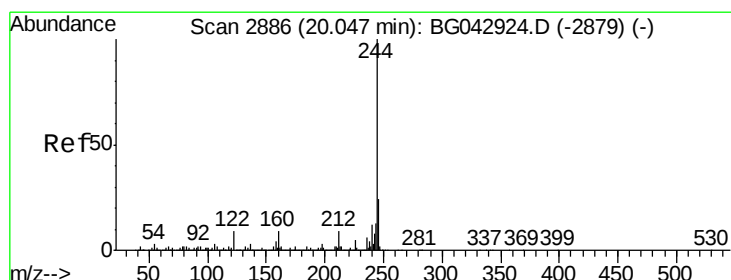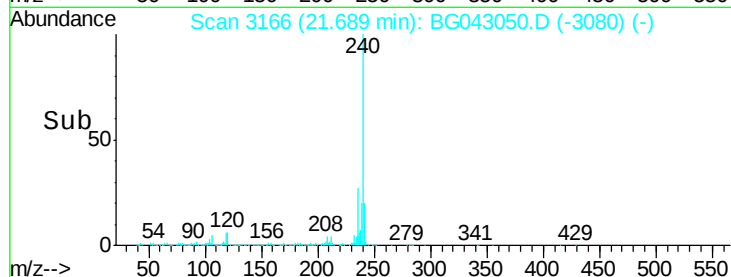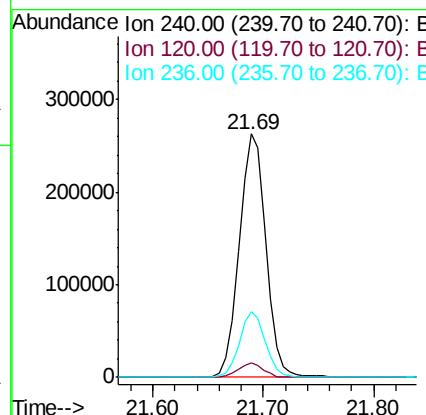

#79
Terphenyl-d14
Concen: 95.974 ng
RT: 20.03 min Scan# 2884
Delta R.T. -0.01 min
Lab File: BG043050.D
Acq: 5 Oct 2019 11:43

Tgt Ion:244 Resp: 2007863
Ion Ratio Lower Upper
244 100
212 8.6 7.4 11.0
122 8.0 7.0 10.4

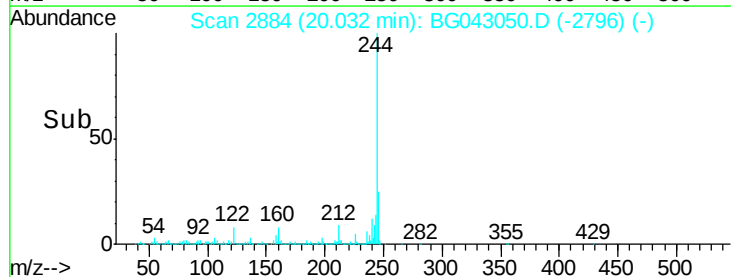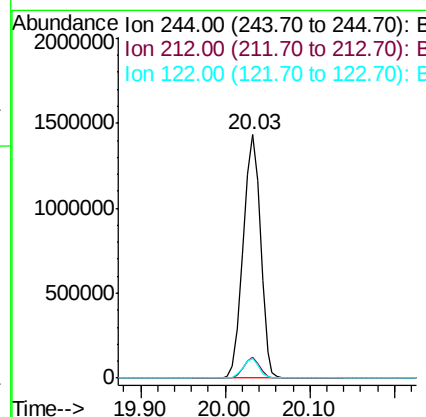

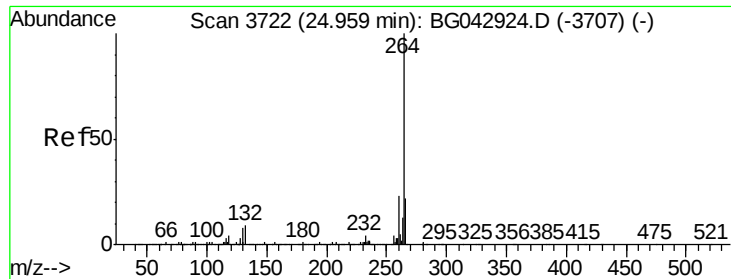

#87
Perylene-d12
Concen: 20.000 ng
RT: 24.90 min Scan# 3713
Delta R.T. -0.06 min
Lab File: BG043050.D
Acq: 5 Oct 2019 11:43

Instrument :
BNA_G
ClientSampleId :
PB123594BL

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.2	18.7	28.1
265	22.3	17.7	26.5

