


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100519\
 Data File : BG043046.D
 Acq On : 5 Oct 2019 9:09
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

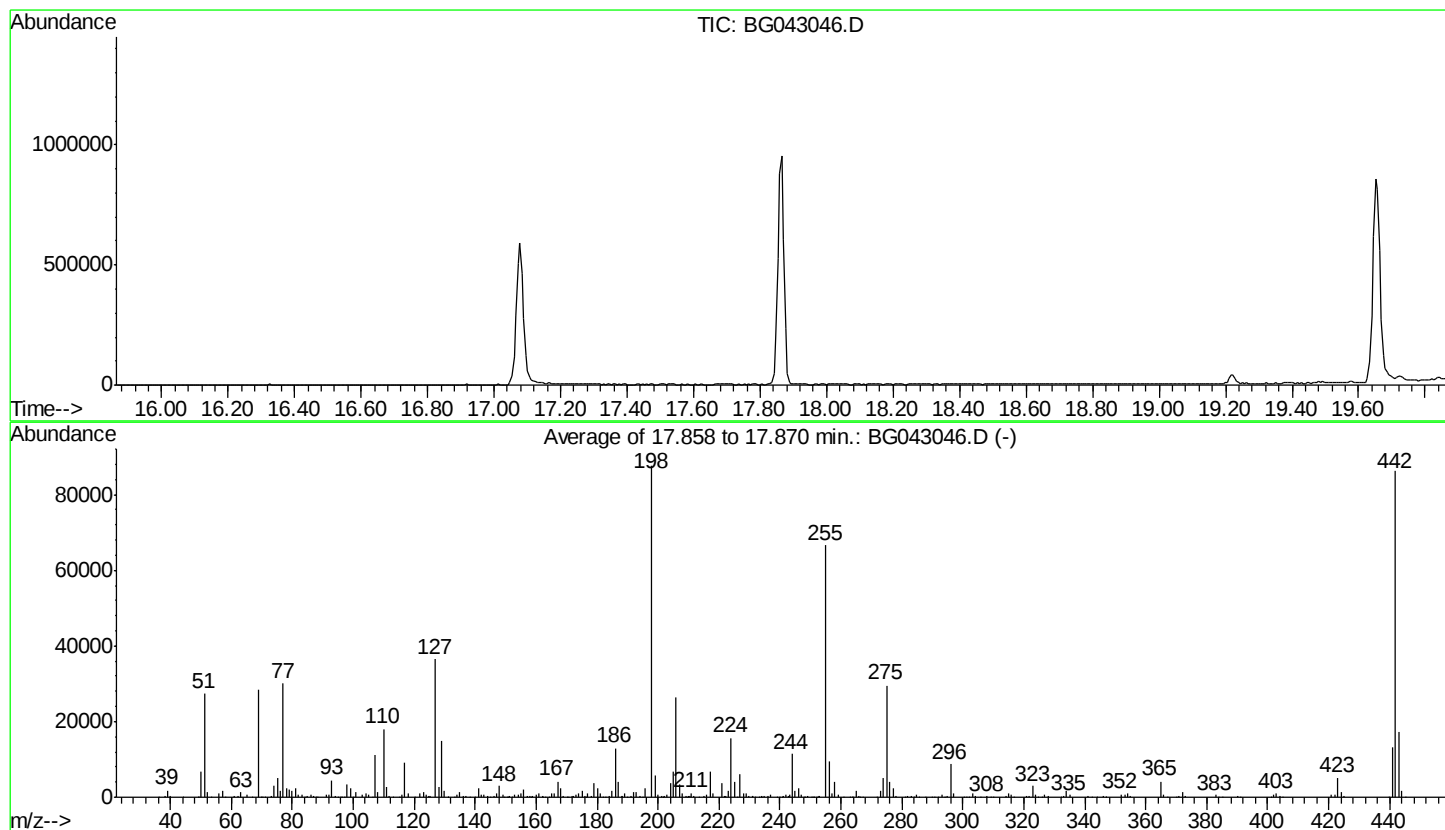

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	27328	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.3	28304	PASS
70	69	0.00	2	0.3	95	PASS
127	198	10	80	41.6	36424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87648	PASS
199	198	5	9	6.7	5911	PASS
275	198	10	60	33.7	29581	PASS
365	198	1	100	4.7	4129	PASS
441	198	0.01	100	15.1	13232	PASS
442	198	50	100	98.6	86378	PASS
443	442	15	24	20.1	17324	PASS