
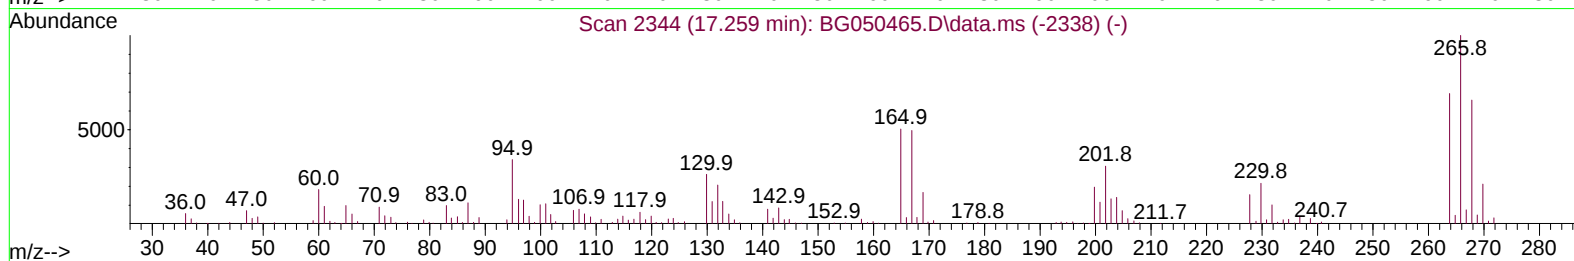
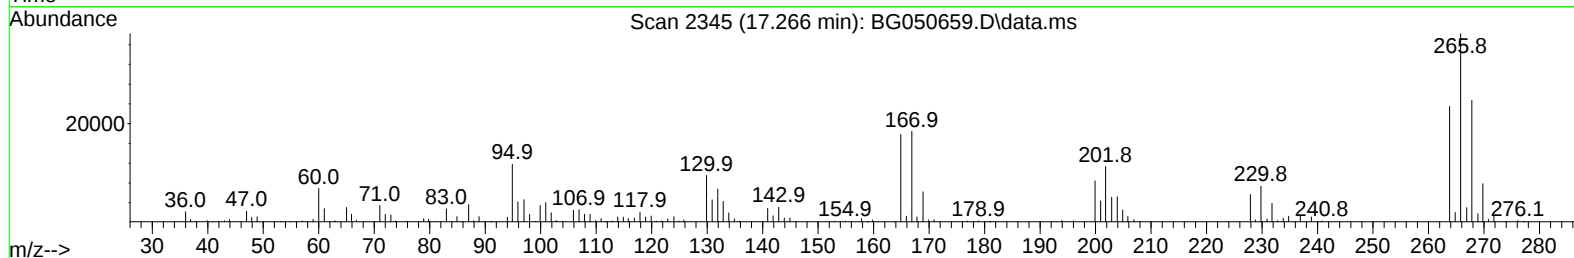


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050659.D
Acq On : 21 Oct 2021 8:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 11:08:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

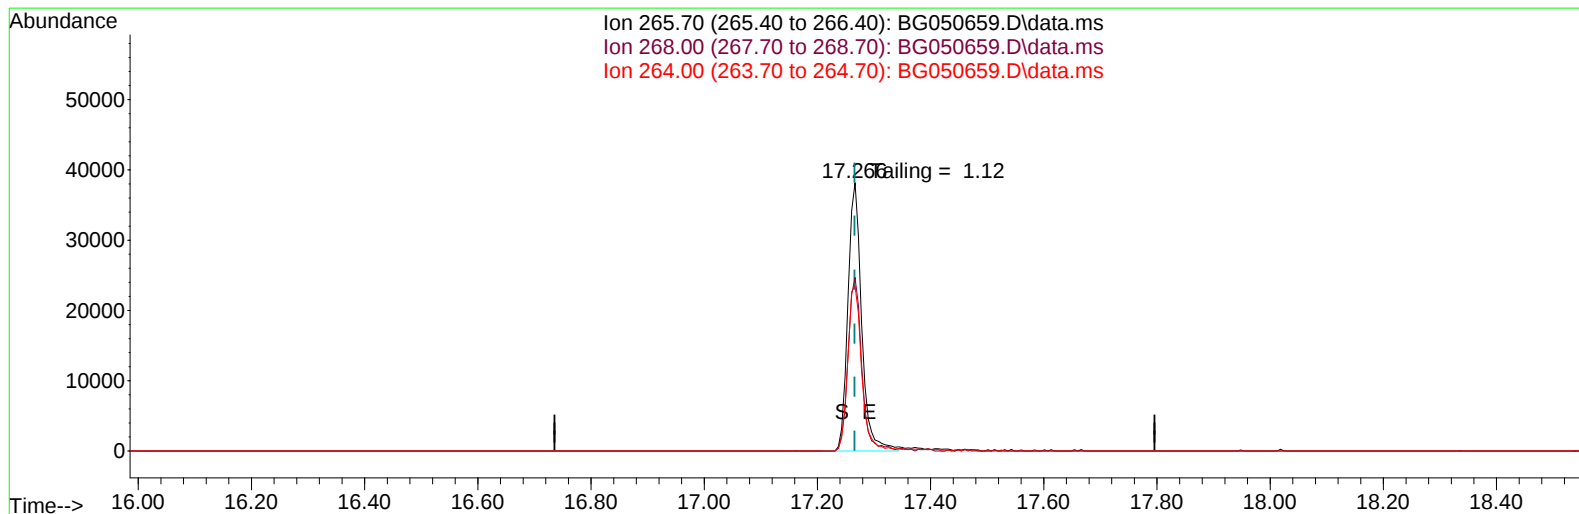

TIC: BG050659.D\data.ms

(70) Pentachlorophenol (C)




17.266min (+ 0.001) 20845.71 ng

response 64950

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.62
264.00	61.30	61.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
 Data File : BG050659.D
 Acq On : 21 Oct 2021 8:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 11:08:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 10:56:22 2021
 Response via : Initial Calibration

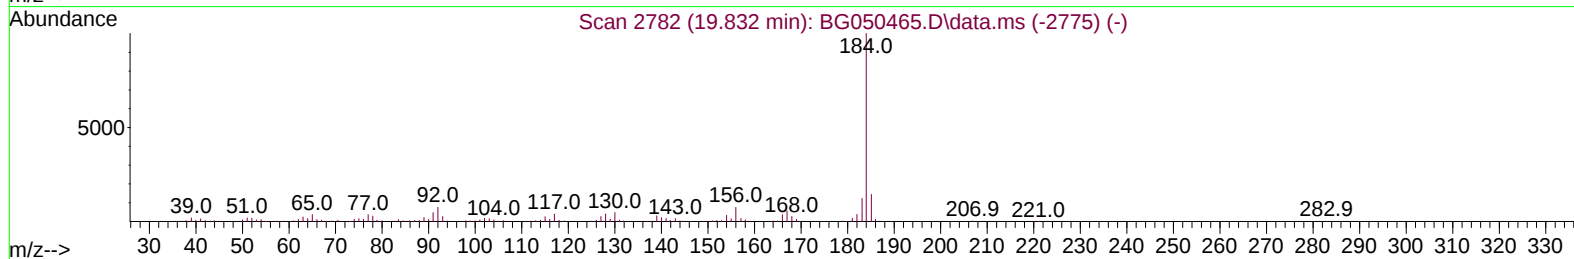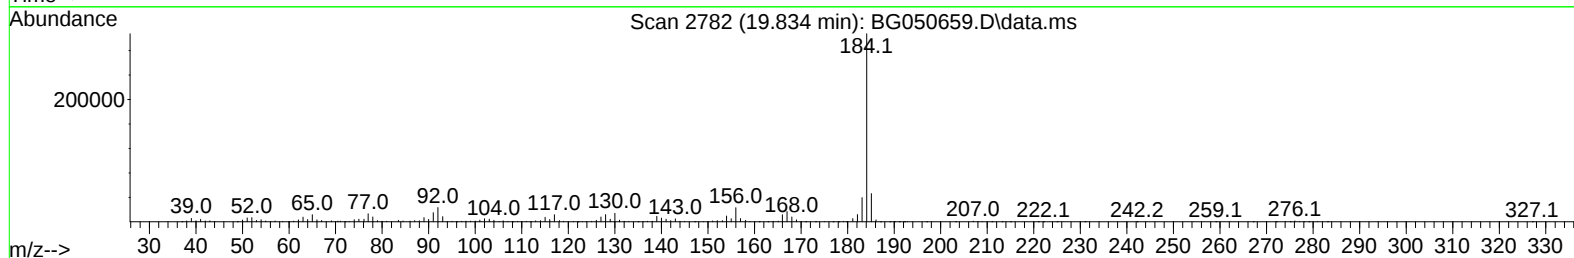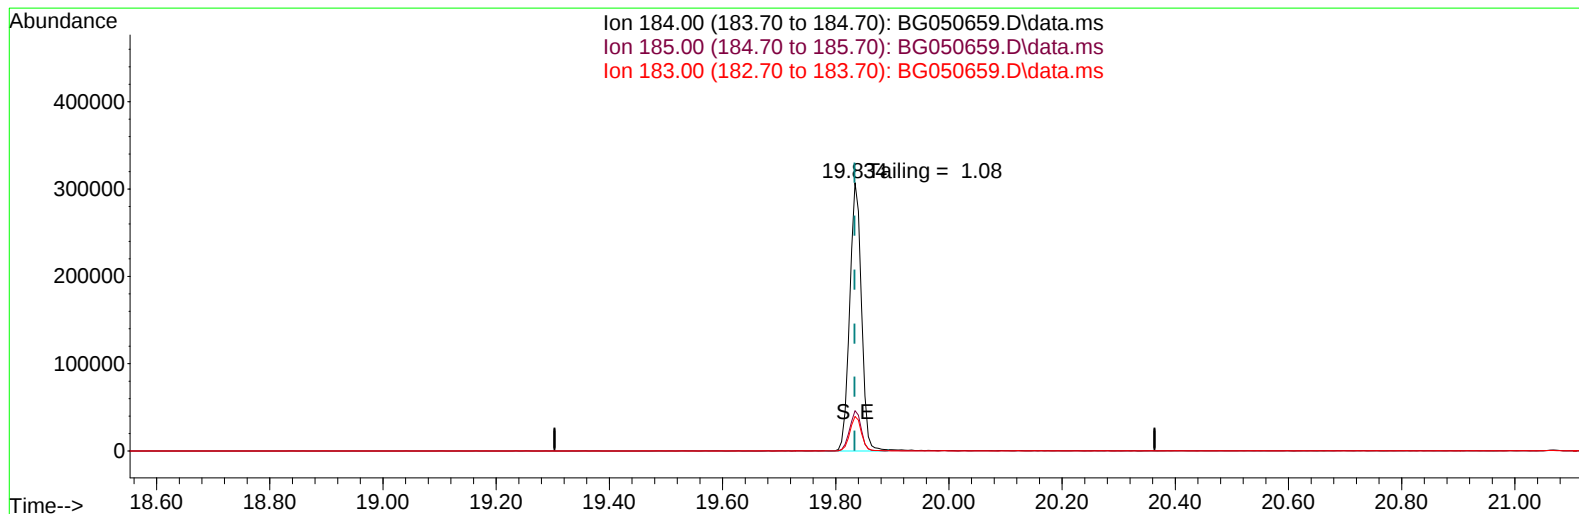

TIC: BG050659.D\data.ms

(77) Benzidine**19.834min (+ 0.001) 241720.81 ng****response 446564**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.02
183.00	11.70	12.88
0.00	0.00	0.00