

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
 Data File : BG050661.D
 Acq On : 21 Oct 2021 10:21
 Operator : CG/JU
 Sample : PB140015BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB140015BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.790	385	392	405	rBV	861415	1414167	49.39%	10.662%
2	7.400	657	666	677	rBV	837998	1512678	52.83%	11.405%
3	8.252	804	811	818	rVB	142007	251861	8.80%	1.899%
4	9.427	1002	1011	1021	rBV	529998	954498	33.34%	7.197%
5	11.078	1284	1292	1300	rBV	208404	374354	13.07%	2.822%
6	13.499	1697	1704	1711	rBV	1281540	2028437	70.85%	15.294%
7	14.874	1931	1938	1948	rVB	342307	533073	18.62%	4.019%
8	16.360	2183	2191	2205	rBV	955948	1485760	51.89%	11.202%
9	17.617	2398	2405	2413	rBV	426366	656933	22.94%	4.953%
10	20.209	2839	2846	2853	rBV	2146698	2863132	100.00%	21.587%
11	21.918	3131	3137	3147	rVB2	327634	573830	20.04%	4.326%
12	25.338	3710	3719	3733	rVB2	200781	614523	21.46%	4.633%




Sum of corrected areas: 13263246

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050661.D
Acq On : 21 Oct 2021 10:21
Operator : CG/JU
Sample : PB140015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

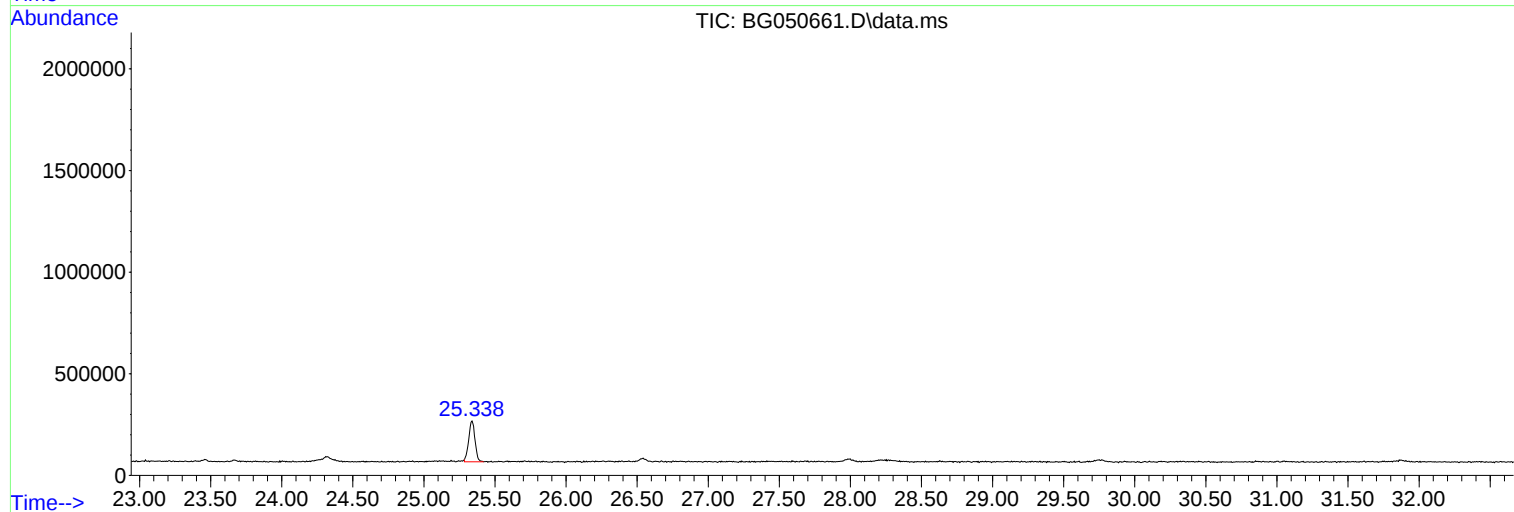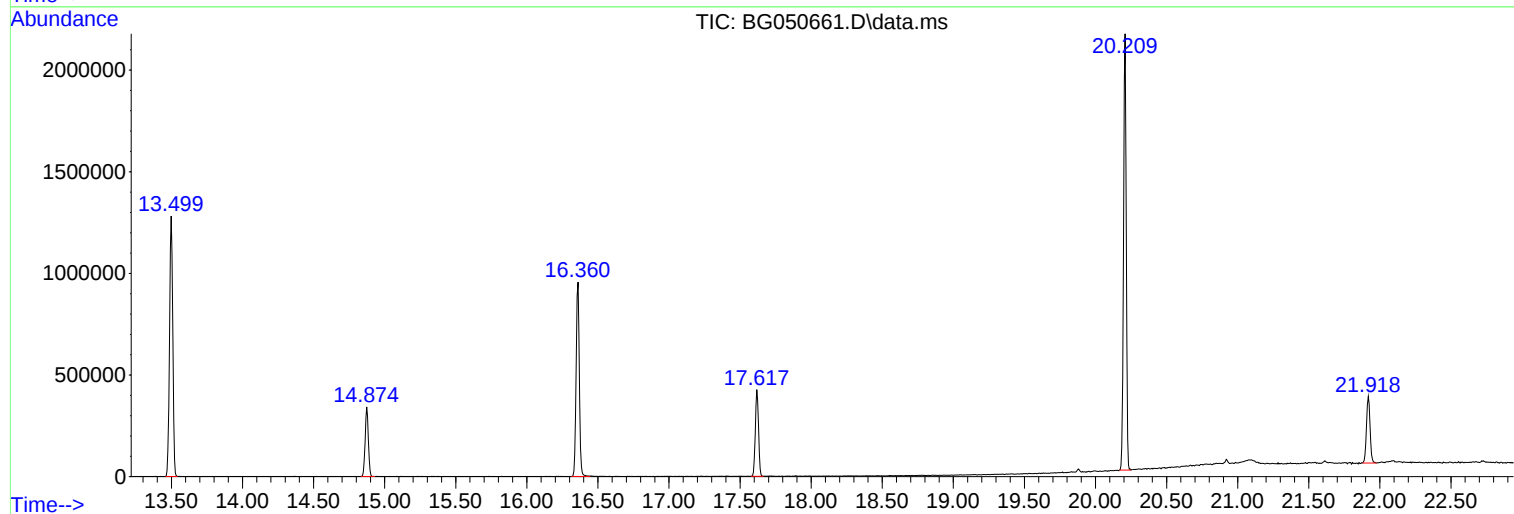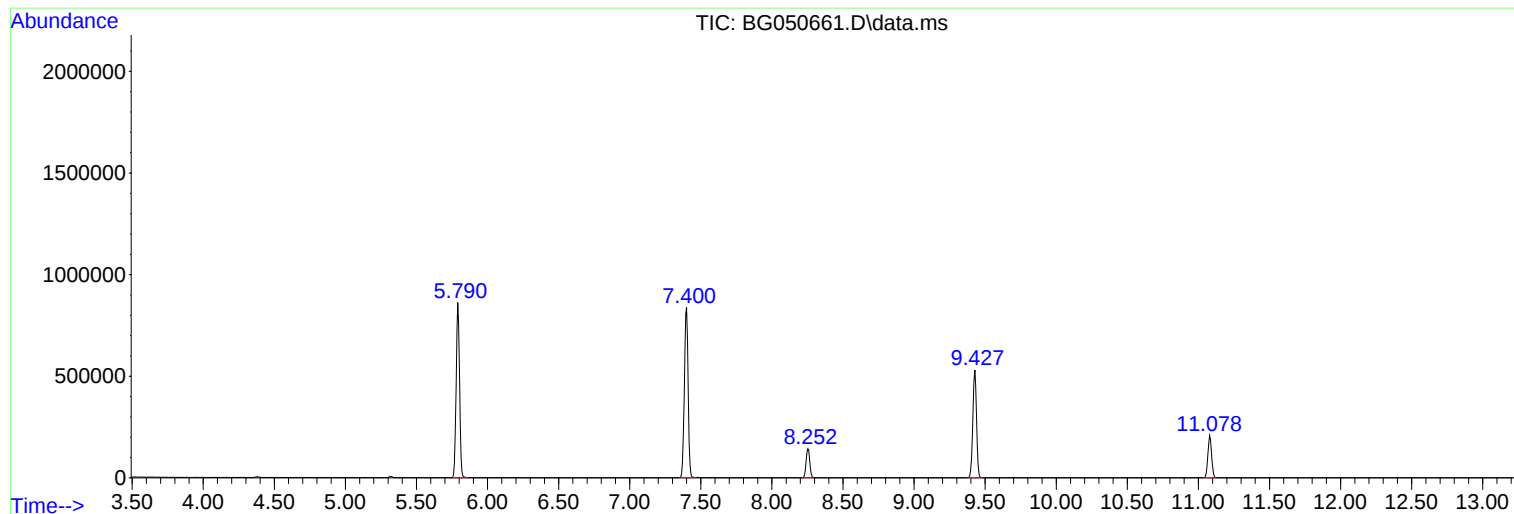

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050661.D
Acq On : 21 Oct 2021 10:21
Operator : CG/JU
Sample : PB140015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050661.D
Acq On : 21 Oct 2021 10:21
Operator : CG/JU
Sample : PB140015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------