

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102121\  
 Data File : BG050669.D  
 Acq On : 21 Oct 2021 15:50  
 Operator : CG/JU  
 Sample : PB140074BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB140074BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050669.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.792       | 381           | 392         | 404          | rBV      | 838427         | 1386391       | 47.68%          | 10.577%       |
| 2         | 7.396       | 656           | 665         | 678          | rBV      | 829424         | 1487752       | 51.16%          | 11.350%       |
| 3         | 8.254       | 803           | 811         | 820          | rVB      | 141056         | 248851        | 8.56%           | 1.898%        |
| 4         | 9.423       | 1002          | 1010        | 1019         | rBV      | 505599         | 941238        | 32.37%          | 7.181%        |
| 5         | 11.074      | 1283          | 1291        | 1302         | rVB      | 192526         | 362518        | 12.47%          | 2.766%        |
| 6         | 13.495      | 1693          | 1703        | 1711         | rBV      | 1226533        | 1965306       | 67.58%          | 14.993%       |
| 7         | 14.870      | 1931          | 1937        | 1946         | rVB      | 324034         | 517904        | 17.81%          | 3.951%        |
| 8         | 16.356      | 2183          | 2190        | 2203         | rBV      | 909003         | 1429361       | 49.15%          | 10.904%       |
| 9         | 17.614      | 2398          | 2404        | 2412         | rBV      | 402080         | 643621        | 22.13%          | 4.910%        |
| 10        | 20.205      | 2839          | 2845        | 2851         | rBV      | 2201947        | 2907973       | 100.00%         | 22.184%       |
| 11        | 21.914      | 3130          | 3136        | 3144         | rVB2     | 333724         | 593819        | 20.42%          | 4.530%        |
| 12        | 25.334      | 3708          | 3718        | 3733         | rVB3     | 199903         | 623453        | 21.44%          | 4.756%        |




Sum of corrected areas: 13108187

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102121\  
Data File : BG050669.D  
Acq On : 21 Oct 2021 15:50  
Operator : CG/JU  
Sample : PB140074BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140074BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

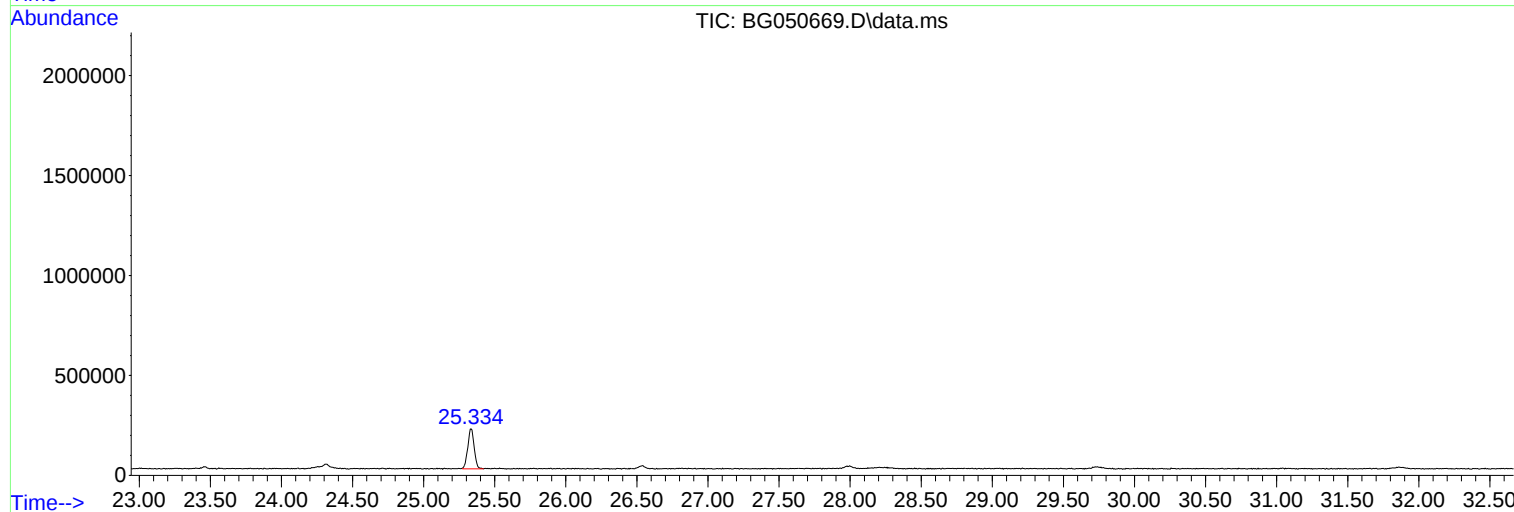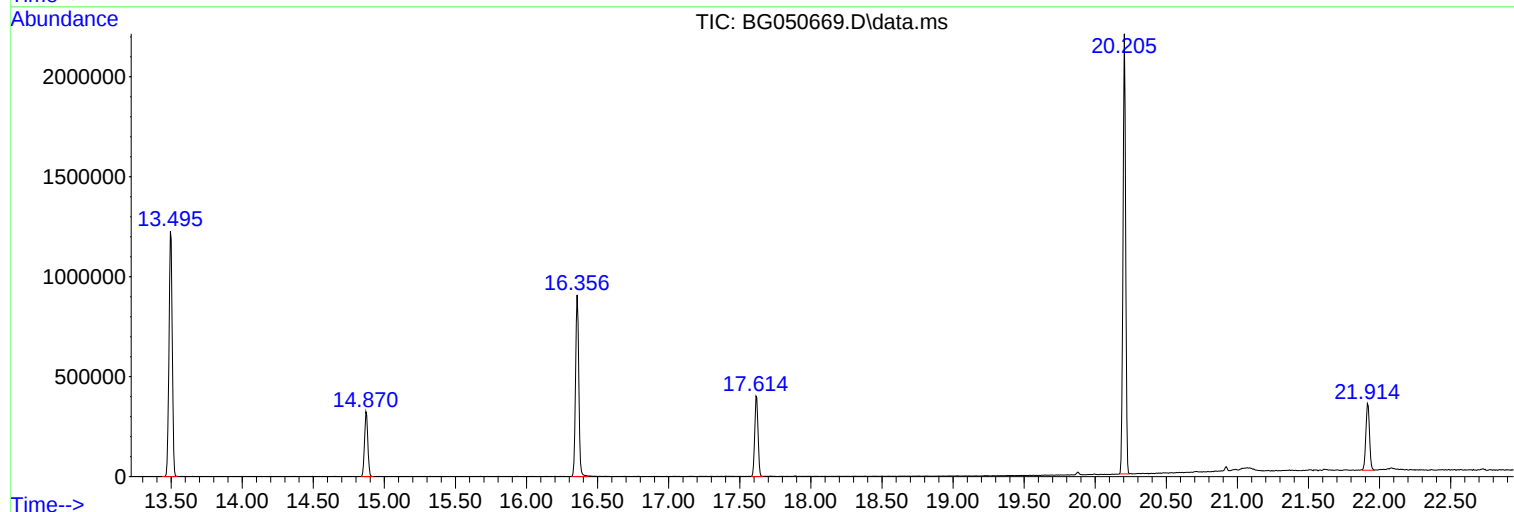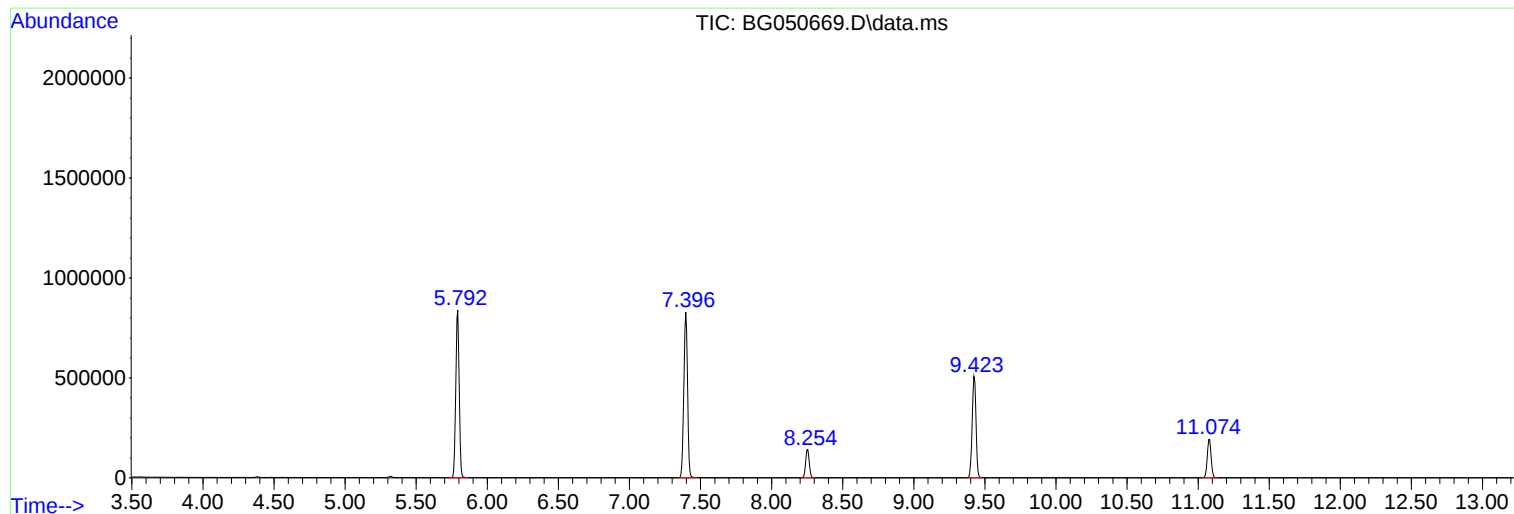

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102121\  
Data File : BG050669.D  
Acq On : 21 Oct 2021 15:50  
Operator : CG/JU  
Sample : PB140074BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140074BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG102121\  
Data File : BG050669.D  
Acq On : 21 Oct 2021 15:50  
Operator : CG/JU  
Sample : PB140074BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB140074BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|