


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
 Data File : BG050659.D
 Acq On : 21 Oct 2021 8:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

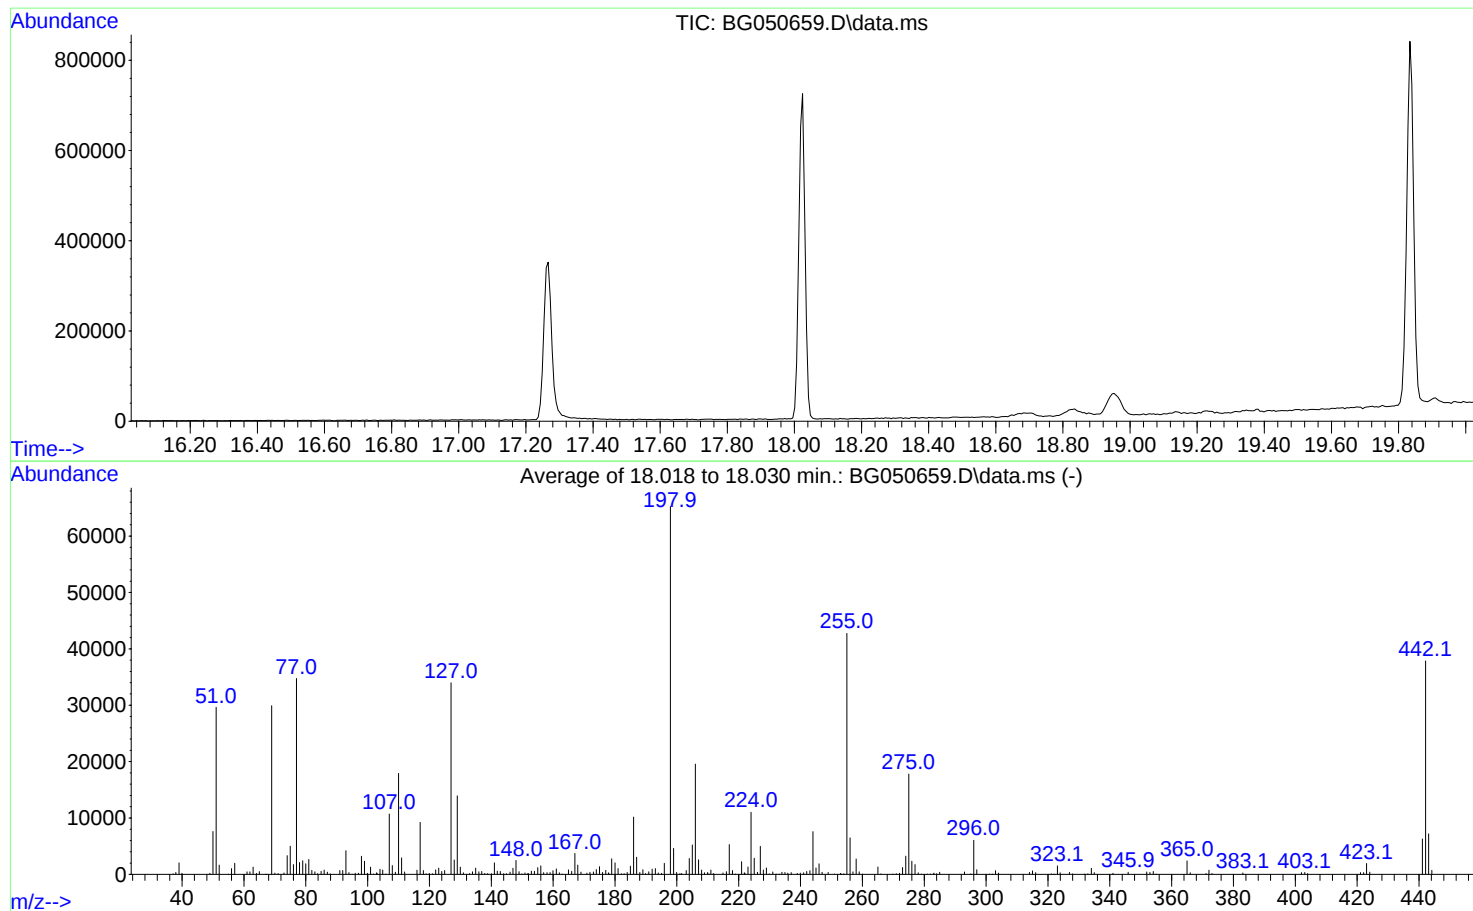




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	29627	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	29911	PASS
70	69	0.00	2	0.8	231	PASS
127	198	10	80	52.1	33981	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65248	PASS
199	198	5	9	7.0	4598	PASS
275	198	10	60	27.3	17811	PASS
365	198	1	100	3.6	2374	PASS
441	198	0.01	100	9.6	6273	PASS
442	442	50	100	100.0	37856	PASS
443	442	15	24	19.0	7181	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050659.D
Acq On : 21 Oct 2021 8:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 21 11:08:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

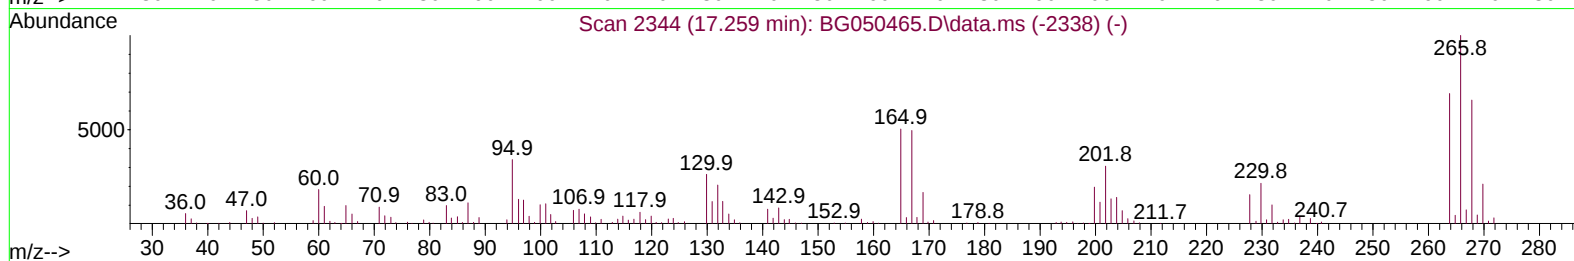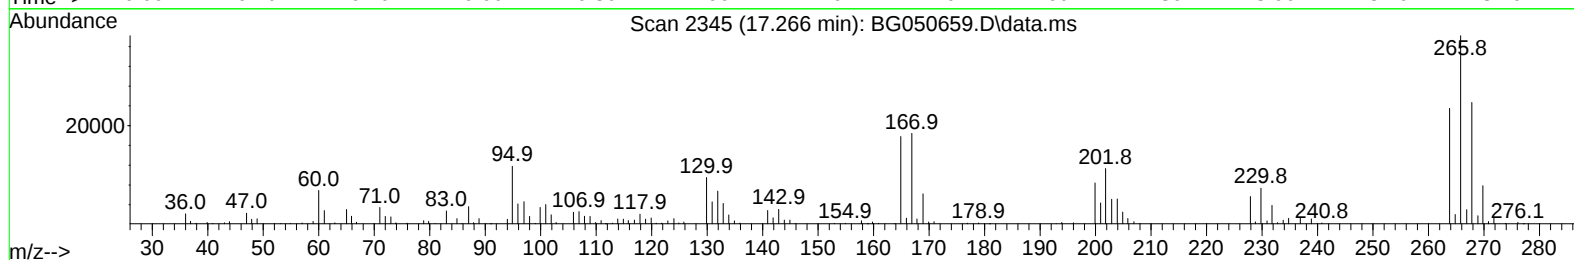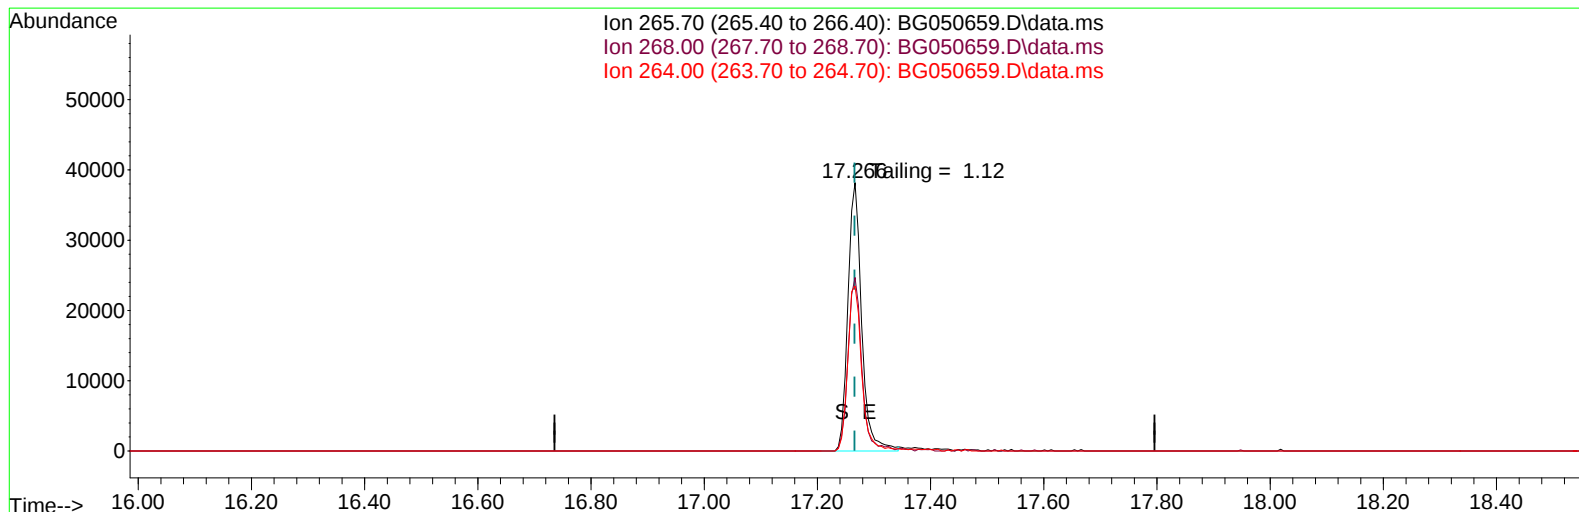

TIC: BG050659.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.001) 20845.71 ng




response 64950

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.62
264.00	61.30	61.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102121\
Data File : BG050659.D
Acq On : 21 Oct 2021 8:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 21 11:08:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

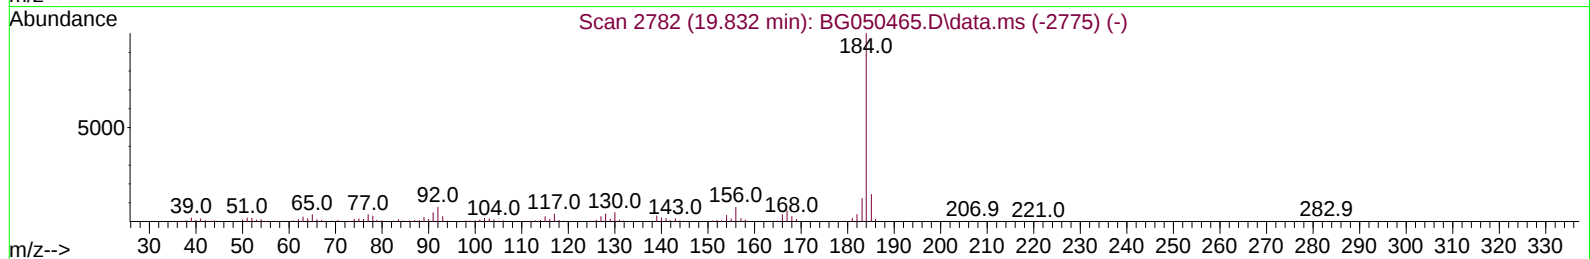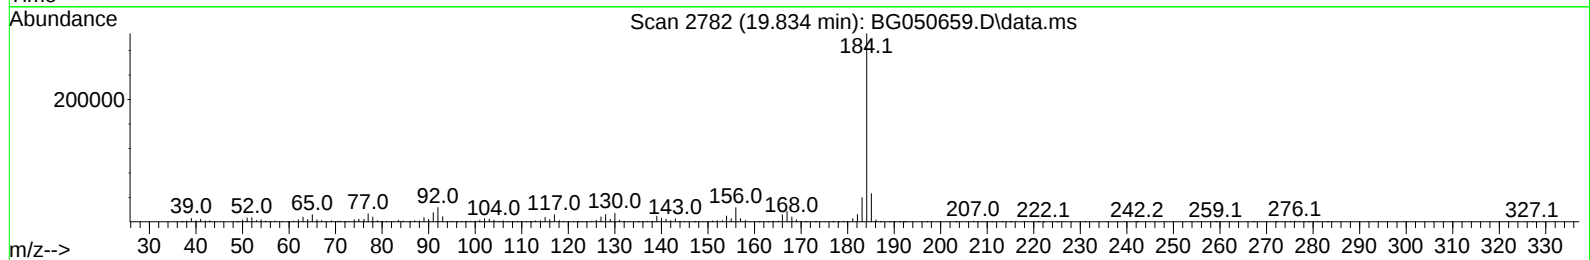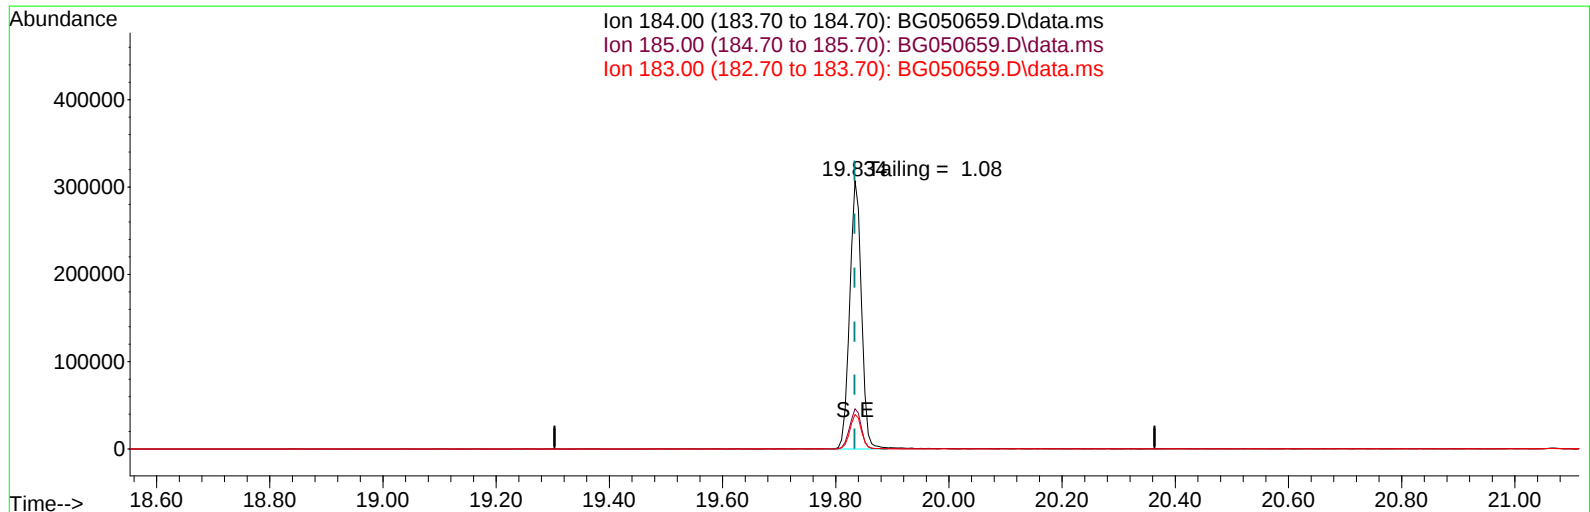

TIC: BG050659.D\data.ms

(77) Benzidine

19.834min (+ 0.001) 241720.81 ng

response 446564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.02
183.00	11.70	12.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/21/2021	BNA_G	BG050659.D
Compound Name	Response	Retention Time
DDT	190697	21.06
DDD	5879	20.61
DDE	901	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6780	197477	3.43

Instrument :
BNA_G
ClientSampleId :
DFTPP