
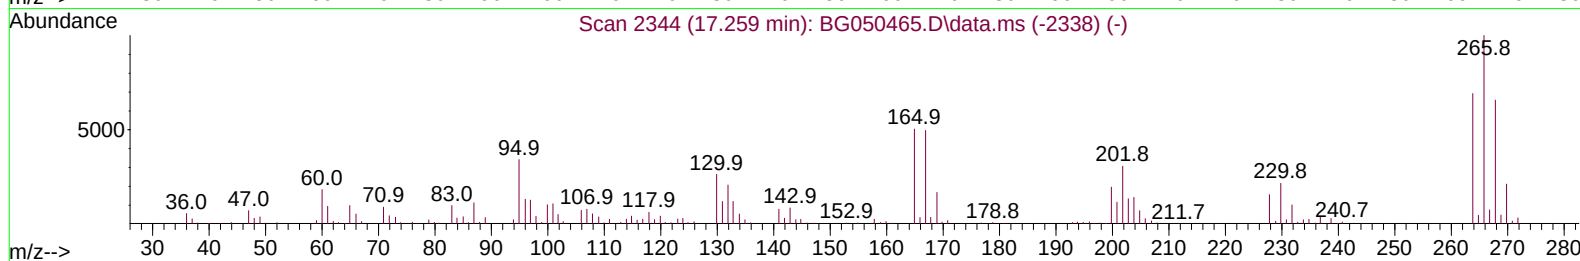
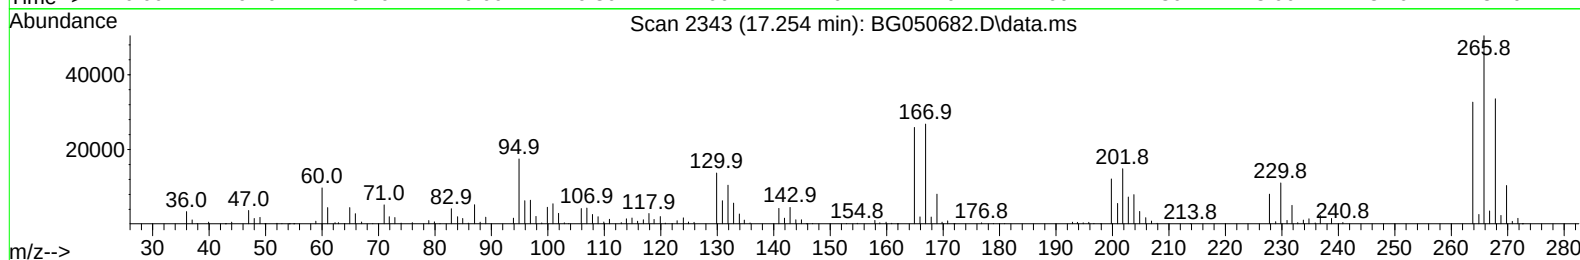


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050682.D
Acq On : 22 Oct 2021 9:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:55:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

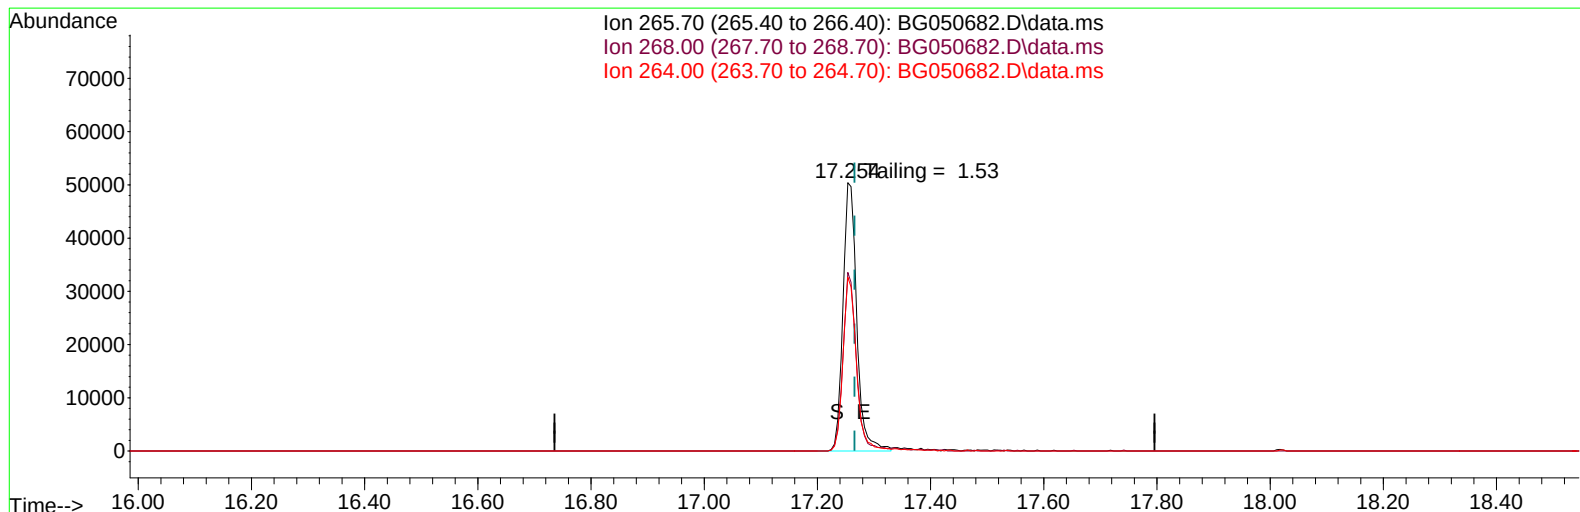

TIC: BG050682.D\data.ms

(70) Pentachlorophenol (C)




17.254min (-0.012) 20284.78 ng

response 86713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	66.54
264.00	61.30	64.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050682.D
Acq On : 22 Oct 2021 9:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 11:55:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

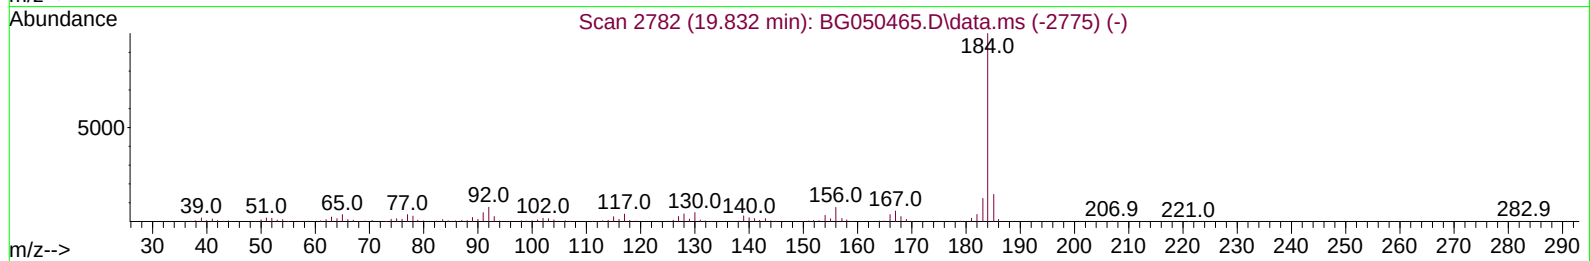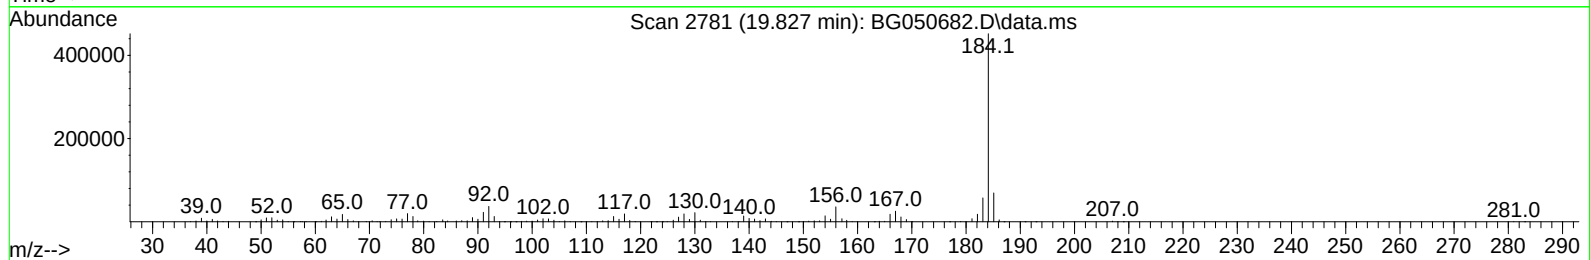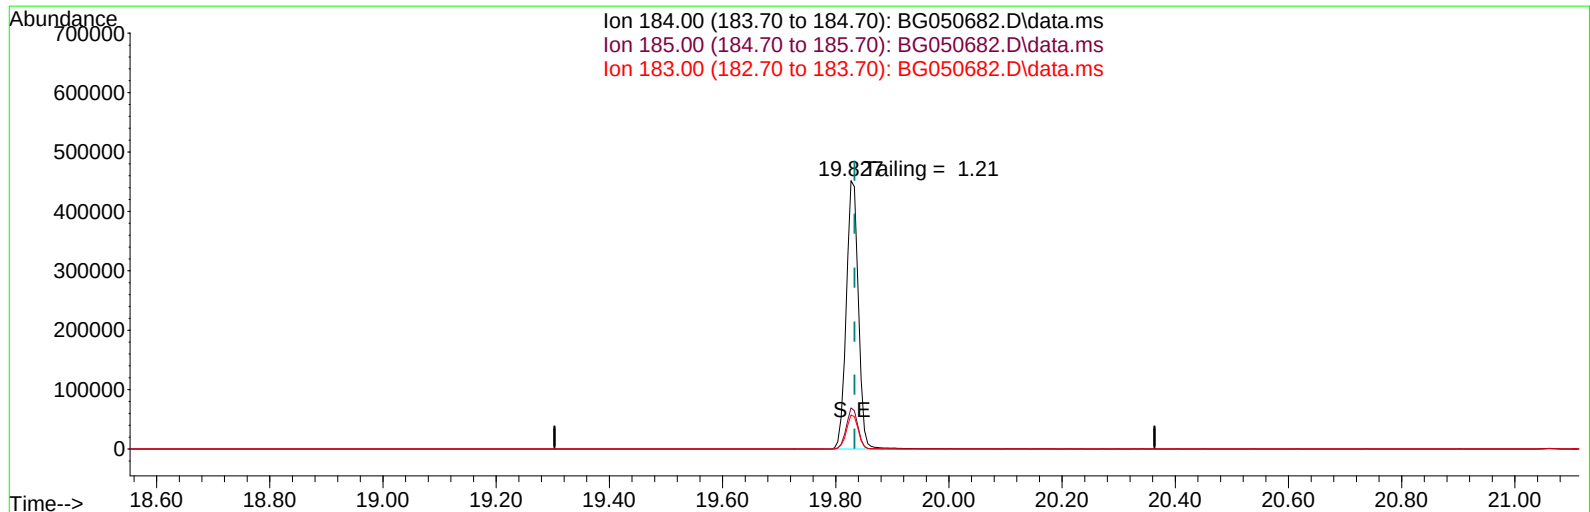

TIC: BG050682.D\data.ms

(77) Benzidine**19.827min (-0.006) 69474.85 ng****response 671025**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.32
183.00	11.70	12.70
0.00	0.00	0.00