
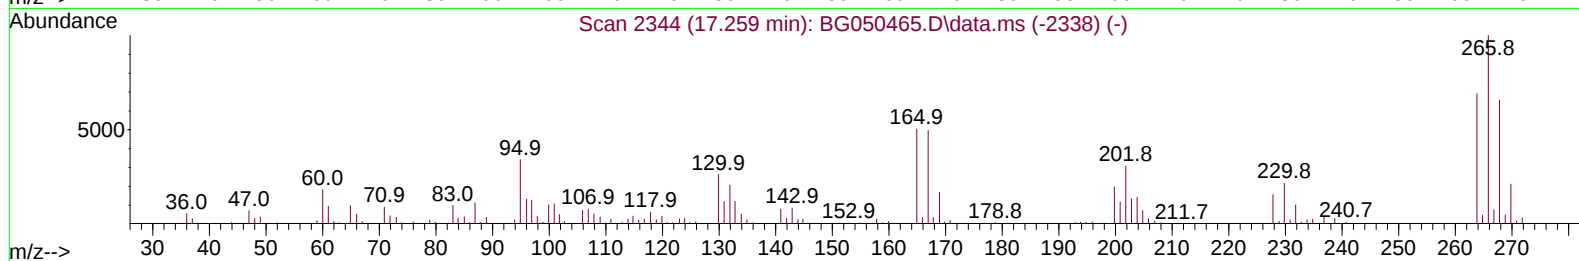
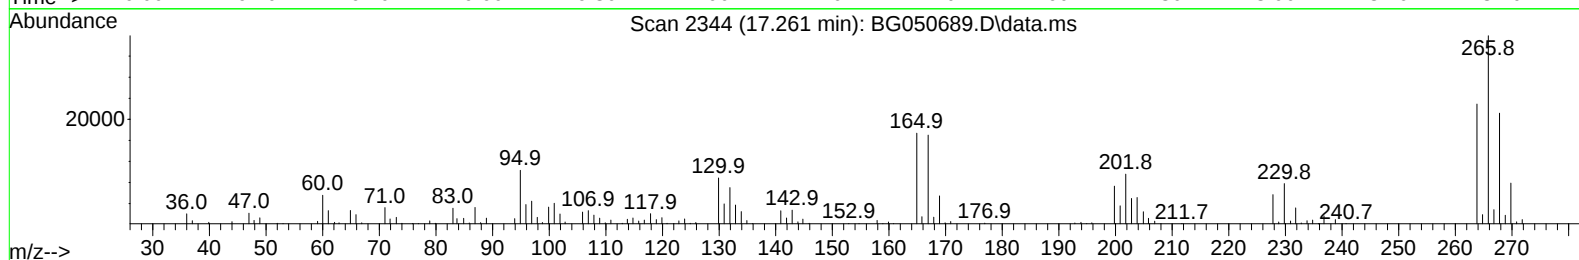


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050689.D
Acq On : 22 Oct 2021 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 16:03:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

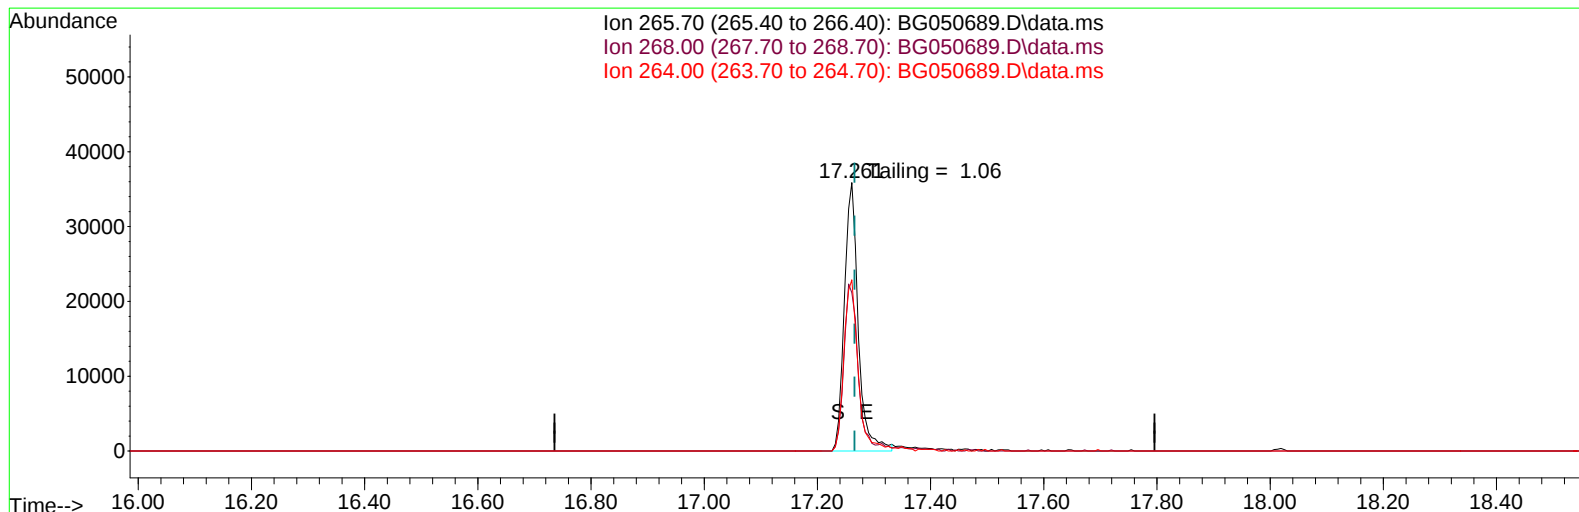

TIC: BG050689.D\data.ms

(70) Pentachlorophenol (C)




17.261min (-0.004) 22766.93 ng

response 63175

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	58.97
264.00	61.30	63.80
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\  
Data File : BG050689.D  
Acq On    : 22 Oct 2021  14:34  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Oct 22 16:03:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

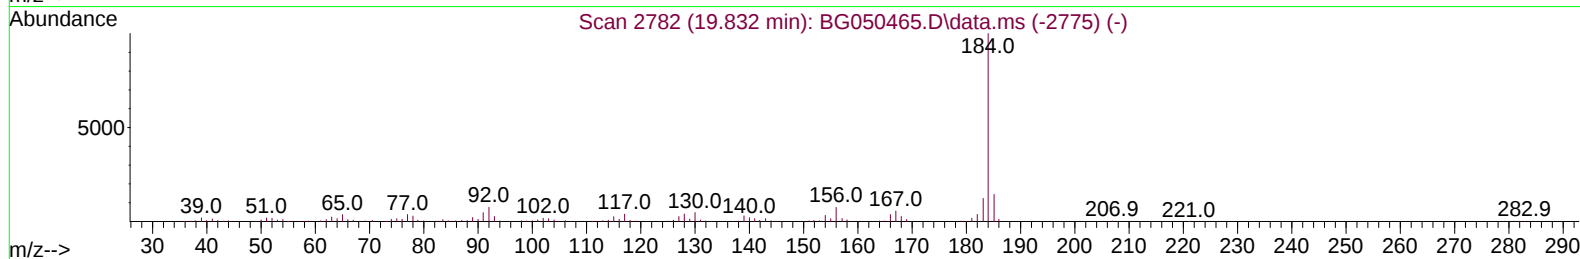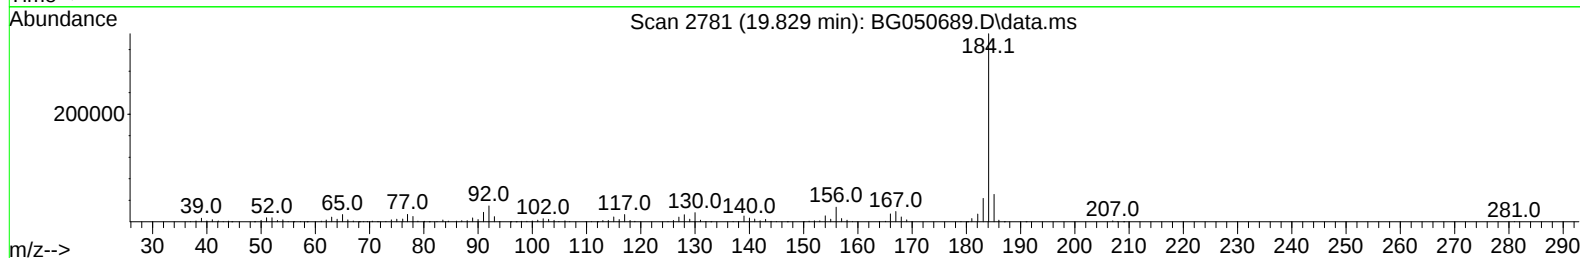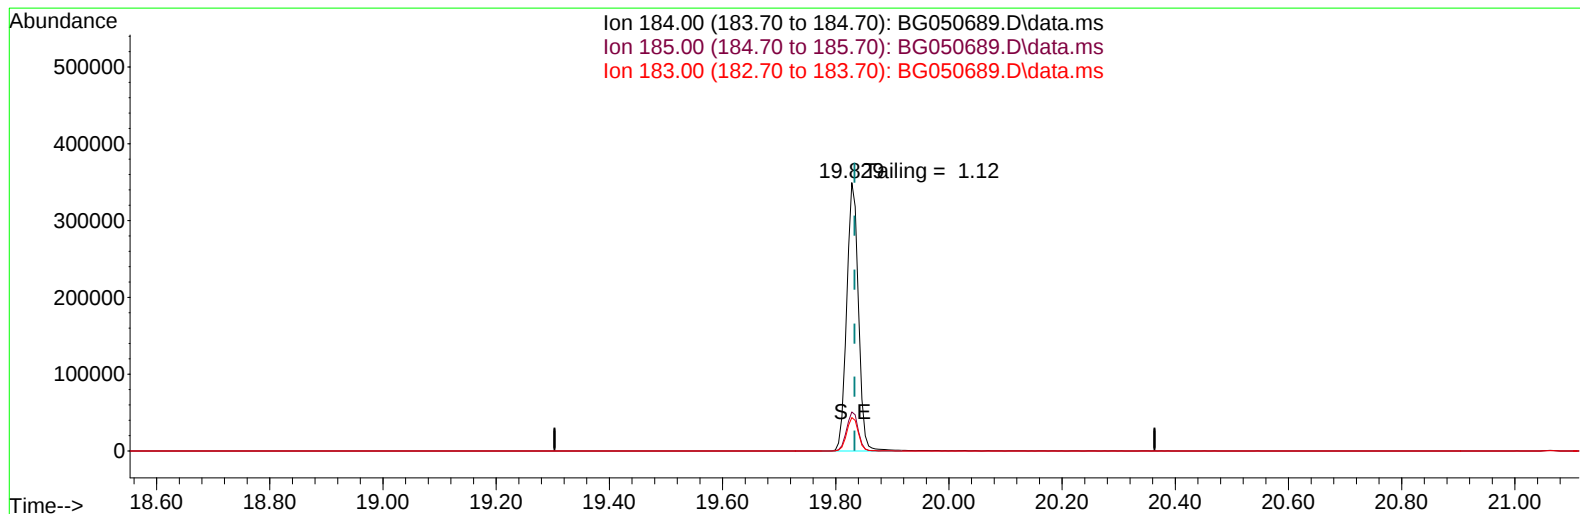

TIC: BG050689.D\data.ms

(77) Benzidine

19.829min (-0.004) 263356.52 ng

response **503606**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.58
183.00	11.70	12.46
0.00	0.00	0.00