

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
 Data File : BG050687.D
 Acq On : 22 Oct 2021 13:12
 Operator : CG/JU
 Sample : PB140104BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB140104BL

Quant Time: Oct 22 14:05:54 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 14 10:56:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.252	152	37873	20.000	ng	0.00
21) Naphthalene-d8	11.073	136	162296	20.000	ng	#-0.01
39) Acenaphthene-d10	14.868	164	105358	20.000	ng	0.00
64) Phenanthrene-d10	17.612	188	232251	20.000	ng	# 0.00
76) Chrysene-d12	21.913	240	218832	20.000	ng	#-0.01
86) Perylene-d12	25.327	264	204709	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.791	112	353074	139.422	ng	0.00
7) Phenol-d6	7.395	99	460913	125.710	ng	0.00
23) Nitrobenzene-d5	9.422	82	327601	83.559	ng	0.00
42) 2,4,6-Tribromophenol	16.355	330	121379	120.784	ng	0.00
45) 2-Fluorobiphenyl	13.493	172	594978	84.992	ng	-0.01
79) Terphenyl-d14	20.203	244	970500	86.429	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050687.D
Acq On : 22 Oct 2021 13:12
Operator : CG/JU
Sample : PB140104BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140104BL

Quant Time: Oct 22 14:05:54 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration



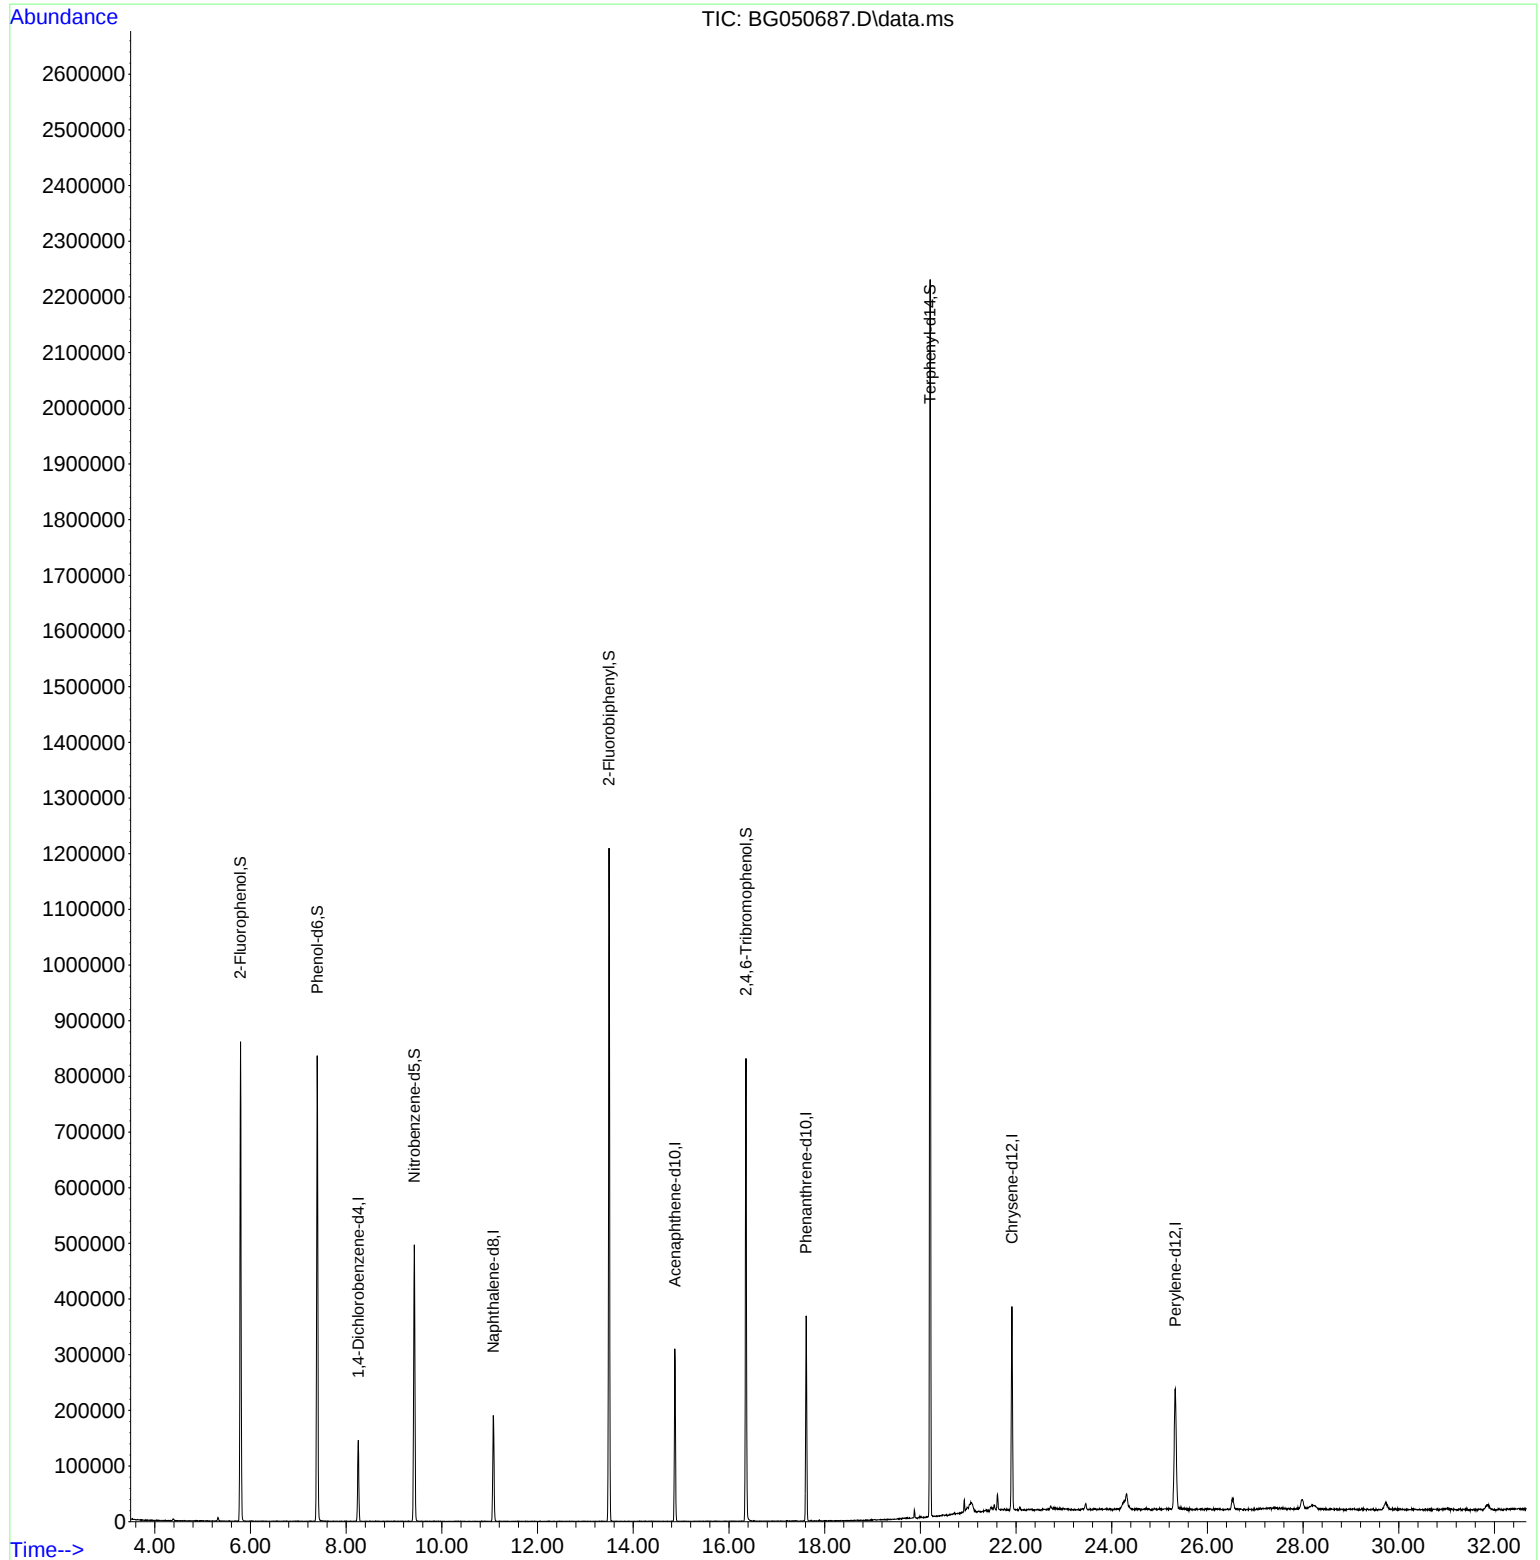


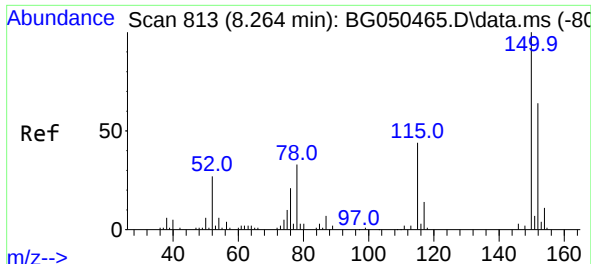

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.252 min Scan# 811
Delta R.T. -0.005 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12




Instrument :
BNA_G
ClientSampleId :
PB140104BL

Tgt Ion:152 Resp: 37873
Ion Ratio Lower Upper
152 100
150 156.3 119.4 179.0
115 62.1 60.2 90.4

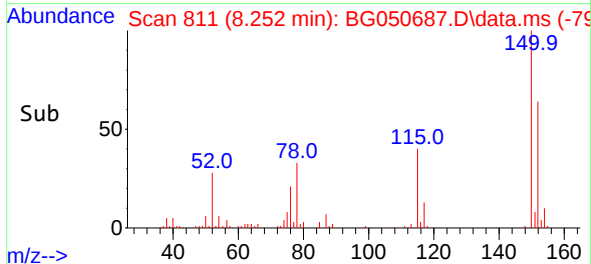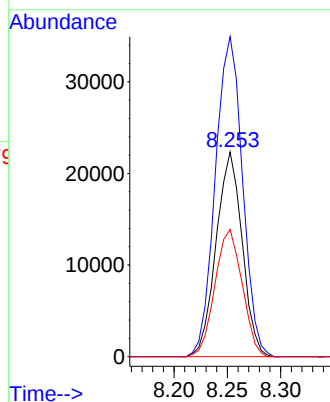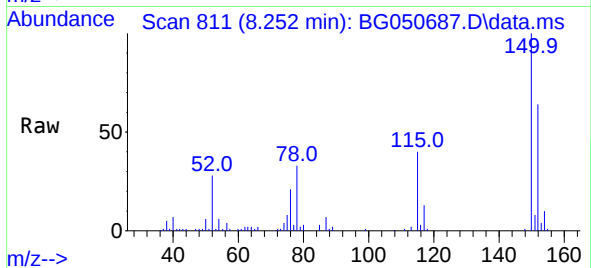

#5
2-Fluorophenol
Concen: 139.422 ng
RT: 5.791 min Scan# 392
Delta R.T. 0.000 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Tgt Ion:112 Resp: 353074
Ion Ratio Lower Upper
112 100
64 70.4 46.7 70.1#
63 38.0 35.3 52.9

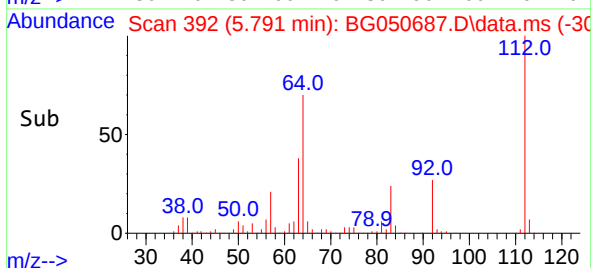
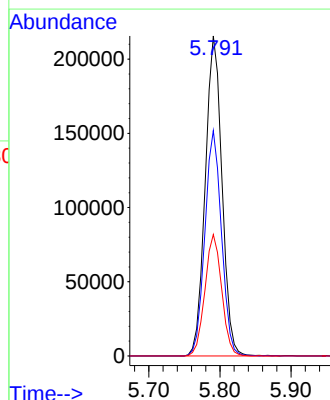
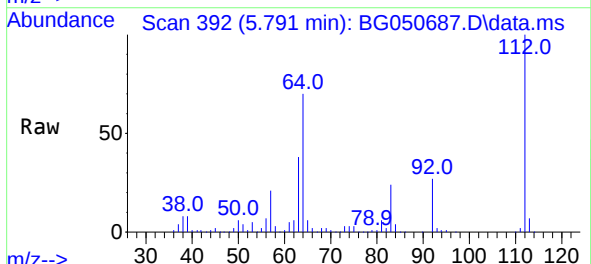




#7
Phenol-d6
Concen: 125.710 ng
RT: 7.395 min Scan# 665
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12




Instrument :
BNA_G
ClientSampleId :
PB140104BL

Tgt Ion: 99 Resp: 460913
Ion Ratio Lower Upper
99 100
42 23.0 20.5 30.7
71 41.8 41.5 62.3

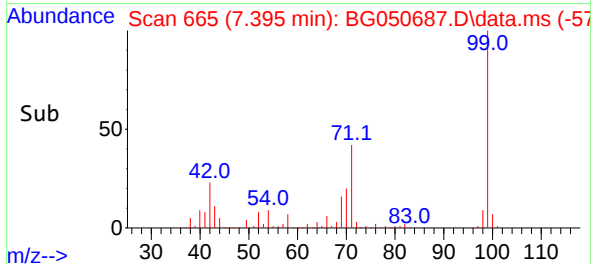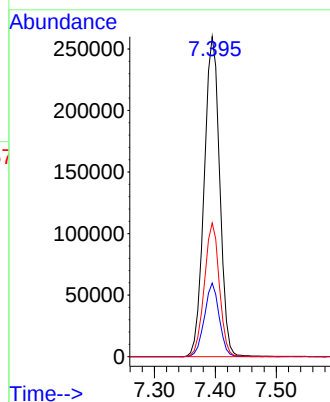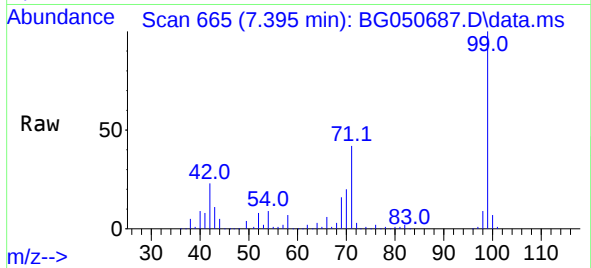

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.073 min Scan# 1291
Delta R.T. -0.012 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Tgt Ion: 136 Resp: 162296
Ion Ratio Lower Upper
136 100
137 10.8 8.2 12.2
54 9.8 5.5 8.3#
68 6.9 2.3 3.5#

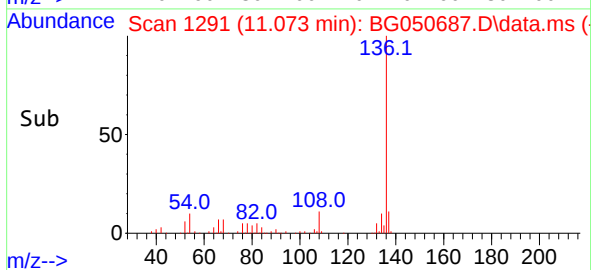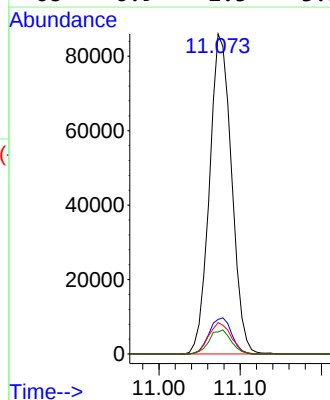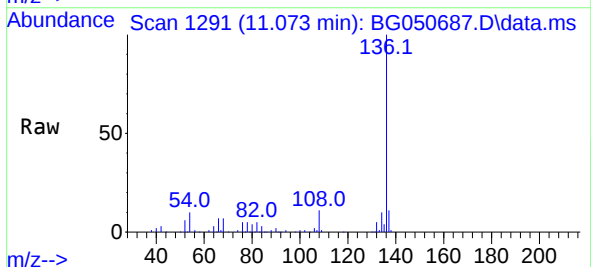







#23
Nitrobenzene-d5
Concen: 83.559 ng
RT: 9.422 min Scan# 1010
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Instrument :
BNA_G
ClientSampleId :
PB140104BL

Tgt Ion: 82 Resp: 327601




Ion	Ratio	Lower	Upper
82	100		
128	35.2	29.8	44.6
54	50.9	45.8	68.8

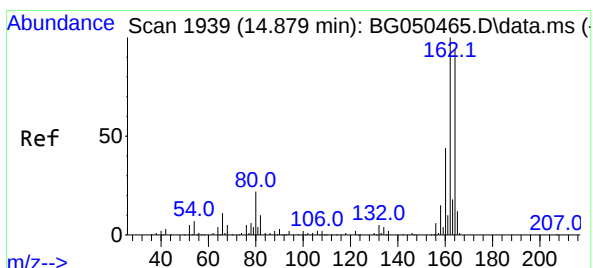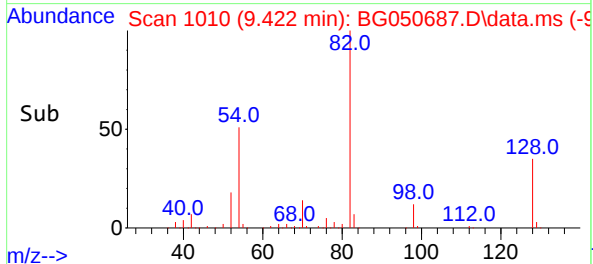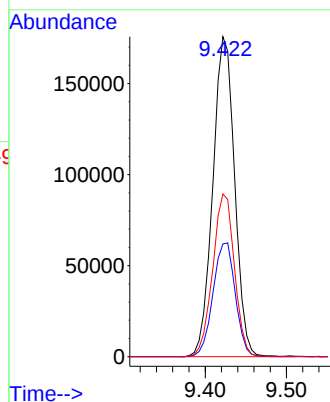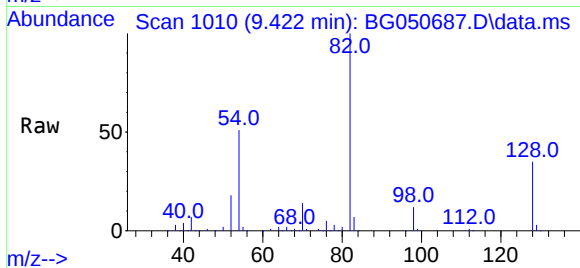


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.868 min Scan# 1937
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Tgt Ion: 164 Resp: 105358


Ion	Ratio	Lower	Upper
164	100		
162	105.1	81.4	122.0
160	43.8	34.9	52.3

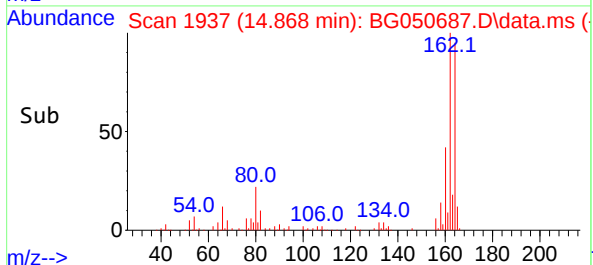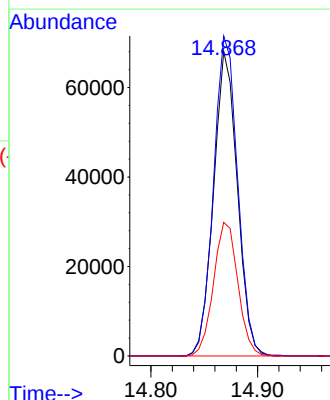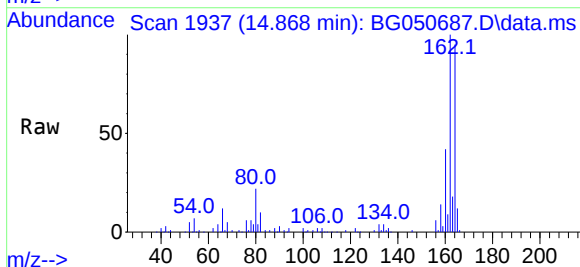


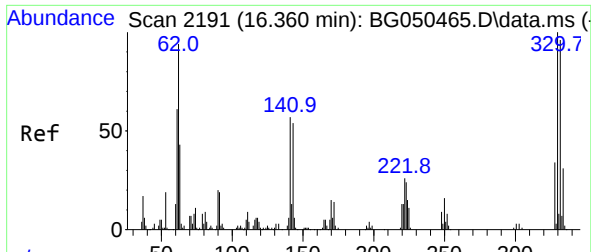


#42
2,4,6-Tribromophenol
Concen: 120.784 ng
RT: 16.355 min Scan# 2190
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12


Instrument :
BNA_G
ClientSampleId :
PB140104BL

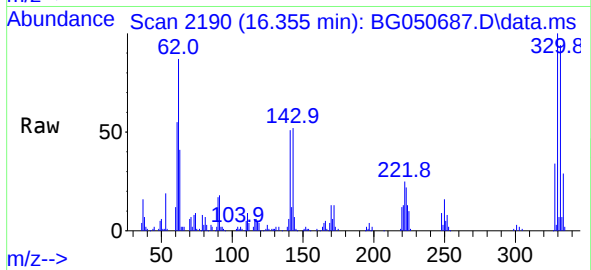



Tgt Ion:330 Resp: 121379
Ion Ratio Lower Upper
330 100
332 95.1 77.3 115.9
141 54.2 35.6 53.4#

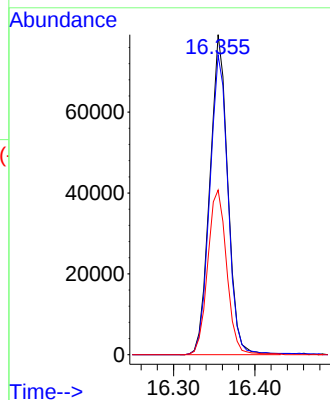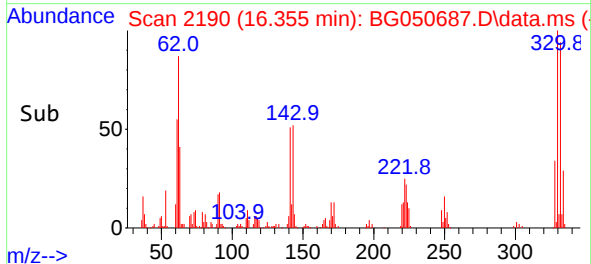


#45
2-Fluorobiphenyl
Concen: 84.992 ng
RT: 13.493 min Scan# 1703
Delta R.T. -0.012 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

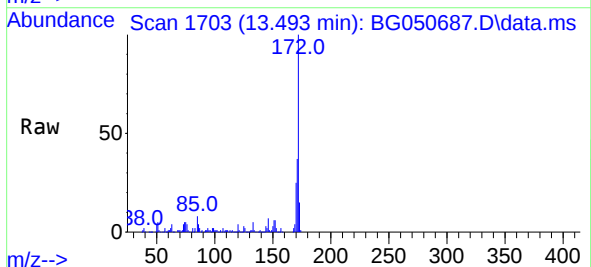

Tgt Ion:172 Resp: 594978
Ion Ratio Lower Upper
172 100
171 37.2 28.6 43.0
170 25.5 18.6 27.8


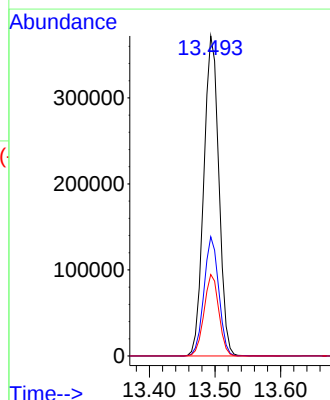
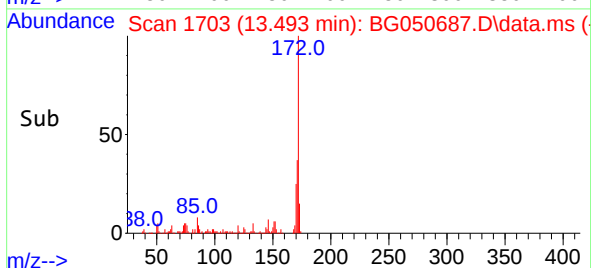


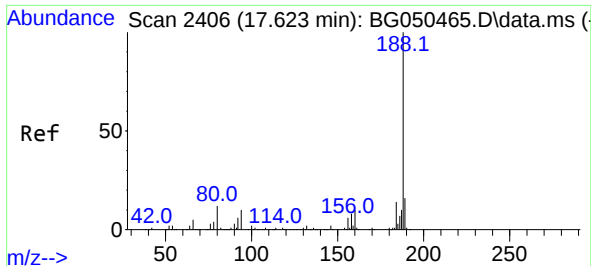

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.612 min Scan# 2404
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12




Instrument :
BNA_G
ClientSampleId :
PB140104BL

Tgt Ion:188 Resp: 232251
Ion Ratio Lower Upper
188 100
94 9.1 5.4 8.0#
80 12.2 3.7 5.5#

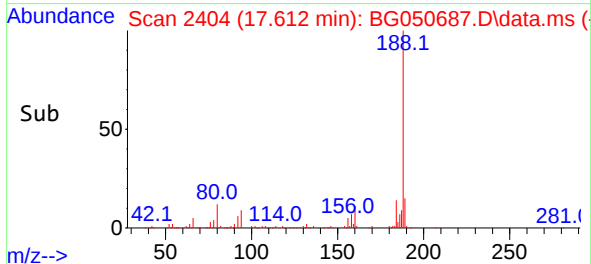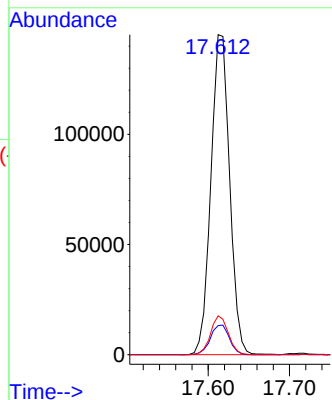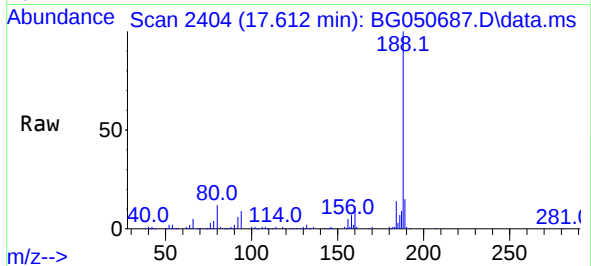

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.913 min Scan# 3136
Delta R.T. -0.012 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Tgt Ion:240 Resp: 218832
Ion Ratio Lower Upper
240 100
120 9.9 4.2 6.2#
236 26.1 21.8 32.6


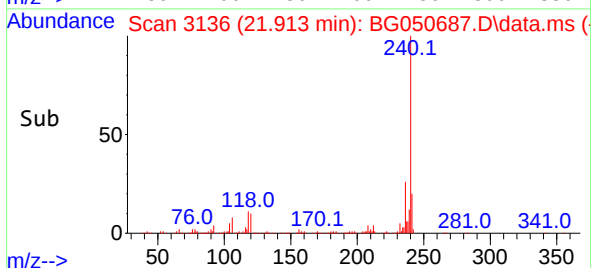
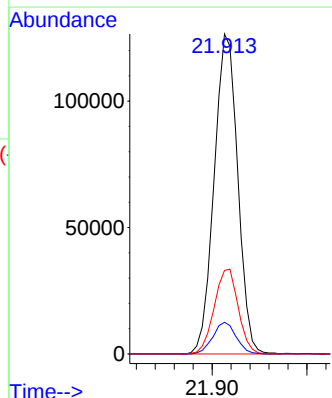
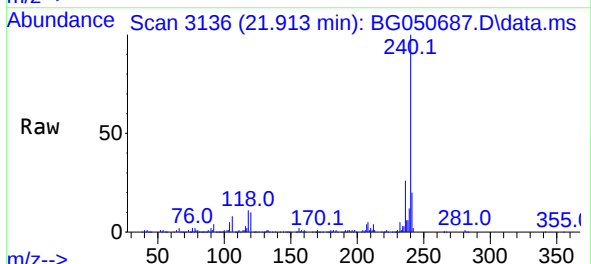




#79
Terphenyl-d14
Concen: 86.429 ng
RT: 20.203 min Scan# 2845
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Instrument :
BNA_G
ClientSampleId :
PB140104BL

Tgt Ion:244 Resp: 970500
Ion Ratio Lower Upper
244 100
212 8.8 6.9 10.3
122 11.4 5.0 7.6#

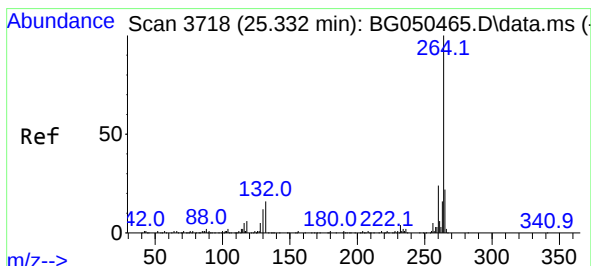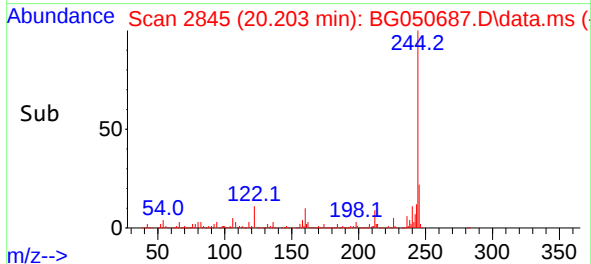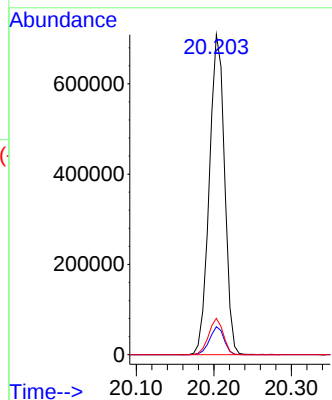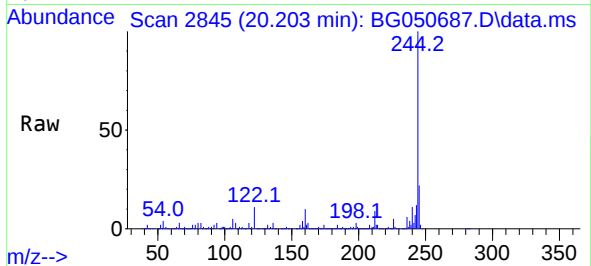

#86
Perylene-d12
Concen: 20.000 ng
RT: 25.327 min Scan# 3717
Delta R.T. -0.006 min
Lab File: BG050687.D
Acq: 22 Oct 2021 13:12

Tgt Ion:264 Resp: 204709
Ion Ratio Lower Upper
264 100
260 25.0 19.4 29.2
265 22.3 16.9 25.3

