

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
 Data File : BG050684.D
 Acq On : 22 Oct 2021 11:09
 Operator : CG/JU
 Sample : PB140070BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB140070BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.791	385	392	408	rVB	825919	1348035	45.04%	10.457%
2	7.395	656	665	675	rBV	804035	1411490	47.16%	10.949%
3	8.253	804	811	822	rVB	141525	245165	8.19%	1.902%
4	9.422	1001	1010	1019	rBV	478299	893995	29.87%	6.935%
5	11.079	1284	1292	1300	rBV	190650	351134	11.73%	2.724%
6	13.494	1696	1703	1711	rBV	1169632	1815891	60.67%	14.086%
7	14.869	1930	1937	1946	rVB	282716	461961	15.43%	3.583%
8	16.355	2183	2190	2203	rBV	833206	1287316	43.01%	9.986%
9	17.612	2398	2404	2416	rBV	367939	584605	19.53%	4.535%
10	20.204	2839	2845	2851	rVB	2280754	2993150	100.00%	23.218%
11	21.478	3056	3062	3066	rBV2	14959	33619	1.12%	0.261%
12	21.549	3069	3074	3078	rVB	20693	36934	1.23%	0.287%
13	21.608	3080	3084	3090	rBV	57597	90146	3.01%	0.699%
14	21.913	3129	3136	3143	rBV	359188	632465	21.13%	4.906%
15	25.327	3707	3717	3730	rVB3	219031	657077	21.95%	5.097%
16	26.531	3914	3922	3930	rVB6	17472	48401	1.62%	0.375%




Sum of corrected areas: 12891384

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050684.D
Acq On : 22 Oct 2021 11:09
Operator : CG/JU
Sample : PB140070BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140070BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

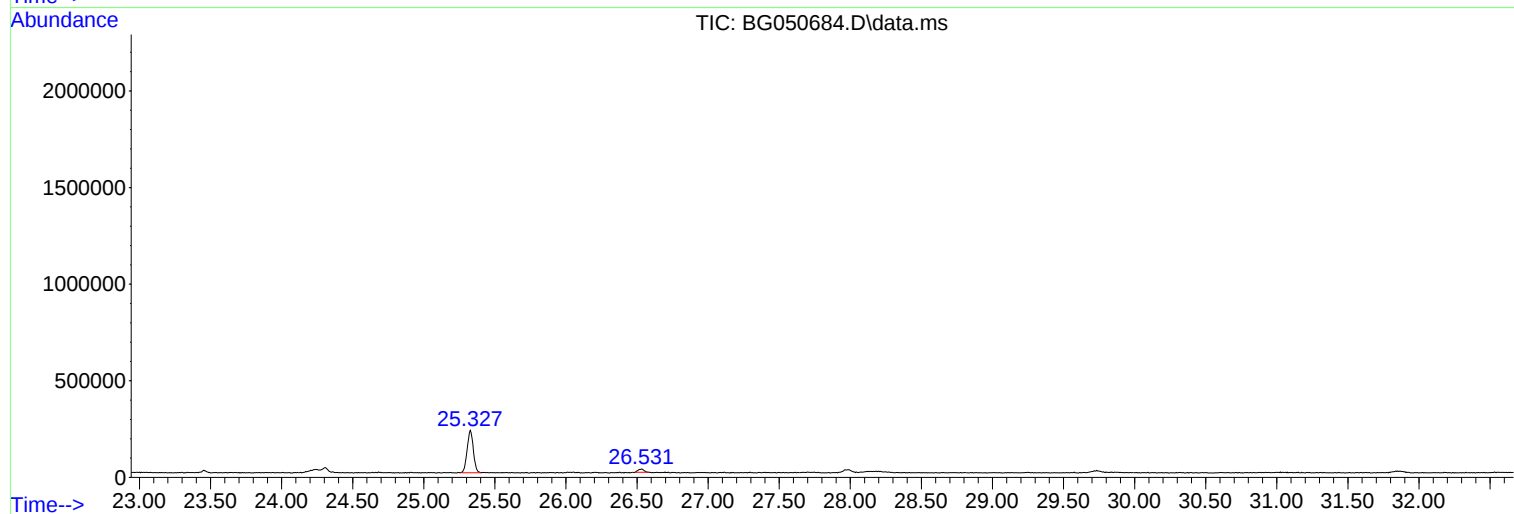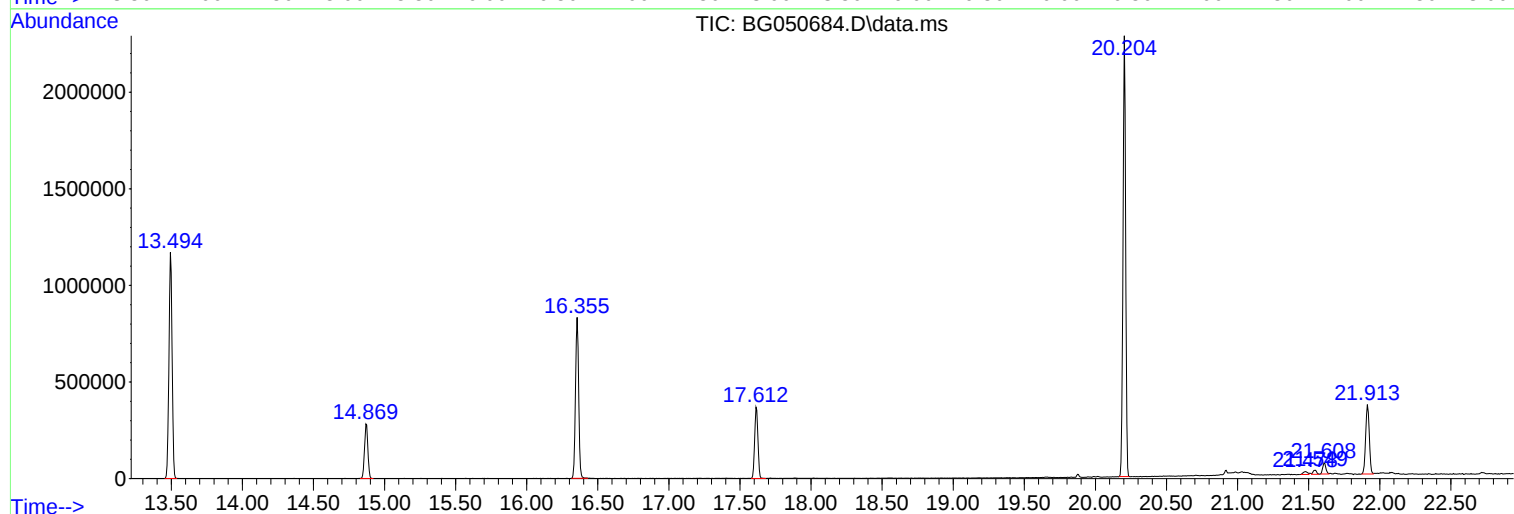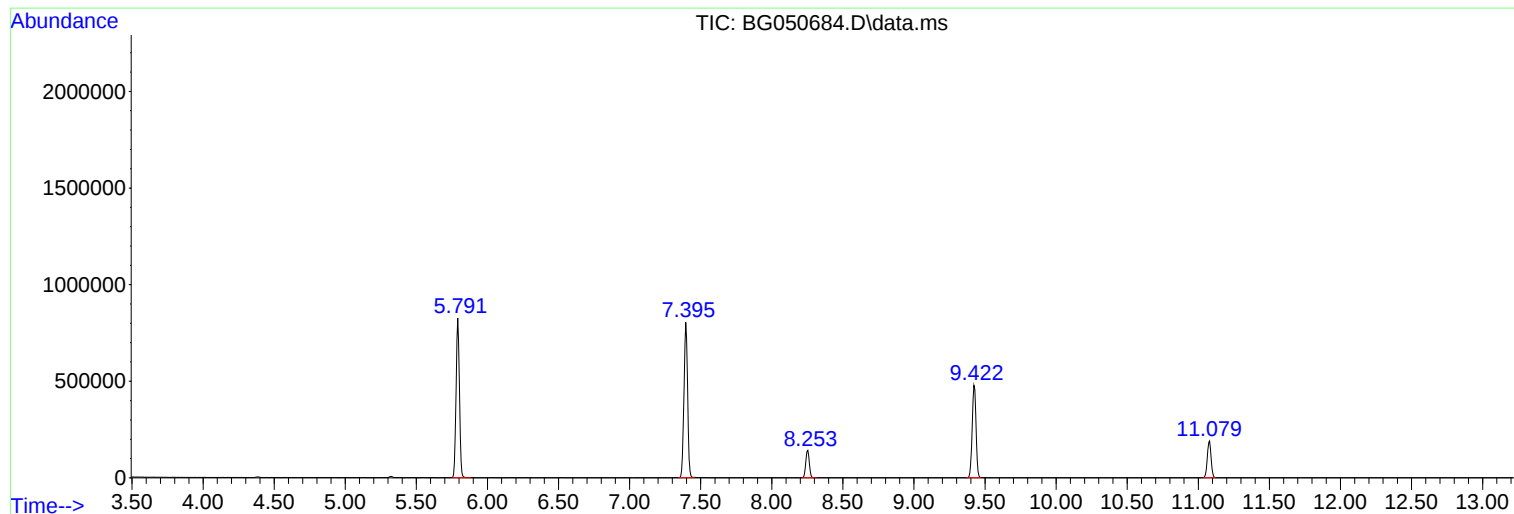

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050684.D
Acq On : 22 Oct 2021 11:09
Operator : CG/JU
Sample : PB140070BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140070BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.608	2.85 ng	90146	Chrysene-d12	21.913

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	78
2			2,2'-(Ethane-1,2-diylbis(oxy))bi...	358	C20H22O6	1000366-99-4	59
3			1,3-Dioxolane, 2-(methoxymethyl)...	194	C11H14O3	1000156-71-2	59
4			3-Benzoylaminochromone	265	C16H11NO3	1000243-49-5	47
5			Benzenepropanenitrile, .beta.-oxo-	145	C9H7NO	000614-16-4	43

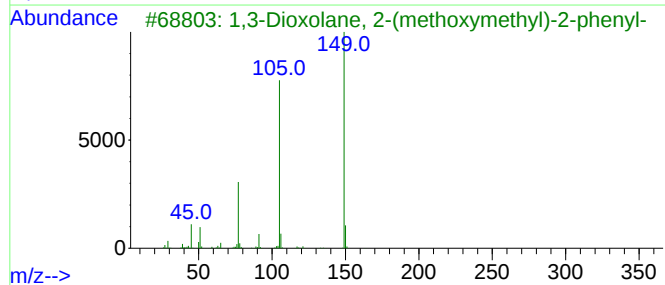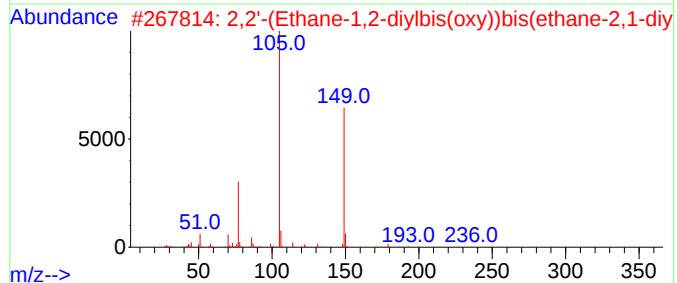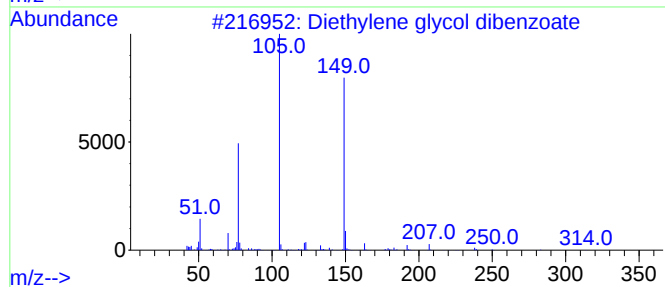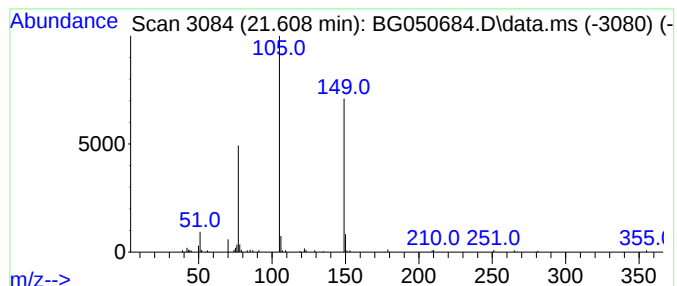

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050684.D
Acq On : 22 Oct 2021 11:09
Operator : CG/JU
Sample : PB140070BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB140070BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glyc...	21.608	2.9	ng	90146	5	21.913	632465	20.0