
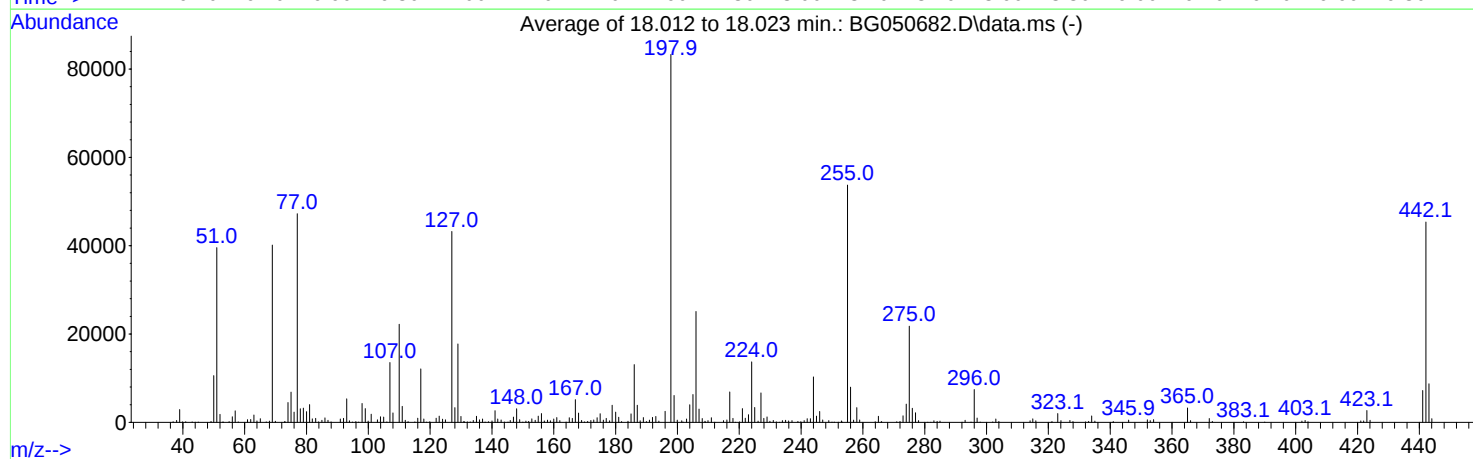


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
 Data File : BG050682.D
 Acq On : 22 Oct 2021 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

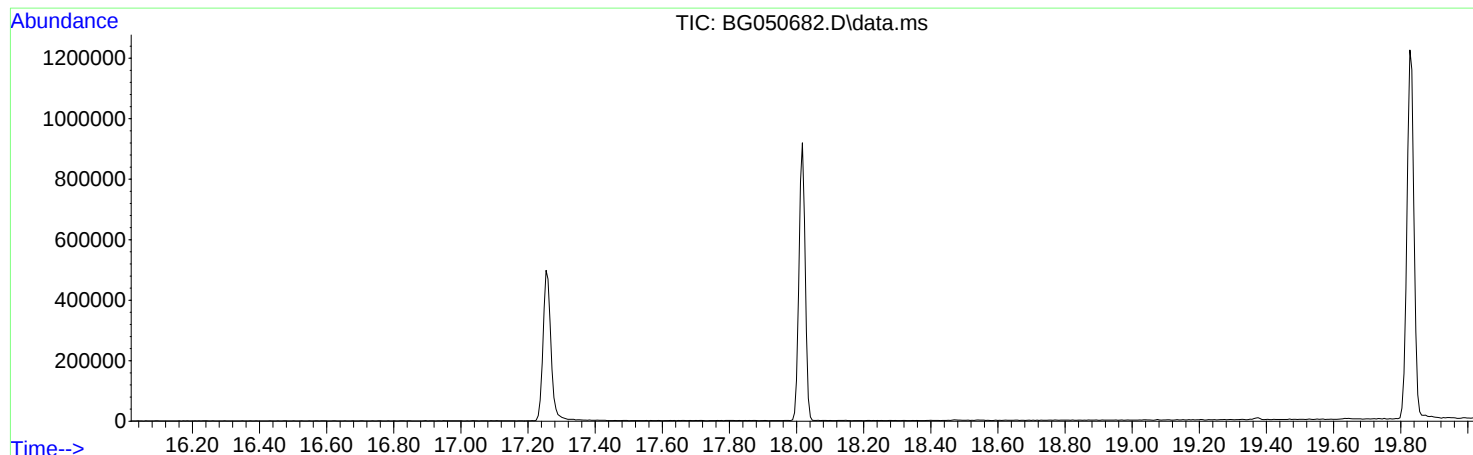




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	39552	PASS
68	69	0.00	2	0.8	304	PASS
69	198	0.00	100	48.2	40149	PASS
70	69	0.00	2	0.6	250	PASS
127	198	10	80	51.9	43216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83299	PASS
199	198	5	9	7.3	6083	PASS
275	198	10	60	26.1	21765	PASS
365	198	1	100	3.9	3272	PASS
441	198	0.01	100	8.7	7215	PASS
442	442	50	100	100.0	45379	PASS
443	442	15	24	19.3	8751	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050682.D
Acq On : 22 Oct 2021 9:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 11:55:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

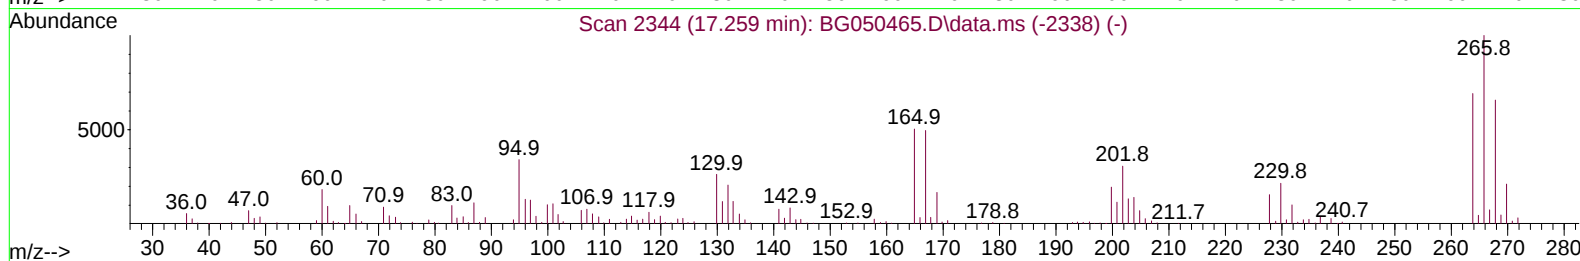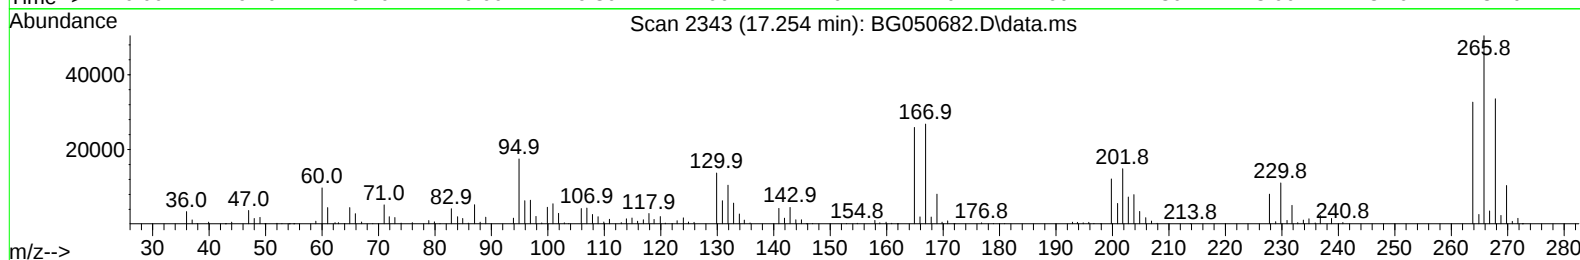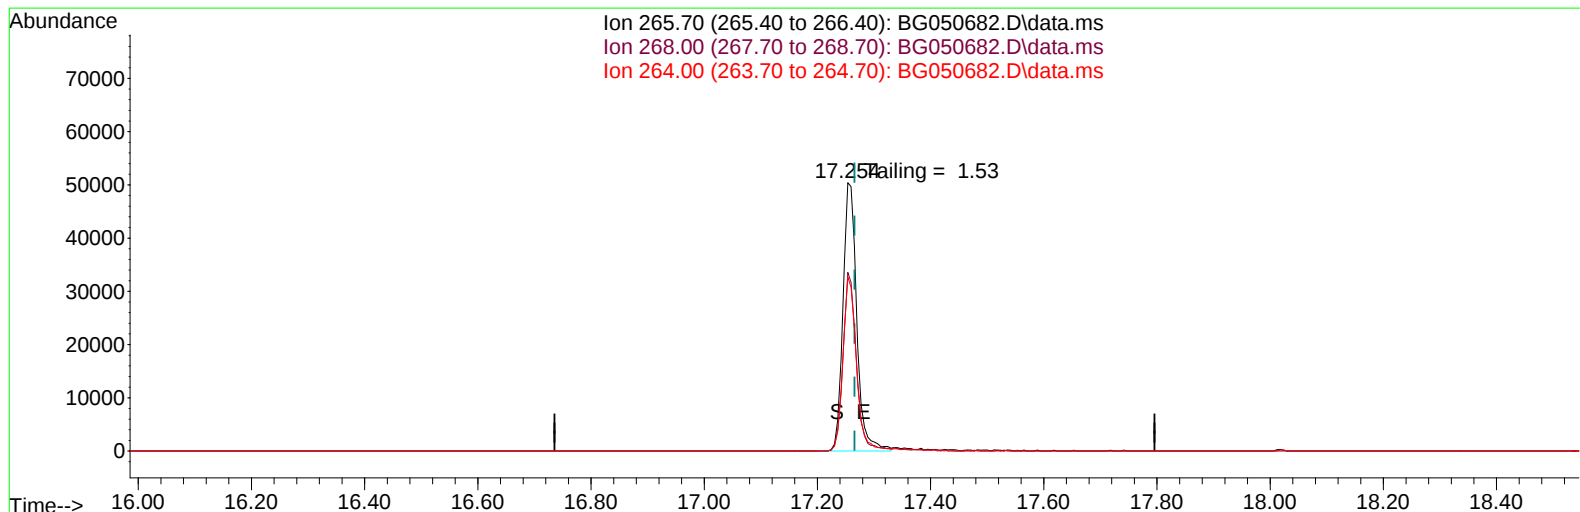

TIC: BG050682.D\data.ms

(70) Pentachlorophenol (C)

17.254min (-0.012) 20284.78 ng




response 86713

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	66.54
264.00	61.30	64.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050682.D
Acq On : 22 Oct 2021 9:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 11:55:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

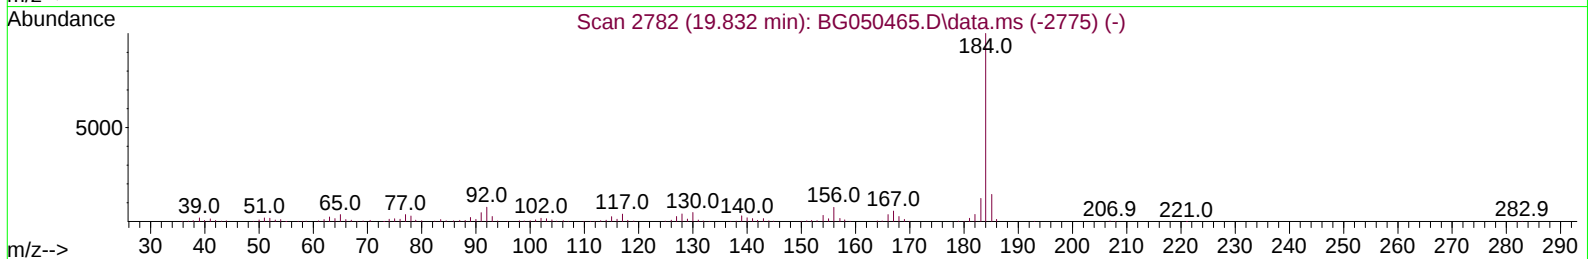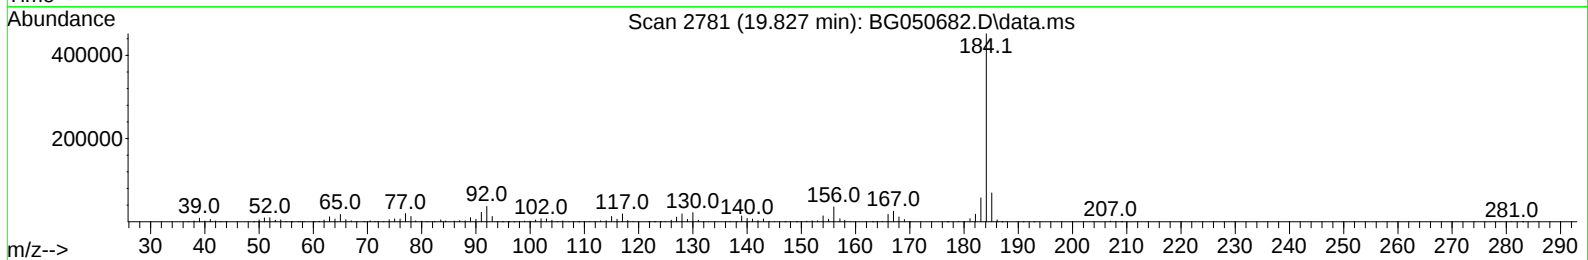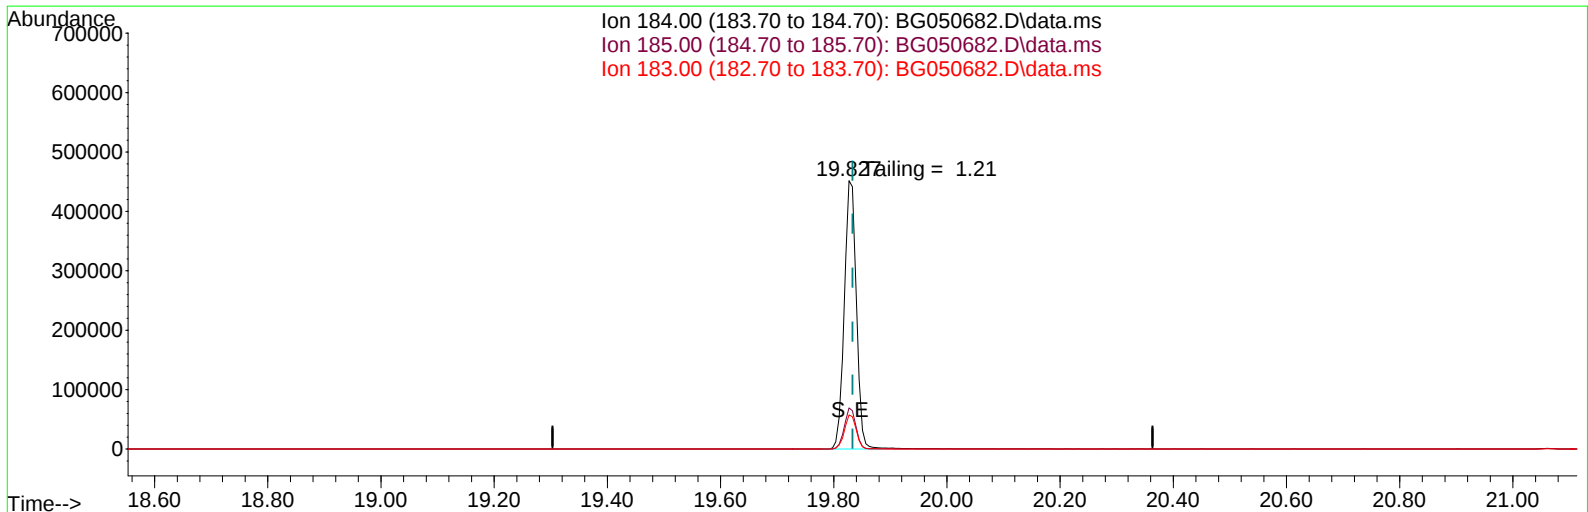

TIC: BG050682.D\data.ms

(77) Benzidine

19.827min (-0.006) 69474.85 ng

response 671025

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.32
183.00	11.70	12.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2021	BNA_G	BG050682.D
Compound Name	Response	Retention Time
DDT	294569	21.06
DDD	4164	20.6
DDE	590	20.1
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4754	299323	1.59

Instrument :
BNA_G
ClientSampleId :
DFTPP