


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
 Data File : BG050689.D
 Acq On : 22 Oct 2021 14:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

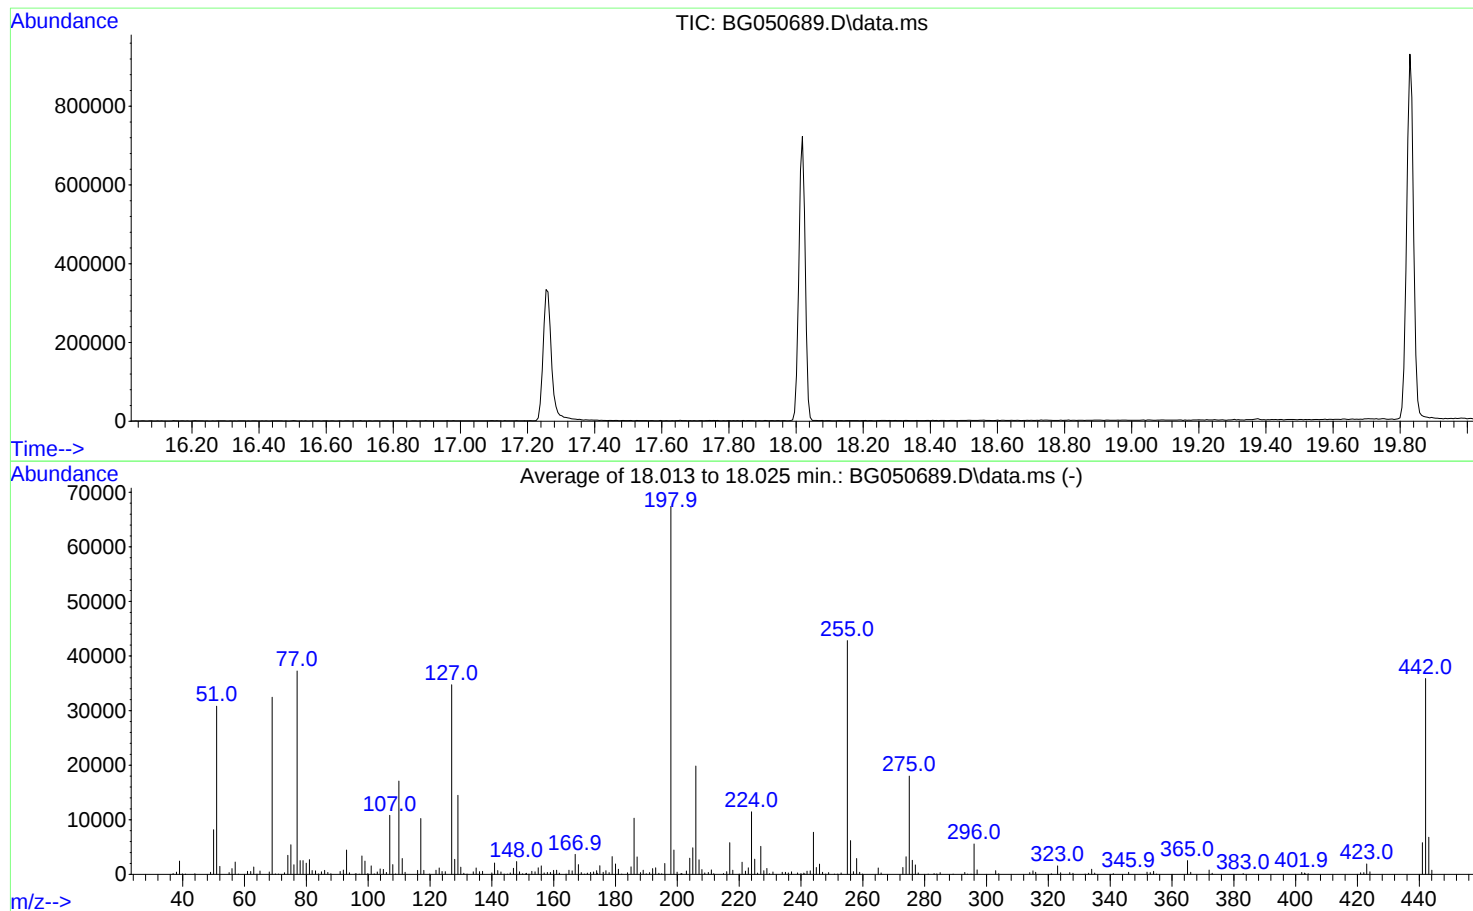




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	30824	PASS
68	69	0.00	2	1.3	428	PASS
69	198	0.00	100	48.1	32443	PASS
70	69	0.00	2	0.3	84	PASS
127	198	10	80	51.5	34733	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67395	PASS
199	198	5	9	6.6	4467	PASS
275	198	10	60	26.7	18000	PASS
365	198	1	100	3.7	2514	PASS
441	198	0.01	100	8.6	5802	PASS
442	442	50	100	100.0	35877	PASS
443	442	15	24	19.0	6804	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050689.D
Acq On : 22 Oct 2021 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 16:03:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

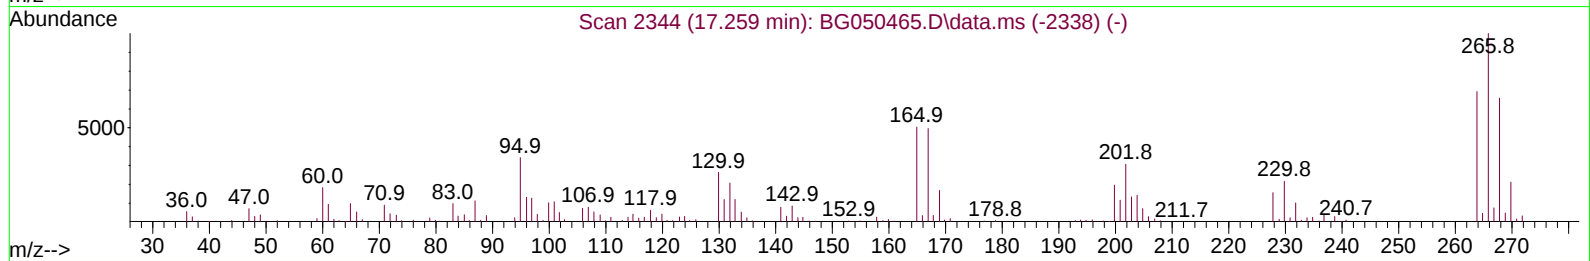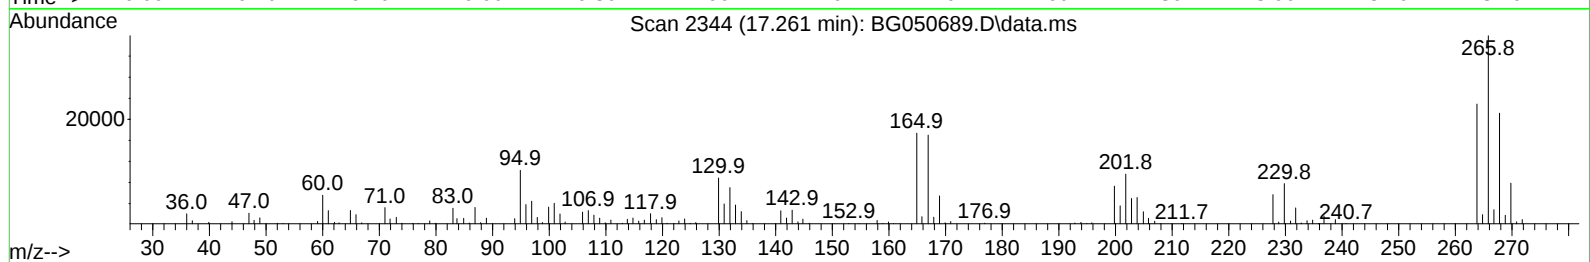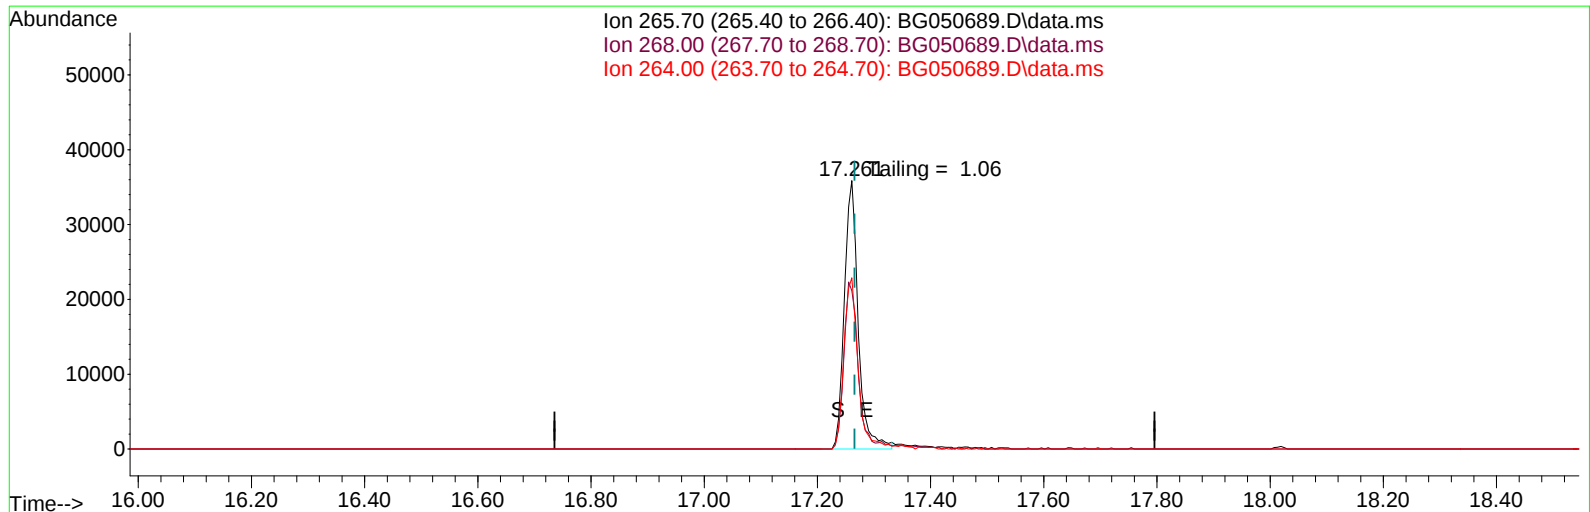

TIC: BG050689.D\data.ms

(70) Pentachlorophenol (C)

17.261min (-0.004) 22766.93 ng




response 63175

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	58.97
264.00	61.30	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102221\
Data File : BG050689.D
Acq On : 22 Oct 2021 14:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 16:03:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

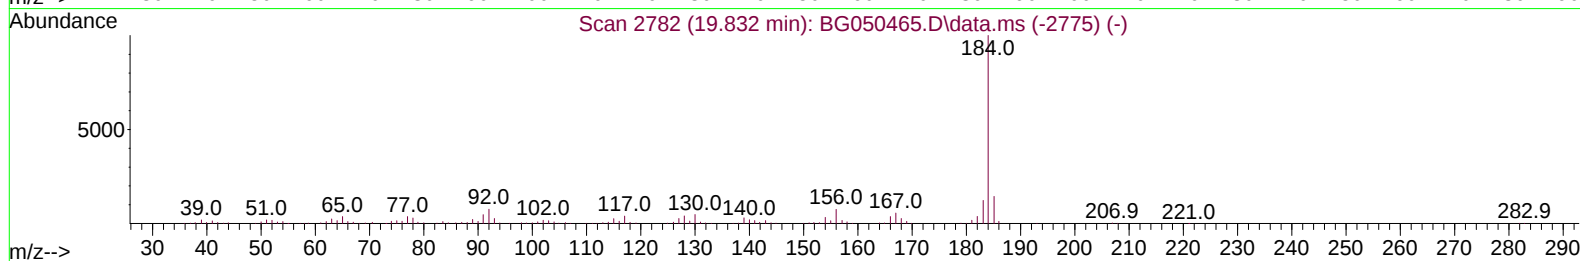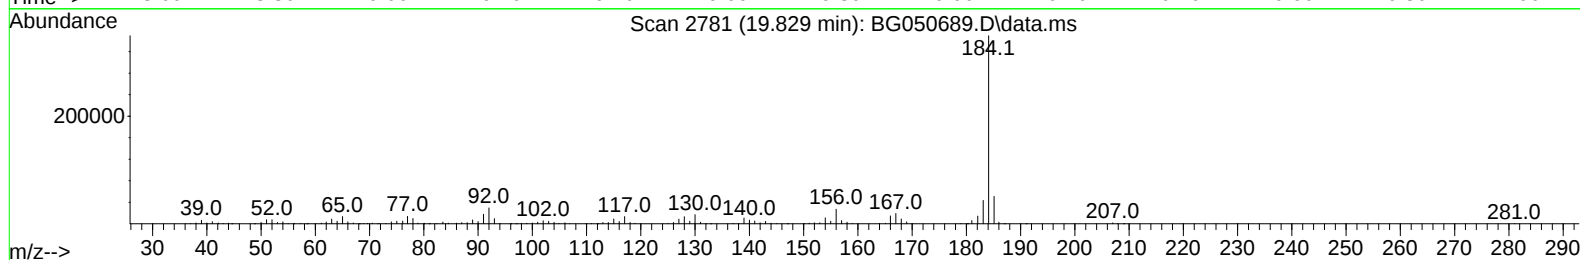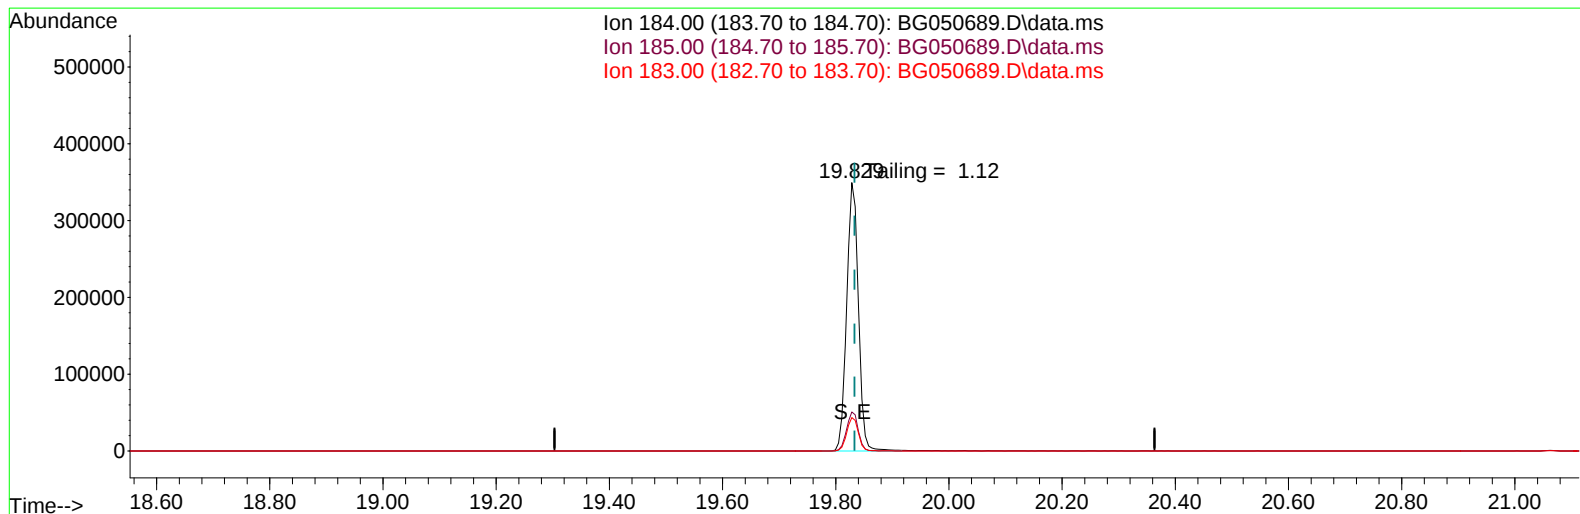

TIC: BG050689.D\data.ms

(77) Benzidine

19.829min (-0.004) 263356.52 ng

response 503606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.58
183.00	11.70	12.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/22/2021	BNA_G	BG050689.D
Compound Name	Response	Retention Time
DDT	221812	21.06
DDD	9544	20.61
DDE	686	20.1
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10230	232042	4.41

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP