
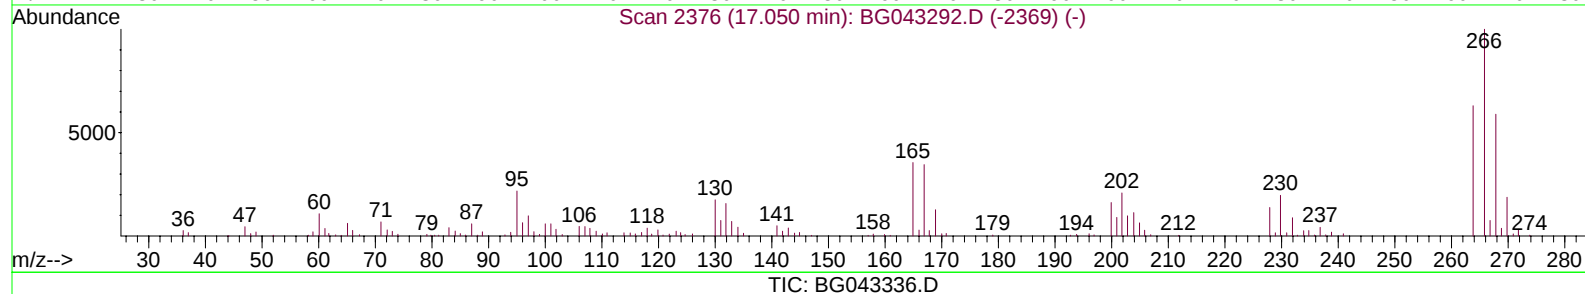
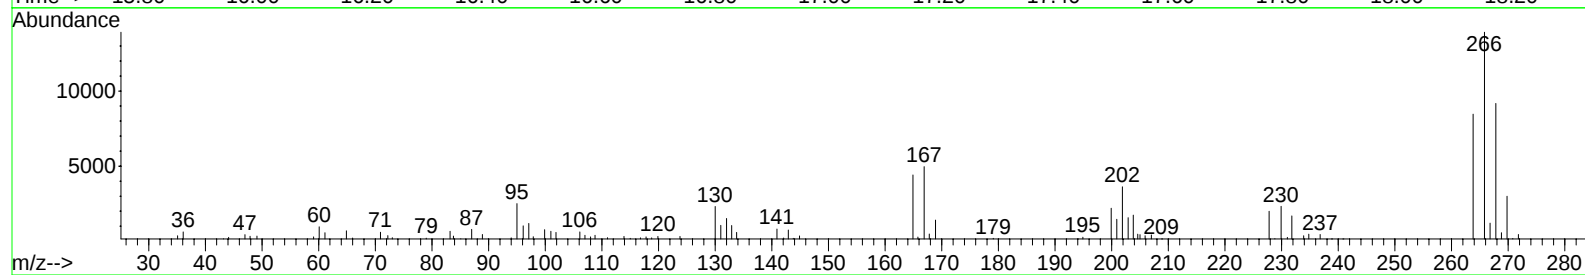


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102519\
Data File : BG043336.D
Acq On : 25 Oct 2019 11:53
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 15:42:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

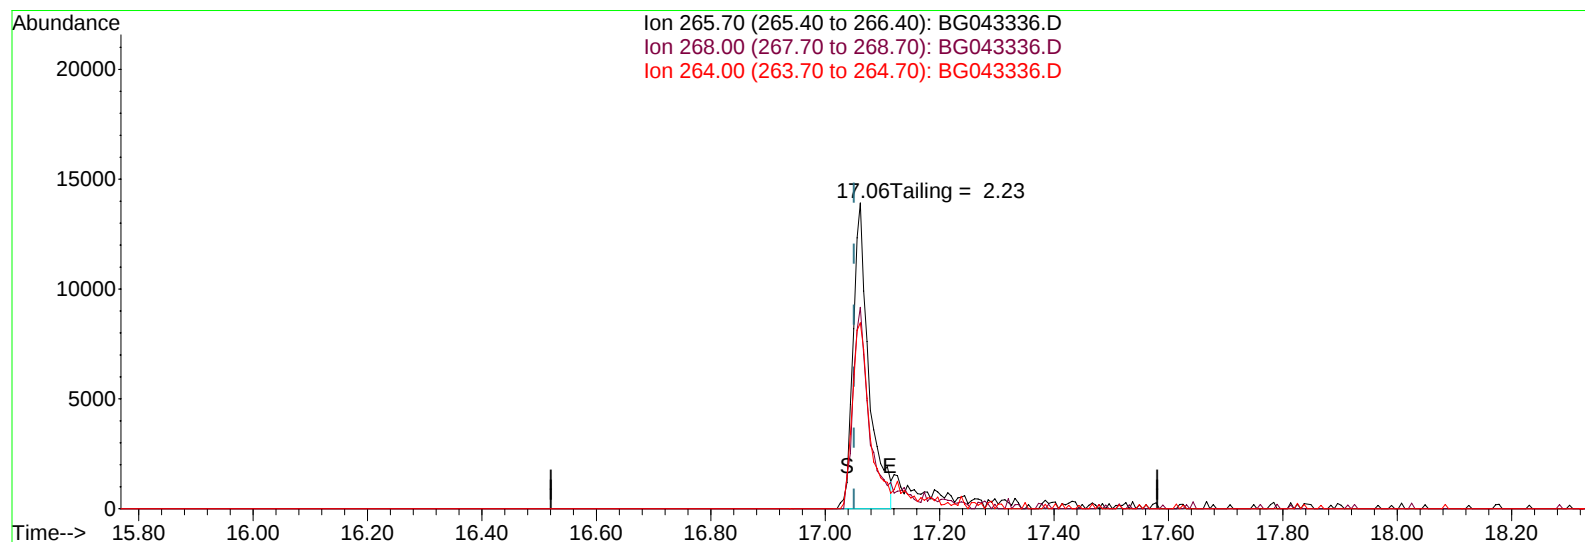

(70) Pentachlorophenol (C)




17.061min (+0.011) 24942.57ng

response 28618

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	65.90
264.00	63.00	60.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102519\
 Data File : BG043336.D
 Acq On : 25 Oct 2019 11:53
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 15:42:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 16:37:43 2019
 Response via : Initial Calibration

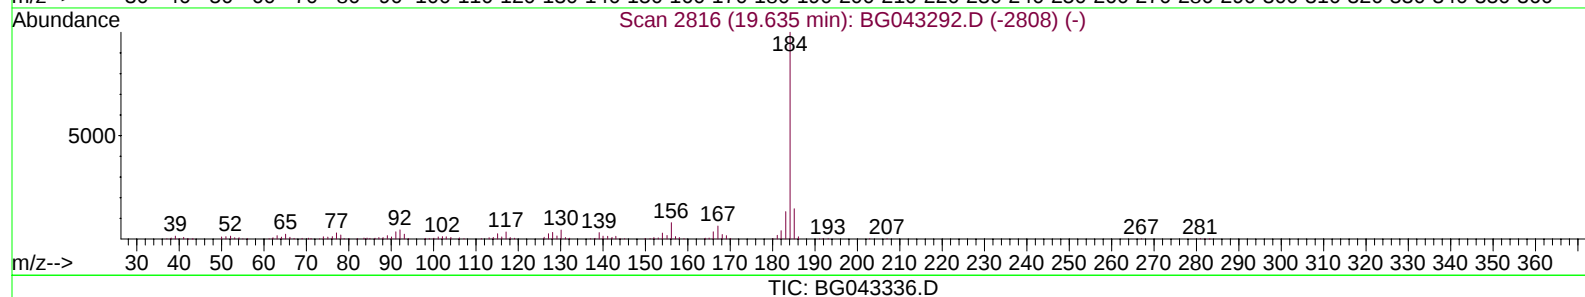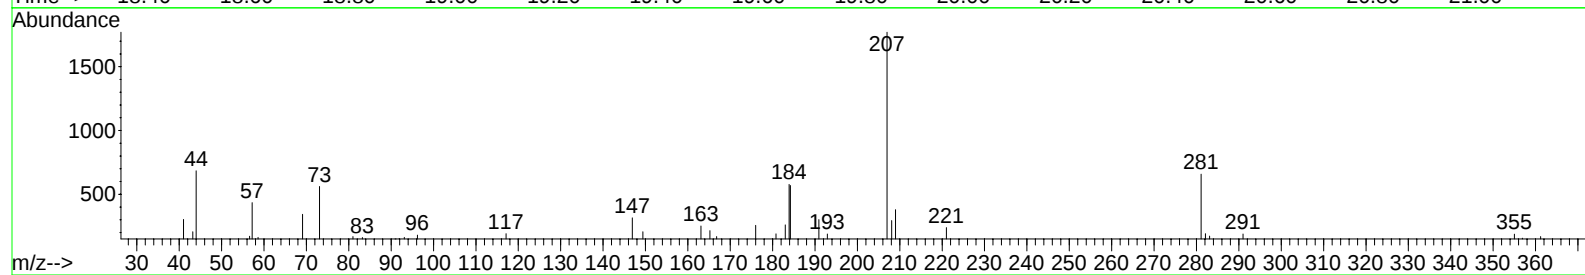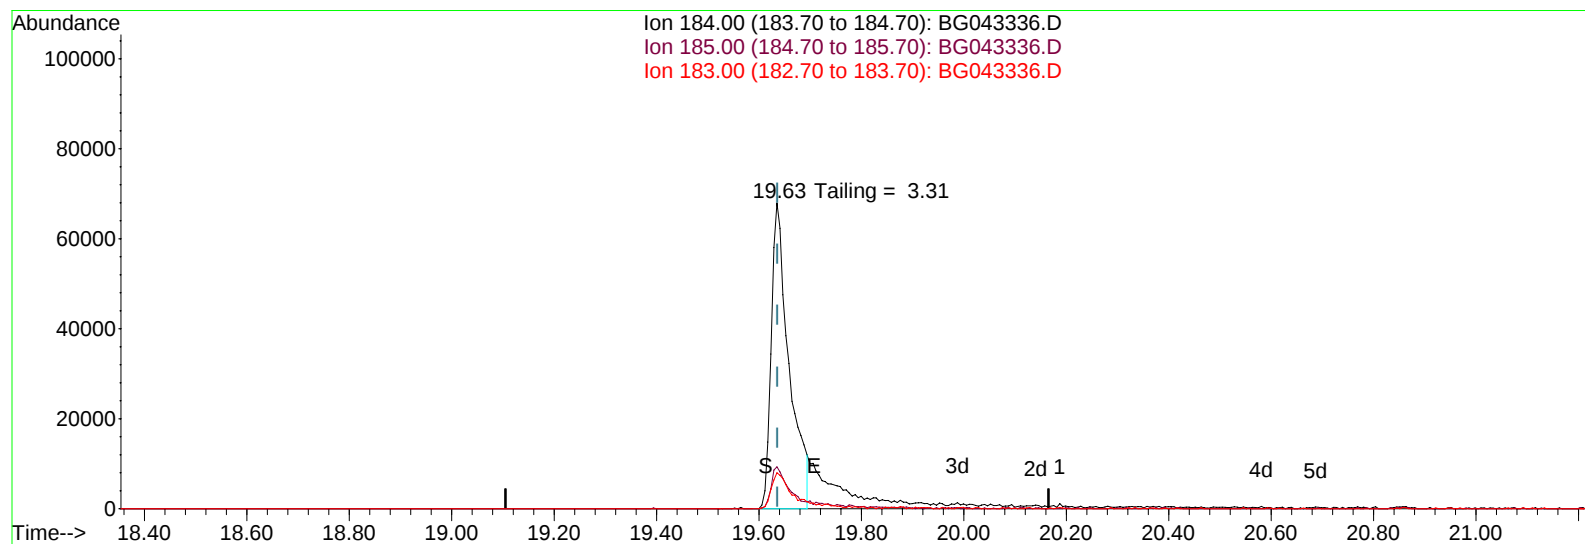

(77) Benzidine

20.187min (+0.552) 716.56ng

response 822

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	0.00#
183.00	13.30	22.67#
0.00	0.00	0.00