

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
 Data File : BG063494.D
 Acq On : 20 Nov 2024 21:38
 Operator : RC/JU
 Sample : P4903-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.272	27	31	41	rVB5	56558	138682	3.12%	0.415%
2	3.706	101	105	114	rBV	59799	107146	2.41%	0.320%
3	3.783	116	118	120	rVB3	8588	6314	0.14%	0.019%
4	4.030	157	160	163	rBV4	10818	13782	0.31%	0.041%
5	4.482	233	237	242	rVB4	10618	16379	0.37%	0.049%
6	4.564	246	251	260	rVB	70473	110178	2.48%	0.330%
7	4.970	316	320	323	rVB5	6381	10012	0.23%	0.030%
8	7.008	656	667	675	rBV	120232	234980	5.29%	0.703%
9	7.161	687	693	704	rVB	343560	560963	12.63%	1.678%
10	7.367	720	728	737	rBV	382748	658810	14.83%	1.971%
11	7.461	739	744	747	rVB4	6742	13544	0.30%	0.041%
12	7.831	798	807	814	rBV	322943	548200	12.34%	1.640%
13	7.890	814	817	822	rVB5	7081	12216	0.28%	0.037%
14	8.542	922	928	935	rBV2	337393	595949	13.42%	1.782%
15	8.595	935	937	940	rVB2	9951	10315	0.23%	0.031%
16	8.983	996	1003	1011	rBV	423699	755339	17.01%	2.259%
17	9.159	1029	1033	1035	rVB4	5656	6059	0.14%	0.018%
18	9.412	1072	1076	1078	rBV4	9004	7714	0.17%	0.023%
19	9.705	1118	1126	1136	rBV2	373829	694140	15.63%	2.076%
20	9.817	1142	1145	1149	rBV4	5328	8078	0.18%	0.024%
21	10.246	1212	1218	1233	rBV2	529626	994546	22.39%	2.975%
22	10.622	1272	1282	1289	rBV	421763	776687	17.49%	2.323%
23	10.757	1295	1305	1317	rBV	342586	673609	15.17%	2.015%
24	12.179	1544	1547	1550	rBV3	7911	9908	0.22%	0.030%
25	12.432	1586	1590	1593	rBV4	5620	9593	0.22%	0.029%
26	13.877	1828	1836	1848	rBV	1161521	1689169	38.03%	5.052%
27	14.112	1873	1876	1877	rBV2	6658	6121	0.14%	0.018%
28	14.165	1878	1885	1893	rVB	1152322	1851399	41.68%	5.538%
29	14.470	1931	1937	1946	rVB	742285	1148293	25.85%	3.435%
30	14.694	1970	1975	1986	rBV3	77927	174251	3.92%	0.521%
31	14.817	1994	1996	2002	rVB5	8563	12529	0.28%	0.037%
32	14.899	2007	2010	2015	rVB6	11073	18582	0.42%	0.056%
33	15.122	2043	2048	2051	rVB4	4061	6890	0.16%	0.021%
34	15.269	2071	2073	2075	rBV2	7427	8786	0.20%	0.026%
35	15.287	2075	2076	2080	rVB2	12102	13062	0.29%	0.039%
36	15.322	2080	2082	2084	rBV	7775	7065	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063494.D
Acq On : 20 Nov 2024 21:38
Operator : RC/JU
Sample : P4903-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Title : SVOA CALIBRATION

37	15.469	2099	2107	2115	rBV	1704777	2558592	57.61%	7.653%
38	15.593	2122	2128	2138	rBV	553233	860170	19.37%	2.573%
39	15.833	2162	2169	2174	rBV	67490	101284	2.28%	0.303%
40	16.174	2222	2227	2229	rBV5	10030	17322	0.39%	0.052%
41	16.374	2256	2261	2263	rBV5	4768	7507	0.17%	0.022%
42	16.550	2289	2291	2295	rVB4	7181	7853	0.18%	0.023%
43	16.985	2362	2365	2368	rBV4	11537	12169	0.27%	0.036%
44	17.144	2389	2392	2397	rVB4	18985	25255	0.57%	0.076%
45	17.226	2399	2406	2414	rBV	1033372	1576183	35.49%	4.714%
46	17.320	2416	2422	2432	rVB2	2072543	3237467	72.89%	9.683%
47	17.508	2451	2454	2457	rBV2	9286	12469	0.28%	0.037%
48	17.725	2486	2491	2493	rBV6	8451	10367	0.23%	0.031%
49	17.761	2495	2497	2500	rBV3	5524	6790	0.15%	0.020%
50	17.896	2518	2520	2524	rVB4	13252	11528	0.26%	0.034%
51	18.054	2546	2547	2553	rBV5	4696	6364	0.14%	0.019%
52	18.413	2606	2608	2609	rBV	11686	9152	0.21%	0.027%
53	18.554	2629	2632	2635	rVB4	9636	10656	0.24%	0.032%
54	18.883	2686	2688	2692	rBV4	5468	8145	0.18%	0.024%
55	19.047	2712	2716	2719	rBV5	7789	12024	0.27%	0.036%
56	19.188	2735	2740	2747	rVB3	40309	62180	1.40%	0.186%
57	19.259	2748	2752	2759	rVB2	31220	59212	1.33%	0.177%
58	19.335	2759	2765	2771	rBV2	52518	80783	1.82%	0.242%
59	19.453	2782	2785	2788	rBV5	7742	13473	0.30%	0.040%
60	19.535	2797	2799	2800	rBV2	9494	7824	0.18%	0.023%
61	19.623	2808	2814	2821	rBV	3128043	4286849	96.52%	12.822%
62	19.970	2871	2873	2875	rBV3	12203	9743	0.22%	0.029%
63	21.480	3124	3130	3138	rBV2	1210953	1973648	44.44%	5.903%
64	24.318	3603	3613	3630	rVB	1720930	4441448	100.00%	13.284%
65	24.523	3639	3648	3660	rVB2	793870	2097685	47.23%	6.274%




Sum of corrected areas: 33433432

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063494.D
Acq On : 20 Nov 2024 21:38
Operator : RC/JU
Sample : P4903-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

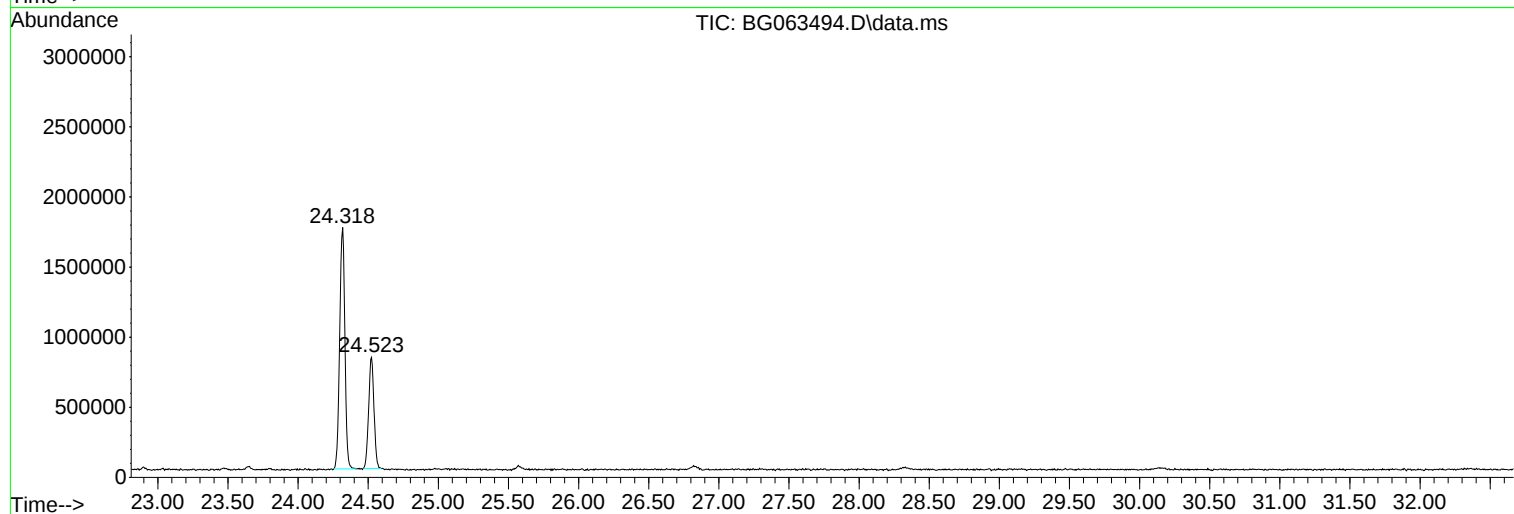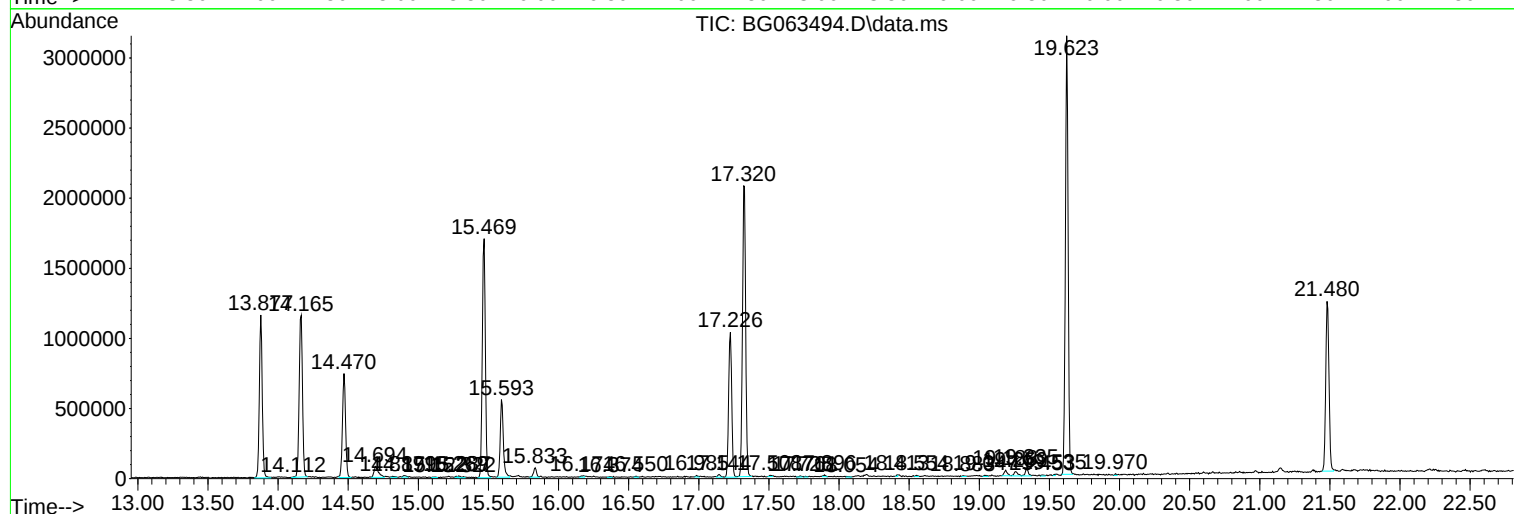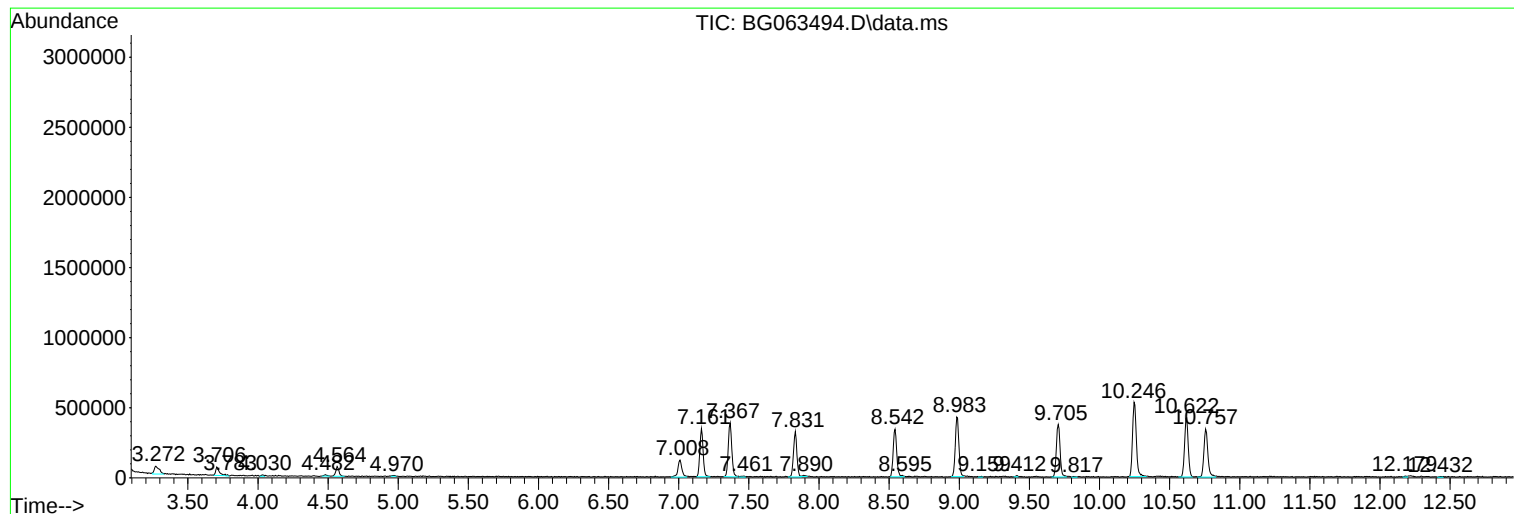

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063494.D
Acq On : 20 Nov 2024 21:38
Operator : RC/JU
Sample : P4903-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063494.D
Acq On : 20 Nov 2024 21:38
Operator : RC/JU
Sample : P4903-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc