

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
 Data File : BG063496.D
 Acq On : 20 Nov 2024 22:54
 Operator : RC/JU
 Sample : P4904-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG416

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.267	28	30	33	rBV3	11508	14233	0.33%	0.044%
2	3.297	33	35	39	rVB4	22215	21139	0.49%	0.065%
3	3.708	101	105	118	rVB	65000	129244	2.97%	0.399%
4	4.031	157	160	166	rBV4	15238	26356	0.61%	0.081%
5	4.566	247	251	256	rVB3	13461	18498	0.43%	0.057%
6	5.459	400	403	408	rBV4	6996	7242	0.17%	0.022%
7	6.475	573	576	578	rBV3	4567	6074	0.14%	0.019%
8	6.563	586	591	593	rBV4	5045	6033	0.14%	0.019%
9	7.010	656	667	677	rVB2	124782	242717	5.58%	0.749%
10	7.163	686	693	702	rVB	309484	524292	12.06%	1.617%
11	7.368	720	728	737	rBV	364896	650139	14.95%	2.006%
12	7.827	800	806	815	rBV	303480	528586	12.16%	1.631%
13	8.467	913	915	920	rBV2	3566	6489	0.15%	0.020%
14	8.538	920	927	935	rBV	387640	679260	15.62%	2.096%
15	8.743	956	962	965	rBV4	3712	7404	0.17%	0.023%
16	8.984	993	1003	1010	rBV	421147	729808	16.78%	2.252%
17	9.707	1116	1126	1134	rBV	372066	666558	15.33%	2.056%
18	10.247	1211	1218	1229	rBV	527572	968821	22.28%	2.989%
19	10.618	1272	1281	1290	rBV	414172	725746	16.69%	2.239%
20	10.759	1297	1305	1316	rBV	367790	720801	16.58%	2.224%
21	11.187	1375	1378	1382	rBV4	3741	6545	0.15%	0.020%
22	12.222	1547	1554	1557	rBV3	8909	15434	0.35%	0.048%
23	13.250	1727	1729	1733	rBV3	4439	6199	0.14%	0.019%
24	13.767	1811	1817	1818	rBV2	4477	5949	0.14%	0.018%
25	13.878	1829	1836	1849	rBV	1110394	1605337	36.92%	4.953%
26	14.160	1871	1884	1894	rBV2	1123798	1837814	42.27%	5.670%
27	14.472	1928	1937	1944	rBV	734228	1111216	25.56%	3.428%
28	14.695	1970	1975	1986	rBV3	78834	187195	4.31%	0.578%
29	14.907	2005	2011	2015	rBV7	5182	13290	0.31%	0.041%
30	15.212	2061	2063	2071	rVB6	6505	10088	0.23%	0.031%
31	15.471	2100	2107	2113	rBV	1600097	2458675	56.54%	7.585%
32	15.594	2122	2128	2136	rBV	547298	846159	19.46%	2.610%
33	15.706	2144	2147	2154	rVB7	13268	23829	0.55%	0.074%
34	15.970	2188	2192	2193	rBV3	6776	8051	0.19%	0.025%
35	16.170	2221	2226	2229	rBV5	5749	9544	0.22%	0.029%
36	16.722	2315	2320	2323	rVB4	6168	9521	0.22%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063496.D
Acq On : 20 Nov 2024 22:54
Operator : RC/JU
Sample : P4904-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG416

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Title : SVOA CALIBRATION

37	17.092	2378	2383	2385	rVB3	6594	9808	0.23%	0.030%
38	17.222	2399	2405	2414	rBV	1020851	1522575	35.02%	4.697%
39	17.321	2416	2422	2430	rVV	2095447	3172086	72.95%	9.786%
40	17.615	2469	2472	2477	rBV6	6529	8917	0.21%	0.028%
41	18.726	2660	2661	2667	rVB6	5146	6496	0.15%	0.020%
42	19.184	2734	2739	2745	rBV2	37659	62439	1.44%	0.193%
43	19.260	2748	2752	2758	rVV2	32149	53109	1.22%	0.164%
44	19.337	2762	2765	2770	rVB5	33028	43568	1.00%	0.134%
45	19.548	2799	2801	2805	rBV5	9053	9019	0.21%	0.028%
46	19.625	2807	2814	2821	rBV	3028440	4251909	97.78%	13.117%
47	20.042	2883	2885	2888	rBV4	9964	9999	0.23%	0.031%
48	21.481	3124	3130	3138	rBV2	1254261	1969431	45.29%	6.076%
49	24.319	3602	3613	3626	rBV	1666275	4348236	100.00%	13.415%
50	24.525	3639	3648	3661	rVB2	792703	2112404	48.58%	6.517%




Sum of corrected areas: 32414282

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063496.D
Acq On : 20 Nov 2024 22:54
Operator : RC/JU
Sample : P4904-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

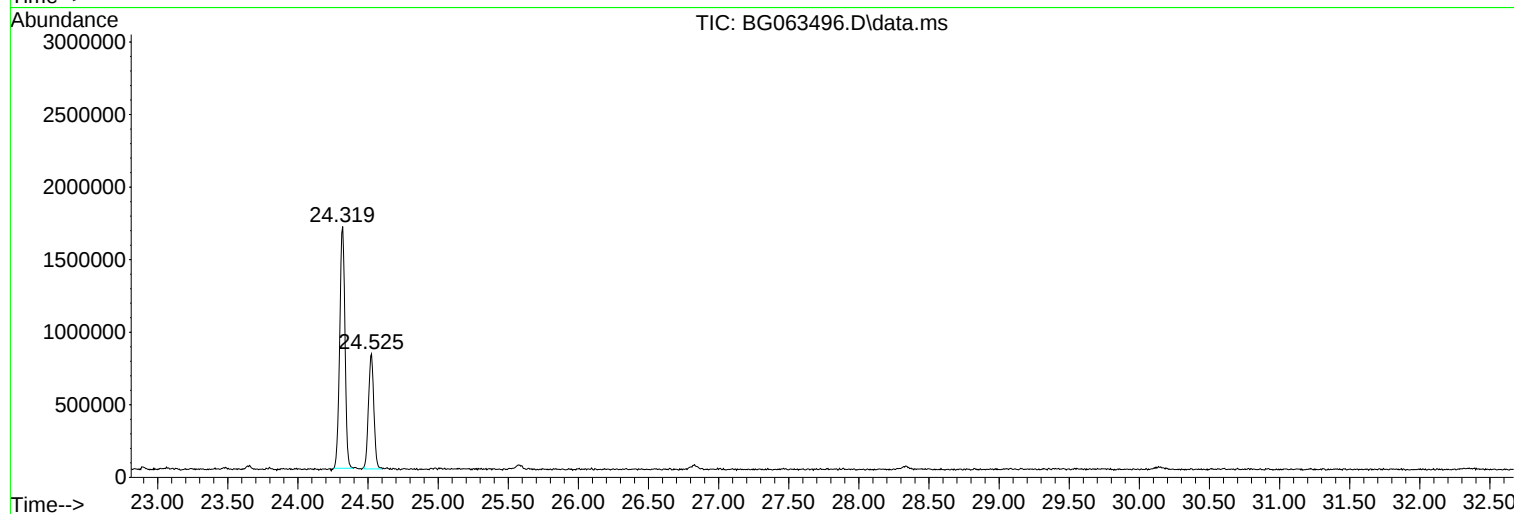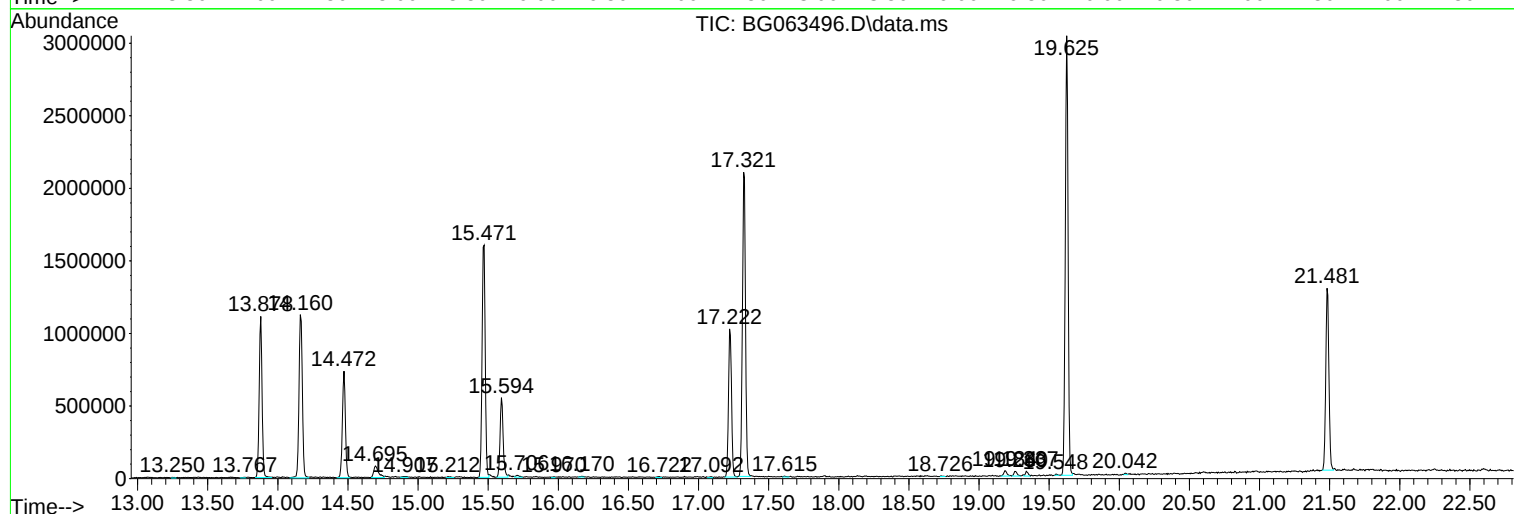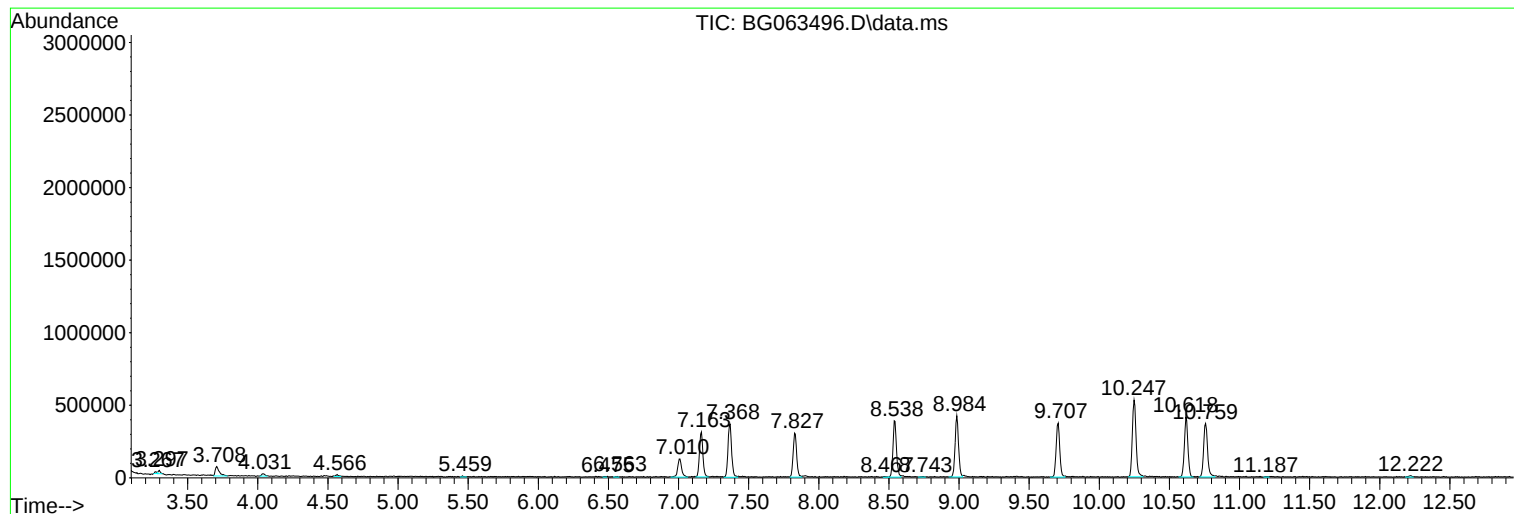

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063496.D
Acq On : 20 Nov 2024 22:54
Operator : RC/JU
Sample : P4904-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG112024\
Data File : BG063496.D
Acq On : 20 Nov 2024 22:54
Operator : RC/JU
Sample : P4904-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG112024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc