

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047467.D
 Acq On : 25 Nov 2020 14:18
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL01
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.444	16	18	19	rBV2	2864	2111	0.16%	0.016%
2	3.503	26	28	29	rBV	2183	2043	0.15%	0.016%
3	3.603	41	45	50	rBV4	9723	16596	1.25%	0.127%
4	3.985	108	110	114	rVB3	3032	2938	0.22%	0.022%
5	4.032	116	118	134	rVV2	114544	224885	16.92%	1.720%
6	4.384	175	178	180	rBV2	3986	3612	0.27%	0.028%
7	4.513	197	200	201	rBV2	2740	2406	0.18%	0.018%
8	4.566	208	209	213	rBV2	2102	2207	0.17%	0.017%
9	4.637	219	221	225	rBV	2127	2761	0.21%	0.021%
10	4.890	262	264	268	rVB	2082	2152	0.16%	0.016%
11	5.213	318	319	324	rVB3	2870	2723	0.20%	0.021%
12	5.266	326	328	330	rBV	2629	2524	0.19%	0.019%
13	5.324	335	338	340	rVB2	2144	1871	0.14%	0.014%
14	5.348	340	342	345	rBV	2094	2617	0.20%	0.020%
15	5.624	385	389	392	rVB	1538	2805	0.21%	0.021%
16	6.159	477	480	483	rBV2	1393	1847	0.14%	0.014%
17	6.823	590	593	596	rBV2	2020	2399	0.18%	0.018%
18	7.316	673	677	678	rBV	1710	2045	0.15%	0.016%
19	7.398	683	691	699	rBV	214036	379261	28.53%	2.901%
20	7.492	706	707	711	rVB2	2125	1920	0.14%	0.015%
21	7.575	714	721	731	rVB	125391	217337	16.35%	1.662%
22	7.792	750	758	767	rBV	211804	367417	27.64%	2.810%
23	8.227	828	832	833	rBV2	1856	1833	0.14%	0.014%
24	8.268	833	839	849	rVB	123370	223373	16.80%	1.709%
25	8.638	900	902	905	rVB2	2885	1978	0.15%	0.015%
26	8.820	931	933	937	rBV	2343	2121	0.16%	0.016%
27	8.955	949	956	966	rVB	254723	433157	32.59%	3.313%
28	9.132	984	986	989	rBV	1819	2227	0.17%	0.017%
29	9.237	1002	1004	1011	rVB	1692	2261	0.17%	0.017%
30	9.431	1030	1037	1045	rBV	200281	365273	27.48%	2.794%
31	9.572	1057	1061	1062	rBV2	2267	2116	0.16%	0.016%
32	9.596	1062	1065	1069	rVB2	1795	2552	0.19%	0.020%
33	10.160	1153	1161	1169	rBV2	188667	344964	25.95%	2.639%
34	10.236	1171	1174	1176	rVB2	1636	2032	0.15%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047467.D
 Acq On : 25 Nov 2020 14:18
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL01
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	10.430	1201	1207	1208	rVB	1216	1922	0.14%	0.015%
36	10.489	1214	1217	1219	rVB2	1942	2211	0.17%	0.017%
37	10.700	1245	1253	1261	rBV	265503	489953	36.86%	3.748%
38	10.971	1295	1299	1301	rBV	2586	2623	0.20%	0.020%
39	11.094	1312	1320	1327	rBV	156970	280098	21.07%	2.142%
40	11.217	1333	1341	1352	rVB	231525	433685	32.63%	3.317%
41	11.388	1366	1370	1371	rVB	1866	2002	0.15%	0.015%
42	11.588	1402	1404	1408	rVB2	2330	2077	0.16%	0.016%
43	11.758	1432	1433	1437	rBV	1976	2260	0.17%	0.017%
44	12.210	1507	1510	1513	rBV2	1947	2319	0.17%	0.018%
45	12.475	1553	1555	1559	rVB	2092	2430	0.18%	0.019%
46	12.663	1580	1587	1593	rVB	4199	8071	0.61%	0.062%
47	13.568	1739	1741	1744	rVB	2312	2070	0.16%	0.016%
48	13.873	1790	1793	1797	rVB2	2088	2082	0.16%	0.016%
49	14.273	1855	1861	1869	rVV	515843	745237	56.06%	5.700%
50	14.331	1869	1871	1873	rVB	2538	1801	0.14%	0.014%
51	14.578	1906	1913	1921	rVB	497549	768946	57.85%	5.881%
52	14.878	1958	1964	1972	rVB	259270	411355	30.95%	3.146%
53	15.042	1983	1992	2008	rBV2	232537	440513	33.14%	3.369%
54	15.360	2043	2046	2049	rVV	1360	1921	0.14%	0.015%
55	15.553	2076	2079	2081	rBV	2092	1849	0.14%	0.014%
56	15.648	2094	2095	2098	rVB	2517	1800	0.14%	0.014%
57	15.794	2118	2120	2123	rBV	1529	1857	0.14%	0.014%
58	15.865	2123	2132	2143	rBV	635640	964329	72.55%	7.376%
59	15.965	2143	2149	2157	rBV2	188846	297397	22.37%	2.275%
60	16.106	2168	2173	2180	rVB4	7720	13486	1.01%	0.103%
61	16.165	2180	2183	2185	rBV	2484	2228	0.17%	0.017%
62	16.259	2194	2199	2201	rBV	2792	3228	0.24%	0.025%
63	16.629	2260	2262	2265	rBV	2583	3350	0.25%	0.026%
64	16.699	2272	2274	2277	rVB	2412	2013	0.15%	0.015%
65	16.723	2277	2278	2281	rBV	1676	2022	0.15%	0.015%
66	16.840	2297	2298	2302	rVB	3038	2334	0.18%	0.018%
67	16.887	2302	2306	2308	rBV	1935	2162	0.16%	0.017%
68	16.987	2319	2323	2327	rVB2	1578	2680	0.20%	0.020%
69	17.075	2335	2338	2339	rBV2	2217	1876	0.14%	0.014%
70	17.105	2341	2343	2346	rVB	2912	2267	0.17%	0.017%
71	17.287	2370	2374	2378	rVB3	4098	6338	0.48%	0.048%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047467.D
 Acq On : 25 Nov 2020 14:18
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL01
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

72	17.616	2423	2430	2438	rVB	358043	555877	41.82%	4.252%
73	17.716	2440	2447	2455	rVV2	721331	1123395	84.51%	8.593%
74	17.774	2455	2457	2460	rVB3	2882	2202	0.17%	0.017%
75	17.845	2467	2469	2471	rBV	1869	2157	0.16%	0.016%
76	17.886	2474	2476	2479	rVB	2675	2940	0.22%	0.022%
77	18.115	2511	2515	2516	rBV	2479	2616	0.20%	0.020%
78	18.145	2519	2520	2523	rBV	2101	1853	0.14%	0.014%
79	18.344	2548	2554	2555	rBV	1571	2096	0.16%	0.016%
80	18.362	2555	2557	2561	rBV	2726	3251	0.24%	0.025%
81	18.620	2599	2601	2604	rBV3	2486	2102	0.16%	0.016%
82	18.861	2640	2642	2643	rVB	3704	2075	0.16%	0.016%
83	18.879	2643	2645	2650	rVV3	2742	4414	0.33%	0.034%
84	18.944	2653	2656	2659	rVV2	4537	4648	0.35%	0.036%
85	18.967	2659	2660	2663	rVB2	4657	3470	0.26%	0.027%
86	19.102	2680	2683	2685	rBV3	2056	1953	0.15%	0.015%
87	19.138	2687	2689	2691	rVB2	3331	2356	0.18%	0.018%
88	19.290	2713	2715	2718	rBV2	4705	4596	0.35%	0.035%
89	19.584	2763	2765	2766	rBV2	3748	2505	0.19%	0.019%
90	19.608	2767	2769	2777	rVB3	8724	13867	1.04%	0.106%
91	19.719	2786	2788	2790	rBV3	2571	2222	0.17%	0.017%
92	19.872	2810	2814	2818	rVB3	10101	17534	1.32%	0.134%
93	19.931	2822	2824	2825	rVB	5337	2973	0.22%	0.023%
94	19.978	2826	2832	2842	rVV	868342	1329282	100.00%	10.167%
95	20.113	2853	2855	2858	rVB4	4437	3259	0.25%	0.025%
96	20.177	2864	2866	2868	rBV2	5070	4488	0.34%	0.034%
97	21.899	3152	3159	3166	rBV	360139	610738	45.94%	4.671%
98	25.066	3689	3698	3709	rVB	407883	1217246	91.57%	9.310%
99	25.301	3729	3738	3753	rVB	187647	597518	44.95%	4.570%
100	31.652	4818	4819	4821	rBV2	10429	5221	0.39%	0.040%


Sum of corrected areas: 13074010

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
Data File : BG047467.D
Acq On : 25 Nov 2020 14:18
Operator : CG/JU
Sample : PB133233BL
Misc : MDL-WATER-BL01
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

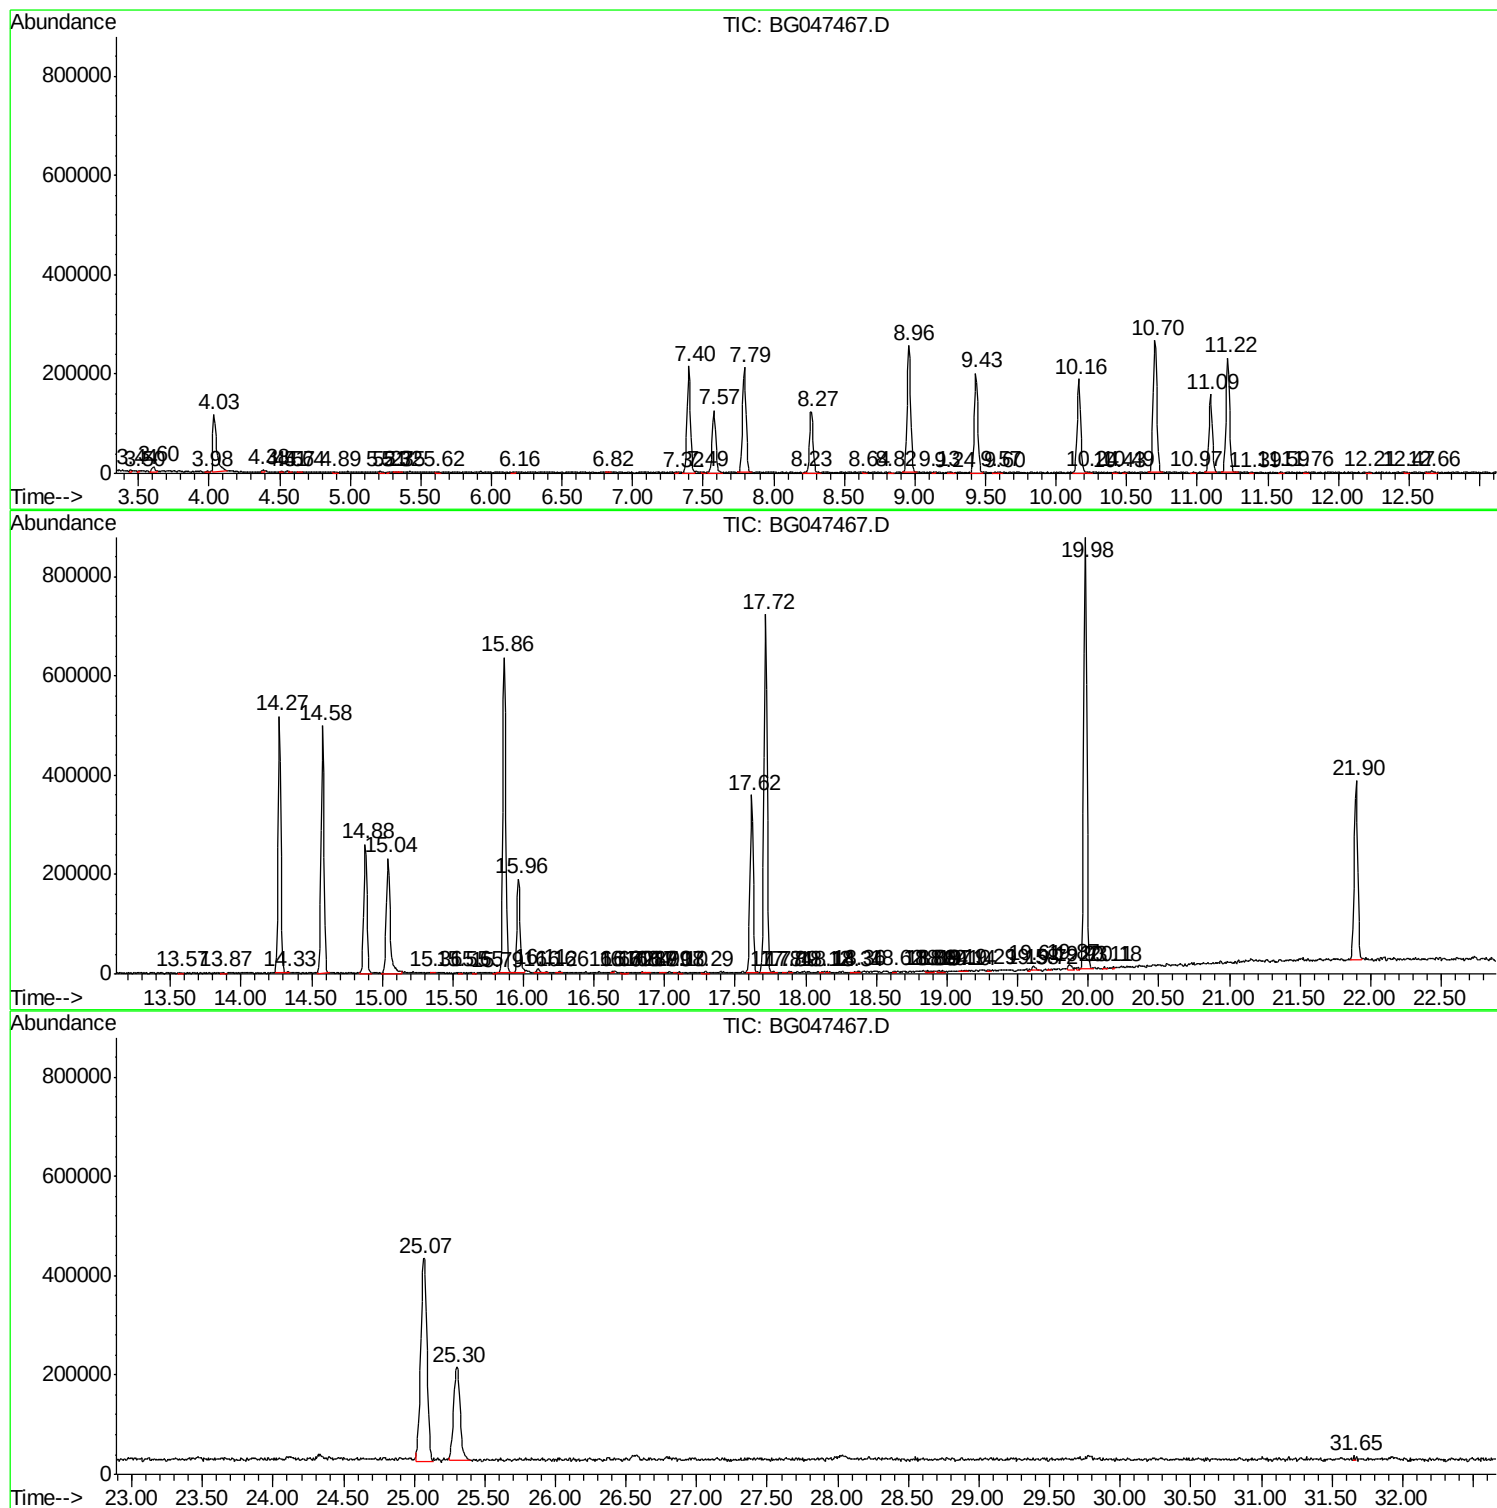

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112520\
Data_File : BG047467.D
Acq_On : 25 Nov 2020 14:188
Operator : CG/JUU
Sample : PB133233BLL
Misc : MDL-WATER-BL011
ALS_Vial : 3 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
