

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047469.D
 Acq On : 25 Nov 2020 15:39
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL02
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.613	43	47	52	rBV4	7620	14023	0.97%	0.103%
2	3.666	54	56	58	rBV2	2406	2638	0.18%	0.019%
3	4.042	116	120	133	rBV	134481	245990	16.96%	1.803%
4	4.189	143	145	148	rVB	2007	2019	0.14%	0.015%
5	4.342	169	171	173	rBV	2425	1926	0.13%	0.014%
6	4.395	175	180	183	rVV4	5202	8802	0.61%	0.065%
7	4.460	187	191	192	rVB	2039	2323	0.16%	0.017%
8	4.753	239	241	244	rVB2	2081	2116	0.15%	0.016%
9	4.818	248	252	255	rVB2	2108	3116	0.21%	0.023%
10	5.253	323	326	328	rBV2	2226	2687	0.19%	0.020%
11	5.511	364	370	373	rBV	2074	3905	0.27%	0.029%
12	5.688	397	400	402	rBV2	2006	2080	0.14%	0.015%
13	6.169	478	482	483	rVB2	2208	2231	0.15%	0.016%
14	6.275	497	500	503	rVB2	1768	1961	0.14%	0.014%
15	6.563	546	549	552	rBV2	2617	2489	0.17%	0.018%
16	6.963	614	617	619	rBV	2023	2072	0.14%	0.015%
17	7.403	683	692	699	rBV	224304	405405	27.95%	2.972%
18	7.579	715	722	730	rBV	131805	231522	15.96%	1.697%
19	7.791	752	758	767	rVB2	212064	389571	26.85%	2.856%
20	7.908	776	778	785	rVB2	2147	3255	0.22%	0.024%
21	7.961	785	787	789	rBV	1915	1956	0.13%	0.014%
22	8.020	793	797	799	rBV	1912	2384	0.16%	0.017%
23	8.267	832	839	847	rBV	121061	204800	14.12%	1.501%
24	8.326	847	849	852	rVB	2328	2112	0.15%	0.015%
25	8.408	861	863	867	rBV	1405	1892	0.13%	0.014%
26	8.549	884	887	890	rBV	2159	2872	0.20%	0.021%
27	8.960	949	957	966	rBV2	259467	470325	32.42%	3.447%
28	9.219	997	1001	1004	rBV2	2148	2816	0.19%	0.021%
29	9.436	1030	1038	1047	rBV	212235	387728	26.73%	2.842%
30	9.771	1093	1095	1098	rBV	1592	2081	0.14%	0.015%
31	10.024	1136	1138	1142	rVB	1568	1908	0.13%	0.014%
32	10.159	1155	1161	1170	rBV2	200118	377476	26.02%	2.767%
33	10.400	1200	1202	1206	rVB2	1873	1970	0.14%	0.014%
34	10.699	1245	1253	1261	rBV	278563	522513	36.02%	3.830%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047469.D
 Acq On : 25 Nov 2020 15:39
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL02
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	10.758	1261	1263	1265	rVB	3017	2485	0.17%	0.018%
36	10.793	1265	1269	1274	rVB	1842	2554	0.18%	0.019%
37	10.852	1276	1279	1282	rBV	1989	2589	0.18%	0.019%
38	11.093	1312	1320	1328	rVB	141128	258765	17.84%	1.897%
39	11.216	1332	1341	1350	rBV	256052	472239	32.55%	3.461%
40	11.592	1402	1405	1408	rBV	2091	2204	0.15%	0.016%
41	12.315	1524	1528	1530	rBV2	1623	2454	0.17%	0.018%
42	12.644	1581	1584	1585	rBV	3204	3141	0.22%	0.023%
43	12.656	1585	1586	1592	rVB3	5211	5857	0.40%	0.043%
44	12.803	1608	1611	1612	rBV3	2552	2232	0.15%	0.016%
45	13.243	1681	1686	1689	rBV	1692	2876	0.20%	0.021%
46	14.207	1849	1850	1852	rBV	2237	1970	0.14%	0.014%
47	14.272	1855	1861	1868	rVV	551268	807838	55.69%	5.921%
48	14.577	1906	1913	1920	rBV2	519587	828539	57.11%	6.073%
49	14.877	1956	1964	1972	rBV	229269	381724	26.31%	2.798%
50	14.988	1980	1983	1985	rBV	2412	2499	0.17%	0.018%
51	15.041	1985	1992	2000	rBV	263741	444470	30.64%	3.258%
52	15.317	2036	2039	2041	rVB	1707	1971	0.14%	0.014%
53	15.717	2104	2107	2110	rBV	2449	3507	0.24%	0.026%
54	15.864	2124	2132	2141	rBV	667344	1034958	71.34%	7.586%
55	15.964	2143	2149	2158	rVV	227151	340377	23.46%	2.495%
56	16.046	2161	2163	2166	rBV	2607	1931	0.13%	0.014%
57	16.099	2166	2172	2178	rVB6	10325	17341	1.20%	0.127%
58	16.152	2178	2181	2182	rBV6	2398	2047	0.14%	0.015%
59	16.540	2245	2247	2251	rVB	1672	2163	0.15%	0.016%
60	16.575	2251	2253	2256	rBV	1965	2051	0.14%	0.015%
61	16.634	2260	2263	2265	rBV	3253	3144	0.22%	0.023%
62	16.763	2282	2285	2288	rBV	1788	2974	0.21%	0.022%
63	17.104	2340	2343	2346	rVB	1906	2282	0.16%	0.017%
64	17.297	2372	2376	2377	rBV	2118	1956	0.13%	0.014%
65	17.615	2423	2430	2436	rVB	329747	504528	34.78%	3.698%
66	17.715	2440	2447	2455	rVV	776214	1187986	81.89%	8.708%
67	17.791	2459	2460	2467	rVB	2091	2871	0.20%	0.021%
68	17.838	2467	2468	2472	rBV3	2231	2965	0.20%	0.022%
69	17.920	2479	2482	2483	rBV2	3197	3196	0.22%	0.023%
70	17.973	2489	2491	2494	rBV2	2085	1958	0.13%	0.014%
71	18.243	2534	2537	2538	rBV2	2827	1894	0.13%	0.014%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047469.D
 Acq On : 25 Nov 2020 15:39
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL02
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

72	18.379	2558	2560	2562	rVB	2777	1993	0.14%	0.015%
73	18.514	2581	2583	2585	rBV3	2598	2219	0.15%	0.016%
74	18.549	2588	2589	2592	rBV	3294	3152	0.22%	0.023%
75	18.637	2602	2604	2606	rVB3	3124	2604	0.18%	0.019%
76	18.702	2609	2615	2619	rBV	3675	8288	0.57%	0.061%
77	19.007	2666	2667	2669	rBV2	3531	2385	0.16%	0.017%
78	19.084	2678	2680	2682	rBV3	2870	2552	0.18%	0.019%
79	19.248	2705	2708	2710	rBV3	1964	2269	0.16%	0.017%
80	19.301	2716	2717	2720	rVB2	3397	2270	0.16%	0.017%
81	19.424	2736	2738	2741	rBV3	3383	2432	0.17%	0.018%
82	19.530	2755	2756	2759	rBV2	2603	3051	0.21%	0.022%
83	19.618	2766	2771	2775	rBV2	8745	13735	0.95%	0.101%
84	19.753	2793	2794	2796	rBV2	4283	2805	0.19%	0.021%
85	19.865	2809	2813	2818	rBV4	11805	19229	1.33%	0.141%
86	19.977	2826	2832	2840	rBV2	968203	1450663	100.00%	10.633%
87	20.159	2861	2863	2866	rVB3	3062	2211	0.15%	0.016%
88	20.182	2866	2867	2869	rBV2	3473	3038	0.21%	0.022%
89	20.300	2885	2887	2889	rBV3	5312	5489	0.38%	0.040%
90	21.898	3152	3159	3167	rVB	319877	593448	40.91%	4.350%
91	25.065	3688	3698	3709	rVB	446157	1306035	90.03%	9.573%
92	25.300	3728	3738	3751	rVB2	172307	545034	37.57%	3.995%
93	27.415	4096	4098	4101	rBV4	8497	8254	0.57%	0.061%


Sum of corrected areas: 13642656

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
Data File : BG047469.D
Acq On : 25 Nov 2020 15:39
Operator : CG/JU
Sample : PB133233BL
Misc : MDL-WATER-BL02
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

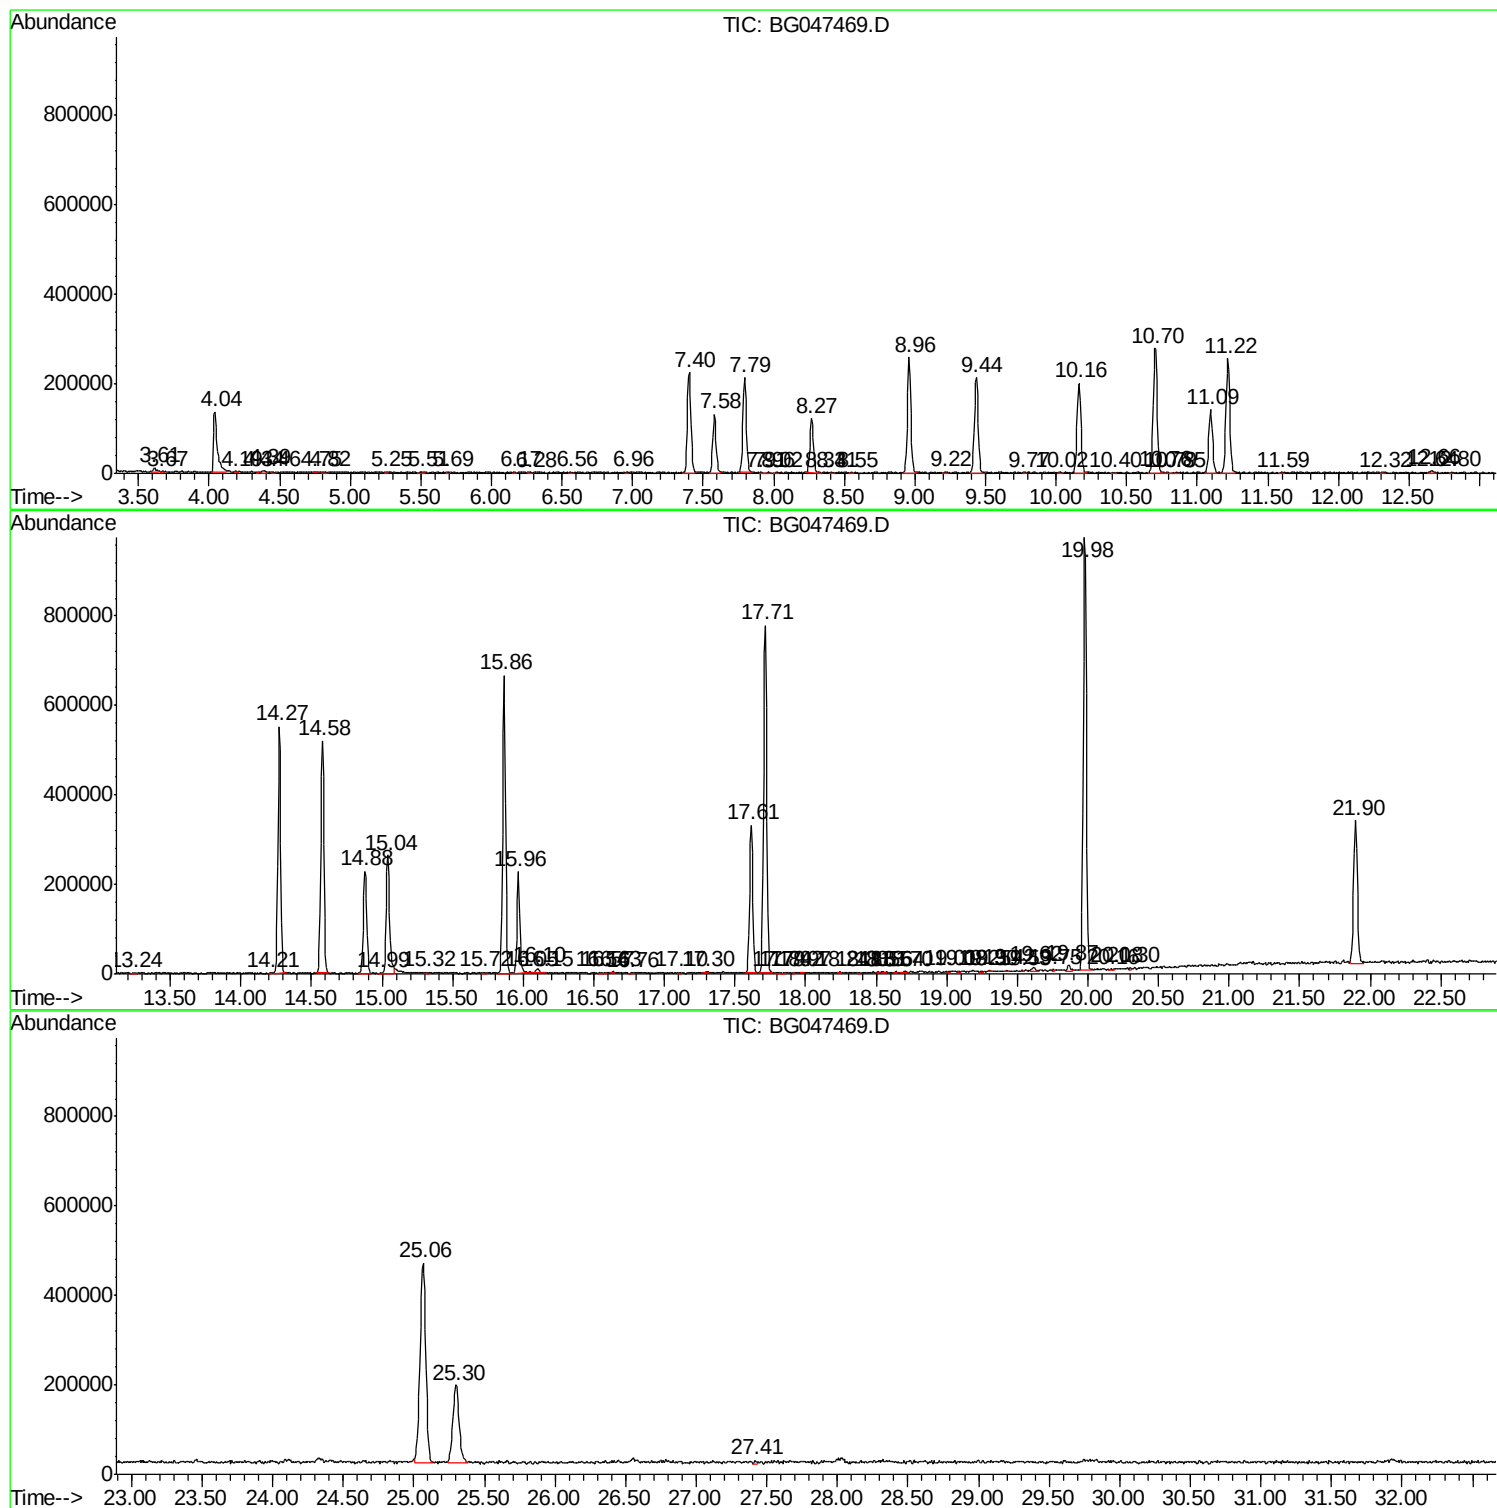

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112520\
Data_File : BG047469.D
Acq_On : 25 Nov 2020 15:399
Operator : CG/JUU
Sample : PB133233BLL
Misc : MDL-WATER-BL022
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
