

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047471.D
 Acq On : 25 Nov 2020 17:00
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL03
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.397	8	10	13	rBV3	1686	2219	0.16%	0.016%
2	3.468	19	22	23	rBV2	2740	2421	0.17%	0.018%
3	3.603	42	45	50	rBV6	7362	12735	0.89%	0.093%
4	3.791	76	77	81	rVB	2425	1992	0.14%	0.015%
5	4.038	115	119	131	rBV	132074	236636	16.60%	1.726%
6	4.196	145	146	149	rVB2	3034	2638	0.19%	0.019%
7	4.231	149	152	154	rBV2	2935	3098	0.22%	0.023%
8	4.384	175	178	182	rBV3	3971	5699	0.40%	0.042%
9	4.466	186	192	194	rBV	1765	2205	0.15%	0.016%
10	4.813	249	251	253	rBV	2358	1850	0.13%	0.013%
11	4.860	255	259	262	rVV2	1824	3030	0.21%	0.022%
12	4.942	271	273	276	rVB2	1847	1992	0.14%	0.015%
13	5.171	309	312	317	rBV	1805	2419	0.17%	0.018%
14	5.401	348	351	354	rBV	2145	2311	0.16%	0.017%
15	5.606	384	386	390	rBV	2152	2409	0.17%	0.018%
16	5.824	419	423	424	rBV	2193	2006	0.14%	0.015%
17	5.929	438	441	444	rBV	1716	2157	0.15%	0.016%
18	5.976	446	449	451	rBV	2569	1909	0.13%	0.014%
19	6.570	547	550	551	rBV	2281	2042	0.14%	0.015%
20	6.881	598	603	604	rBV	1702	2032	0.14%	0.015%
21	7.110	639	642	643	rBV	2560	2329	0.16%	0.017%
22	7.234	659	663	665	rBV	2724	3167	0.22%	0.023%
23	7.351	680	683	684	rBV	2201	1899	0.13%	0.014%
24	7.398	684	691	703	rVB	207405	390146	27.38%	2.845%
25	7.580	715	722	730	rBV	129811	229832	16.13%	1.676%
26	7.710	739	744	745	rBV	2565	2045	0.14%	0.015%
27	7.792	747	758	767	rVV	218404	388407	27.25%	2.833%
28	7.880	770	773	775	rBV	1489	1825	0.13%	0.013%
29	8.097	809	810	813	rBV	1909	2066	0.14%	0.015%
30	8.268	833	839	846	rBV	126956	214184	15.03%	1.562%
31	8.368	853	856	859	rBV	1845	1857	0.13%	0.014%
32	8.955	946	956	965	rBV	254495	462375	32.44%	3.372%
33	9.108	981	982	985	rBV	2237	1984	0.14%	0.014%
34	9.437	1030	1038	1045	rBV	205001	386952	27.15%	2.822%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047471.D
 Acq On : 25 Nov 2020 17:00
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL03
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

35	9.531	1051	1054	1057	rBV	2312	2886	0.20%	0.021%
36	10.160	1154	1161	1171	rVB2	208140	377210	26.47%	2.751%
37	10.700	1246	1253	1260	rBV	282013	514988	36.14%	3.756%
38	10.753	1260	1262	1267	rVB	1818	2180	0.15%	0.016%
39	11.094	1312	1320	1327	rVB	151567	276161	19.38%	2.014%
40	11.217	1334	1341	1351	rVV	252679	463876	32.55%	3.383%
41	11.294	1351	1354	1358	rVV	1970	3010	0.21%	0.022%
42	11.341	1358	1362	1367	rVB	1739	3077	0.22%	0.022%
43	11.864	1448	1451	1453	rBV	1616	1907	0.13%	0.014%
44	12.275	1519	1521	1525	rVB	1991	1869	0.13%	0.014%
45	12.340	1529	1532	1534	rVB	1821	1907	0.13%	0.014%
46	12.657	1580	1586	1591	rBV2	5269	11065	0.78%	0.081%
47	12.810	1610	1612	1615	rBV2	1408	1899	0.13%	0.014%
48	13.203	1675	1679	1682	rBV2	1956	1847	0.13%	0.013%
49	13.509	1730	1731	1736	rBV2	2199	2510	0.18%	0.018%
50	13.967	1807	1809	1812	rBV	2188	1829	0.13%	0.013%
51	14.273	1854	1861	1868	rVB	570770	803760	56.40%	5.862%
52	14.390	1876	1881	1884	rVB	2365	2643	0.19%	0.019%
53	14.578	1906	1913	1920	rBV	525411	822521	57.71%	5.999%
54	14.796	1948	1950	1953	rBV	1405	1943	0.14%	0.014%
55	14.878	1958	1964	1973	rVB2	249753	405898	28.48%	2.960%
56	15.042	1985	1992	2006	rBV	251914	448450	31.47%	3.271%
57	15.177	2014	2015	2017	rBV	3065	1936	0.14%	0.014%
58	15.271	2029	2031	2036	rVB	2481	3695	0.26%	0.027%
59	15.424	2055	2057	2060	rBV	1900	2069	0.15%	0.015%
60	15.477	2063	2066	2068	rBV	2066	2249	0.16%	0.016%
61	15.806	2121	2122	2124	rBV	2518	1841	0.13%	0.013%
62	15.865	2125	2132	2139	rVV	669744	1029879	72.26%	7.511%
63	15.965	2143	2149	2162	rVV	226436	349225	24.50%	2.547%
64	16.100	2169	2172	2177	rVB4	10434	12349	0.87%	0.090%
65	16.182	2184	2186	2188	rBV4	2307	1843	0.13%	0.013%
66	16.317	2208	2209	2215	rVB4	1757	1931	0.14%	0.014%
67	16.640	2259	2264	2266	rBV	5144	5816	0.41%	0.042%
68	16.729	2276	2279	2281	rBV	2826	2835	0.20%	0.021%
69	16.770	2284	2286	2288	rBV	2086	2034	0.14%	0.015%
70	16.858	2298	2301	2303	rBV	2033	2220	0.16%	0.016%
71	16.905	2306	2309	2312	rVB	2316	3592	0.25%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
 Data File : BG047471.D
 Acq On : 25 Nov 2020 17:00
 Operator : CG/JU
 Sample : PB133233BL
 Misc : MDL-WATER-BL03
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK233

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
 Title : SVOA CALIBRATION

72	17.210	2360	2361	2363	rBV	2589	1867	0.13%	0.014%
73	17.293	2373	2375	2376	rBV	3178	2272	0.16%	0.017%
74	17.410	2393	2395	2397	rVB	2513	1919	0.13%	0.014%
75	17.545	2415	2418	2420	rVB	1492	1932	0.14%	0.014%
76	17.616	2423	2430	2437	rVV	351484	537100	37.69%	3.917%
77	17.716	2439	2447	2457	rVV2	747808	1180494	82.83%	8.610%
78	17.845	2465	2469	2470	rVB	2420	2920	0.20%	0.021%
79	17.874	2472	2474	2477	rVB	2477	2708	0.19%	0.020%
80	18.003	2494	2496	2502	rVB	2634	3084	0.22%	0.022%
81	18.268	2538	2541	2544	rBV	1814	2435	0.17%	0.018%
82	18.732	2615	2620	2621	rBV2	2380	2401	0.17%	0.018%
83	18.808	2632	2633	2639	rVB	2901	3597	0.25%	0.026%
84	18.914	2644	2651	2652	rBV5	2640	4259	0.30%	0.031%
85	19.102	2681	2683	2688	rBV	2148	3312	0.23%	0.024%
86	19.537	2755	2757	2759	rBV2	3046	1832	0.13%	0.013%
87	19.555	2759	2760	2763	rVV2	2851	1958	0.14%	0.014%
88	19.613	2767	2770	2778	rVV2	8119	13906	0.98%	0.101%
89	19.696	2782	2784	2788	rBV4	2823	3344	0.23%	0.024%
90	19.831	2805	2807	2808	rBV	3053	2165	0.15%	0.016%
91	19.860	2810	2812	2819	rVB3	9418	16990	1.19%	0.124%
92	19.978	2825	2832	2842	rBV	944560	1425158	100.00%	10.394%
93	20.060	2845	2846	2848	rBV2	3793	1992	0.14%	0.015%
94	20.148	2859	2861	2862	rBV2	3391	1863	0.13%	0.014%
95	20.213	2870	2872	2876	rBV4	4291	6227	0.44%	0.045%
96	20.342	2892	2894	2895	rBV2	3987	2980	0.21%	0.022%
97	21.893	3152	3158	3167	rVB	356979	623412	43.74%	4.547%
98	22.786	3308	3310	3312	rBV3	7071	5833	0.41%	0.043%
99	25.066	3688	3698	3709	rVB2	443652	1289658	90.49%	9.406%
100	25.295	3728	3737	3754	rVB3	193965	603866	42.37%	4.404%


Sum of corrected areas: 13711302

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG112520\
Data File : BG047471.D
Acq On : 25 Nov 2020 17:00
Operator : CG/JU
Sample : PB133233BL
Misc : MDL-WATER-BL03
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG111820.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

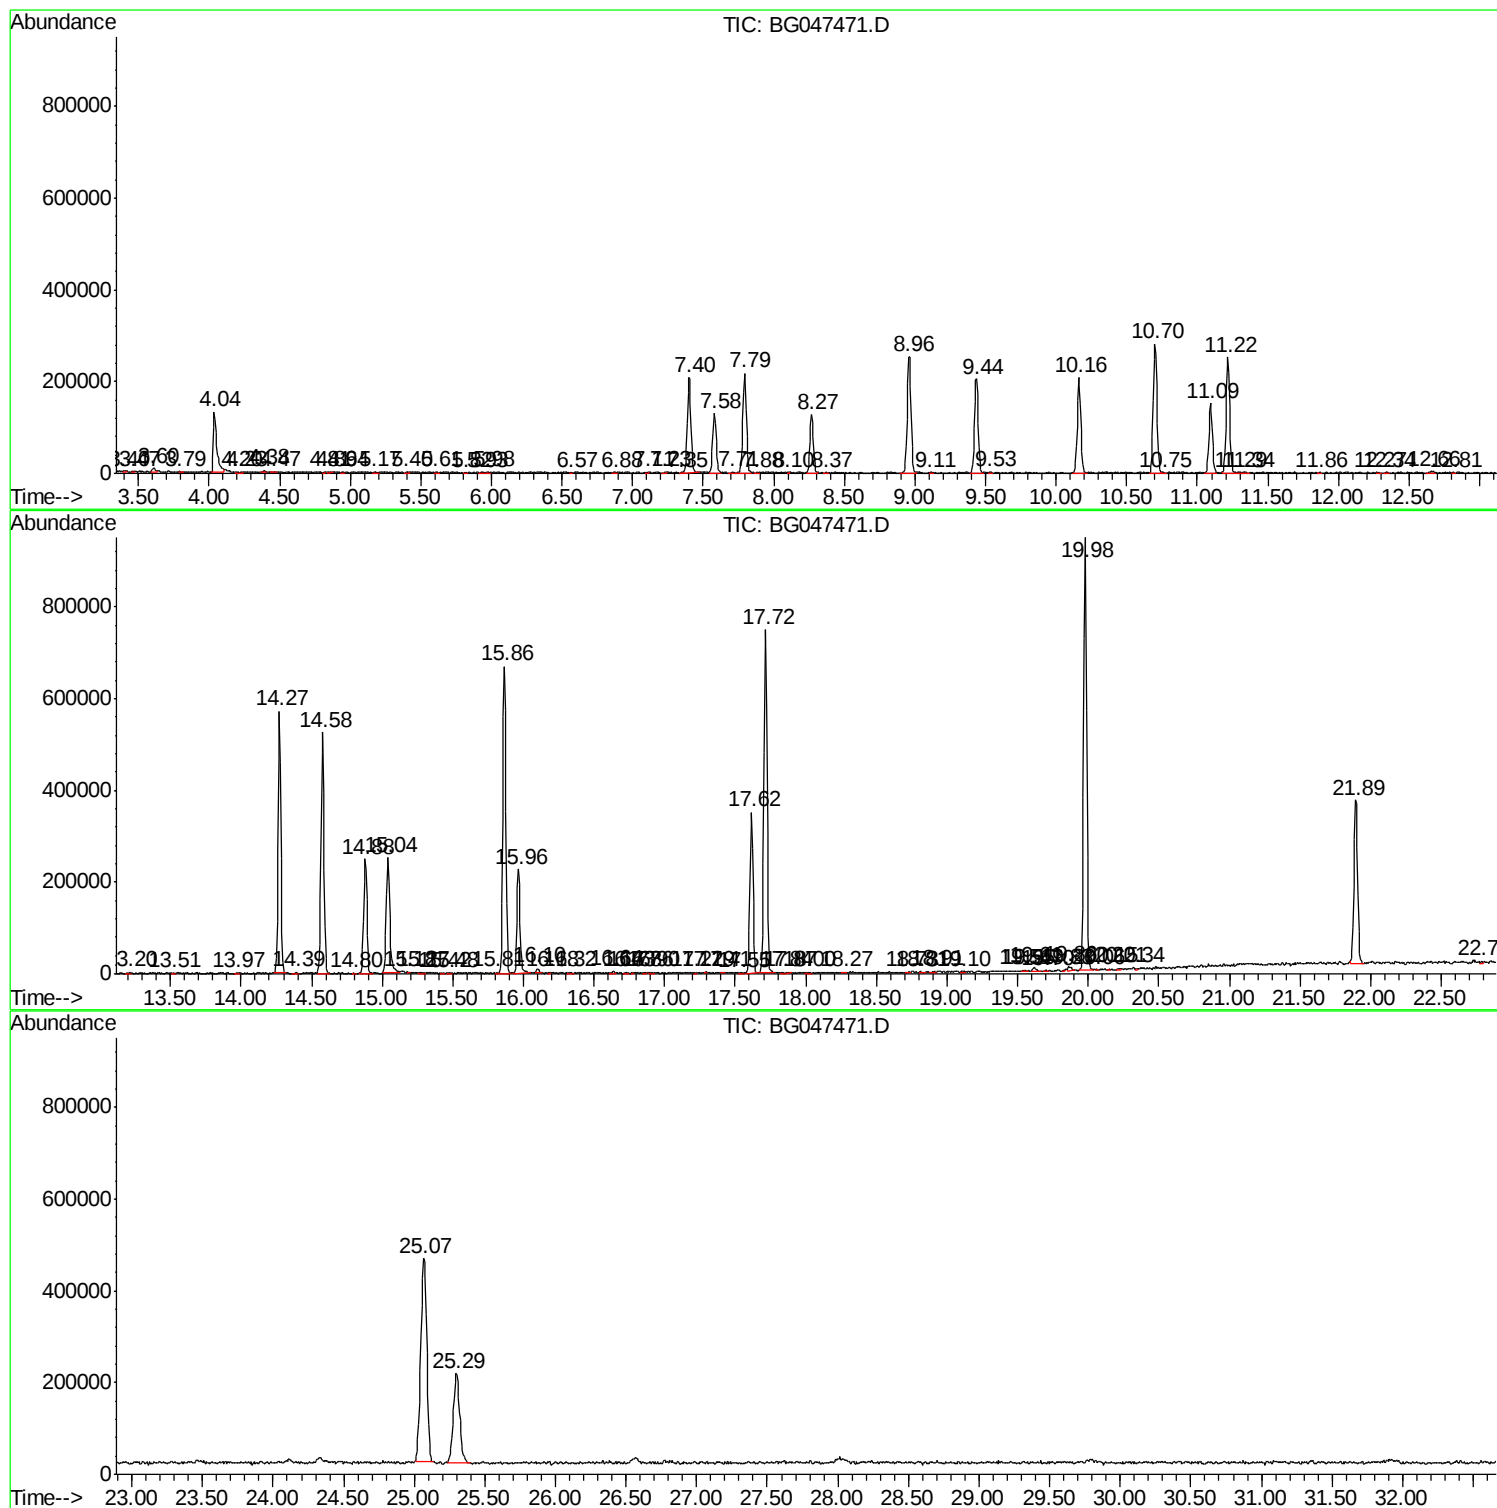

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG112520\
Data_File : BG047471.D
Acq_On : 25-Nov-2020 17:000
Operator : CG/JUU
Sample : PB133233BLL
Misc : MDL-WATER-BL033
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK233

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SEAM-EPA-BG111820.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
