

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120320\
 Data File : BG047538.D
 Acq On : 3 Dec 2020 14:42
 Operator : CG/JU
 Sample : PB133285BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.582	37	41	47	rBV3	8313	12733	0.81%	0.095%
2	4.363	169	174	181	rBV3	3177	5771	0.37%	0.043%
3	4.539	196	204	205	rBV	1864	3173	0.20%	0.024%
4	4.581	208	211	214	rBV2	1820	2426	0.15%	0.018%
5	4.727	235	236	240	rVB2	2574	2300	0.15%	0.017%
6	4.839	253	255	258	rVB2	2140	2399	0.15%	0.018%
7	5.438	354	357	362	rVB2	1814	2810	0.18%	0.021%
8	7.383	681	688	698	rBV	179697	318553	20.28%	2.387%
9	7.559	712	718	726	rBV	107365	177146	11.28%	1.327%
10	7.777	744	755	765	rBV	174249	306415	19.51%	2.296%
11	8.247	828	835	842	rBV2	120353	217662	13.86%	1.631%
12	8.940	946	953	960	rVB2	205865	362318	23.06%	2.715%
13	9.169	989	992	996	rBV2	2095	2641	0.17%	0.020%
14	9.234	1000	1003	1005	rBV2	2353	2683	0.17%	0.020%
15	9.416	1026	1034	1045	rBV2	171119	317701	20.22%	2.381%
16	10.145	1149	1158	1168	rBV2	168259	310733	19.78%	2.328%
17	10.685	1242	1250	1258	rBV	223609	404433	25.74%	3.031%
18	10.738	1258	1259	1262	rVB	3854	2586	0.16%	0.019%
19	10.809	1267	1271	1273	rBV	2172	2828	0.18%	0.021%
20	11.073	1308	1316	1326	rVB	153267	284056	18.08%	2.129%
21	11.196	1330	1337	1349	rVB	200712	387321	24.66%	2.902%
22	11.384	1368	1369	1373	rBV	2026	2207	0.14%	0.017%
23	11.431	1373	1377	1382	rVV	1986	2945	0.19%	0.022%
24	12.630	1577	1581	1582	rBV	3896	3558	0.23%	0.027%
25	13.570	1738	1741	1745	rVB	1843	3041	0.19%	0.023%
26	14.257	1850	1858	1864	rBV	552773	787812	50.15%	5.903%
27	14.563	1902	1910	1917	rBV	455723	743483	47.33%	5.571%
28	14.675	1926	1929	1932	rBV	2310	2795	0.18%	0.021%
29	14.863	1954	1961	1967	rBV	262085	418756	26.66%	3.138%
30	15.021	1982	1988	1997	rBV	278731	449652	28.62%	3.369%
31	15.585	2081	2084	2088	rBV	2207	2672	0.17%	0.020%
32	15.850	2118	2129	2137	rBV	644004	984957	62.70%	7.381%
33	15.950	2141	2146	2158	rVV2	259788	396003	25.21%	2.967%
34	16.091	2165	2170	2176	rVB4	7967	13627	0.87%	0.102%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120320\
 Data File : BG047538.D
 Acq On : 3 Dec 2020 14:42
 Operator : CG/JU
 Sample : PB133285BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK85

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	16.355	2213	2215	2220	rVB	3451	3947	0.25%	0.030%
36	16.402	2220	2223	2224	rBV	2608	2447	0.16%	0.018%
37	16.631	2259	2262	2266	rVB3	3825	3721	0.24%	0.028%
38	16.766	2283	2285	2291	rBV	1845	3824	0.24%	0.029%
39	17.125	2341	2346	2348	rBV	1571	2456	0.16%	0.018%
40	17.225	2362	2363	2367	rBV	2610	2876	0.18%	0.022%
41	17.601	2421	2427	2434	rVV	387146	594969	37.87%	4.458%
42	17.695	2437	2443	2455	rVB2	764282	1195699	76.11%	8.960%
43	17.783	2455	2458	2460	rBV2	2489	2593	0.17%	0.019%
44	18.000	2492	2495	2500	rVB2	2777	4199	0.27%	0.031%
45	18.041	2500	2502	2505	rBV	2282	2241	0.14%	0.017%
46	18.071	2505	2507	2509	rBV2	2039	2232	0.14%	0.017%
47	18.335	2549	2552	2553	rBV3	2648	3092	0.20%	0.023%
48	18.464	2573	2574	2576	rBV	3003	2499	0.16%	0.019%
49	18.541	2585	2587	2593	rVB2	1804	2875	0.18%	0.022%
50	18.588	2593	2595	2598	rBV3	2512	2697	0.17%	0.020%
51	18.876	2641	2644	2645	rBV	3519	3600	0.23%	0.027%
52	18.893	2645	2647	2651	rVB2	3087	4584	0.29%	0.034%
53	18.970	2658	2660	2661	rBV	2620	2408	0.15%	0.018%
54	18.993	2663	2664	2670	rVV2	2608	4753	0.30%	0.036%
55	19.046	2671	2673	2675	rVB2	4018	2708	0.17%	0.020%
56	19.134	2686	2688	2689	rBV	4009	3062	0.19%	0.023%
57	19.287	2712	2714	2717	rBV2	2034	2804	0.18%	0.021%
58	19.563	2760	2761	2763	rBV	2595	2394	0.15%	0.018%
59	19.604	2763	2768	2771	rVB	9250	15249	0.97%	0.114%
60	19.669	2777	2779	2782	rVB3	3864	3105	0.20%	0.023%
61	19.692	2782	2783	2787	rBV4	3677	4429	0.28%	0.033%
62	19.786	2795	2799	2802	rBV3	3743	6712	0.43%	0.050%
63	19.851	2806	2810	2815	rVB5	10902	19453	1.24%	0.146%
64	19.963	2820	2829	2835	rBV	1137169	1570942	100.00%	11.772%
65	20.162	2861	2863	2866	rBV3	3732	3117	0.20%	0.023%
66	20.344	2892	2894	2895	rBV2	4047	2705	0.17%	0.020%
67	20.362	2895	2897	2898	rBV2	4977	4223	0.27%	0.032%
68	21.878	3148	3155	3162	rVB2	446177	755632	48.10%	5.662%
69	25.027	3681	3691	3703	rVB	494305	1438355	91.56%	10.778%
70	25.262	3722	3731	3744	rVB2	244546	717684	45.68%	5.378%
71	31.708	4826	4828	4831	rVB4	7177	4599	0.29%	0.034%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120320\
Data File : BG047538.D
Acq On : 3 Dec 2020 14:42
Operator : CG/JU
Sample : PB133285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK85

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 13345081

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120320\
Data File : BG047538.D
Acq On : 3 Dec 2020 14:42
Operator : CG/JU
Sample : PB133285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

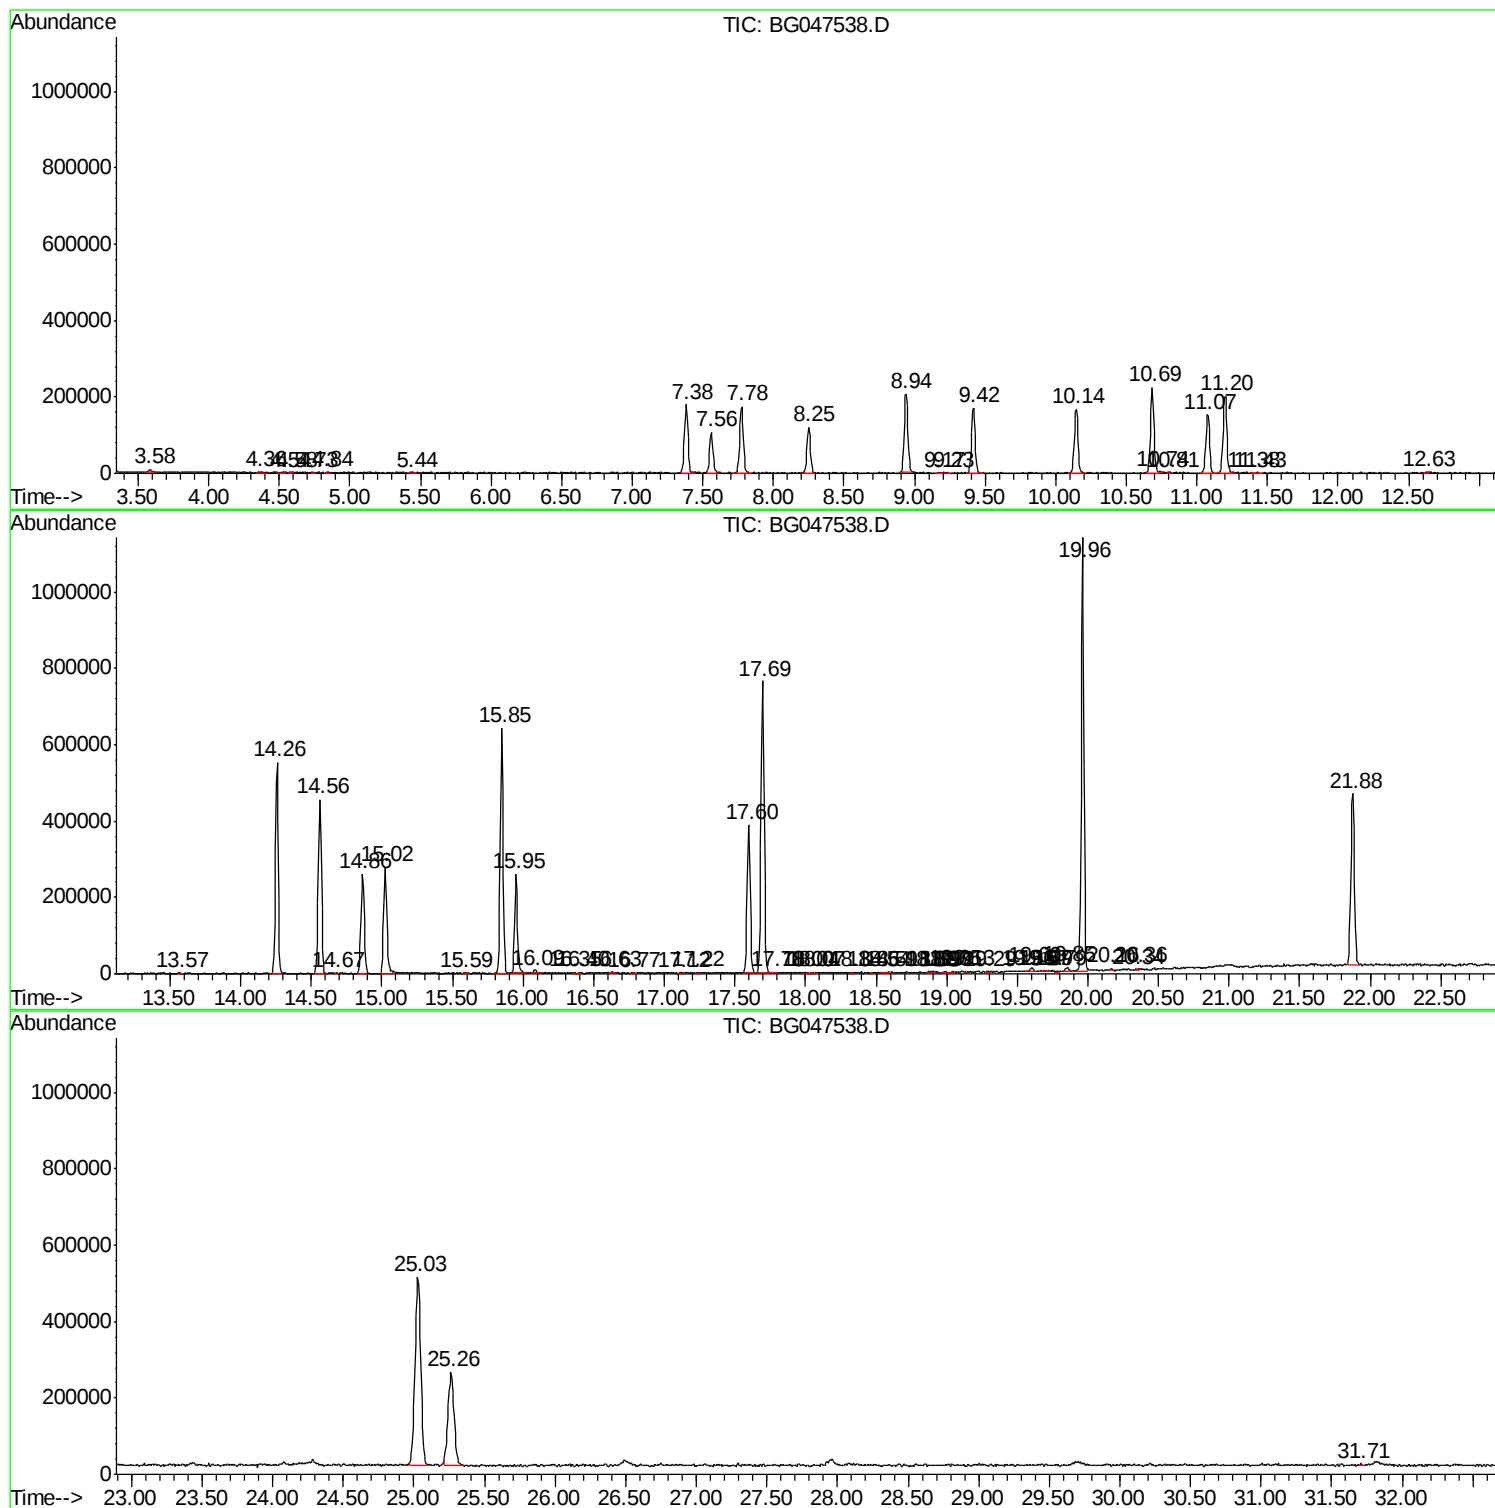

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120320\
Data File : BG047538.D
Acq On : 3 Dec 2020 14:42
Operator : CG/JU
Sample : PB133285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120320\
Data File : BG047538.D
Acq On : 3 Dec 2020 14:42
Operator : CG/JU
Sample : PB133285BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK85

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc