




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
 Data File : BG063683.D
 Acq On : 16 Dec 2024 11:12
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/18/2024

Quant Time: Dec 17 02:02:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 23:59:23 2024
 Response via : Initial Calibration

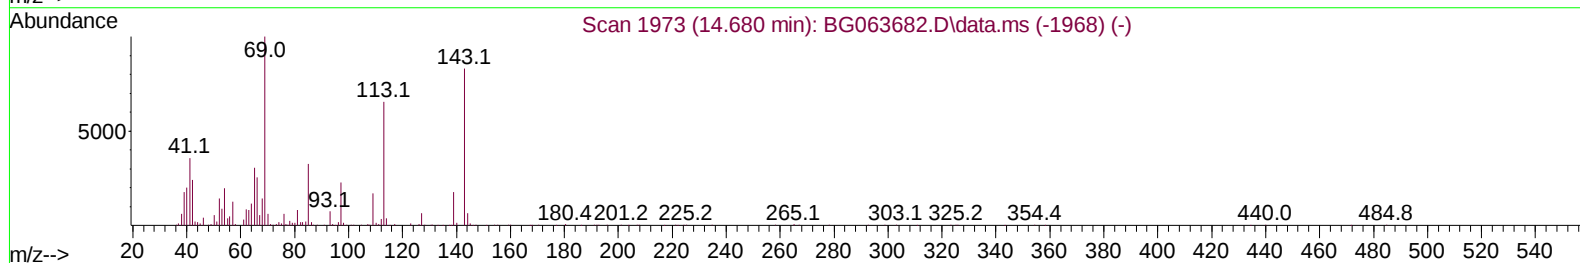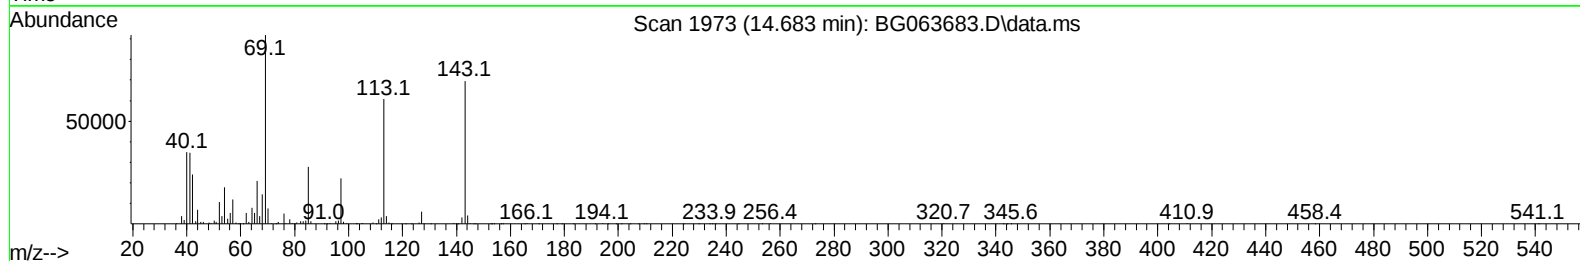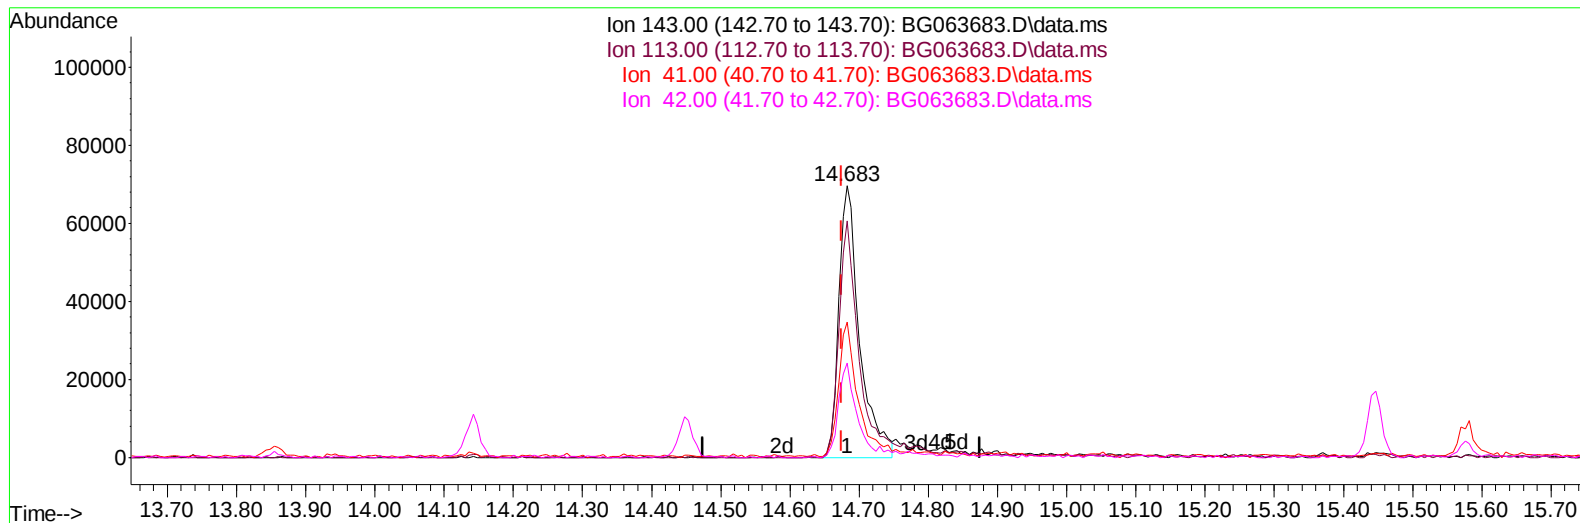

TIC: BG063683.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.683min (+ 0.008) 31.05 ng/u1

response 143697

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	87.15
41.00	48.20	49.94
42.00	26.60	34.72#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
 Data File : BG063683.D
 Acq On : 16 Dec 2024 11:12
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Manual IntegrationsAPPROVED

Quant Time: Dec 17 02:02:46 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 23:59:23 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/18/2024

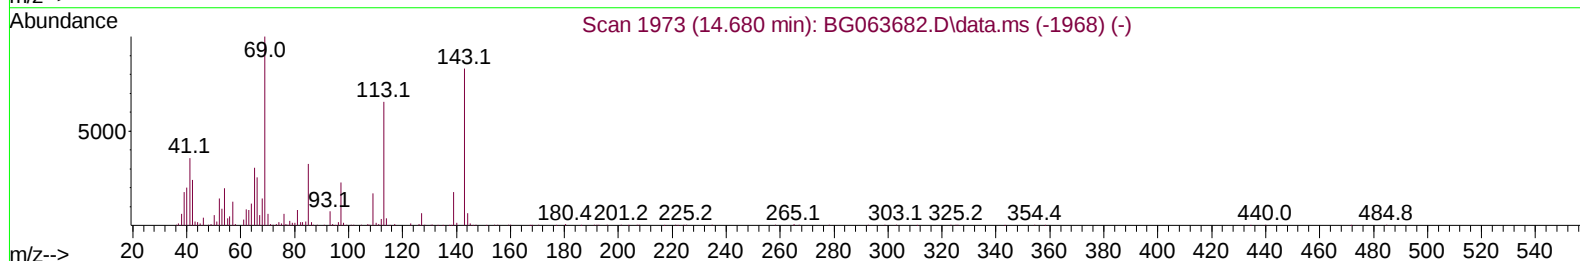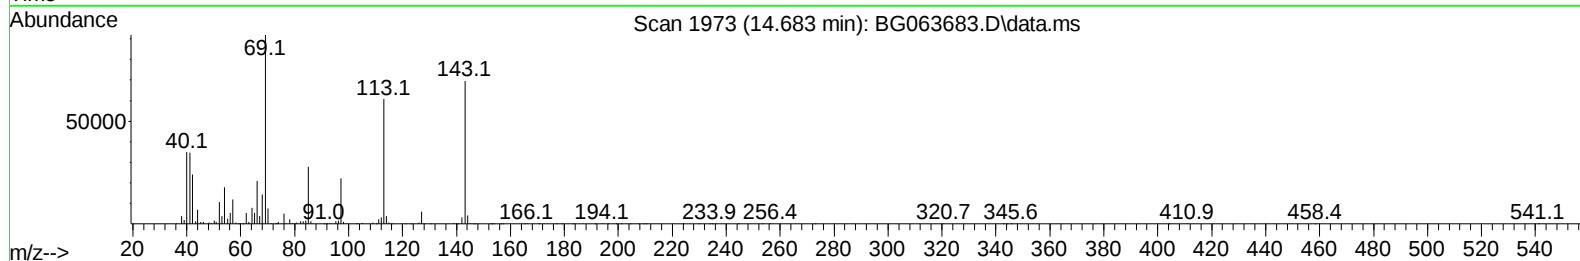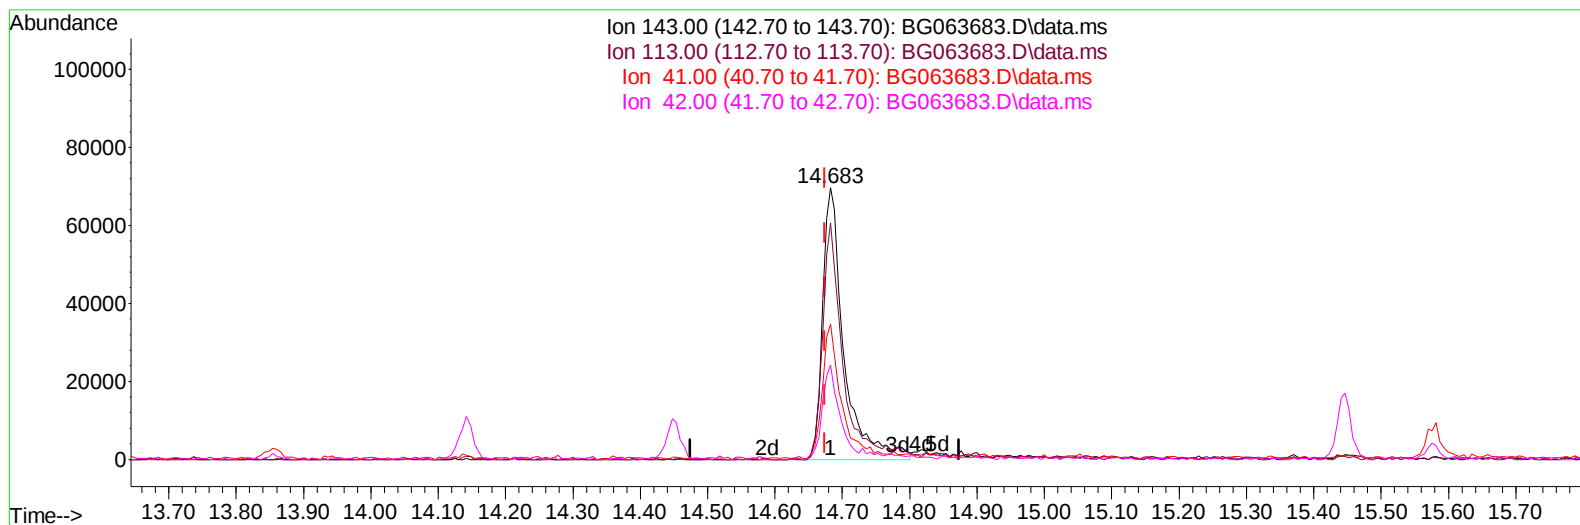

TIC: BG063683.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.683min (+ 0.008) 33.07 ng/ul m

response 153042

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	89.70	87.15
41.00	48.20	49.94
42.00	26.60	34.72#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
 Data File : BG063683.D
 Acq On : 16 Dec 2024 11:12
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/18/2024
 Supervised By :mohammad ahmed 12/18/2024

Quant Time: Dec 17 02:03:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 23:59:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.808	152	147189	20.000	ng/ul	0.00
20) Naphthalene-d8	10.599	136	605036	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.454	164	479961	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.203	188	1166431	20.000	ng/ul	0.00
79) Chrysene-d12	21.451	240	1124533	20.000	ng/ul	0.00
88) Perylene-d12	24.477	264	1223812	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.273	96	21682	5.773	ng/uL	0.00
4) Pyridine-d5	3.684	84	303291	25.597	ng/ul	0.00
7) Phenol-d5	6.998	99	410268	30.265	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.144	67	268336	28.660	ng/ul	0.00
11) 2-Chlorophenol-d4	7.350	132	273764	31.194	ng/ul	0.00
15) 4-Methylphenol-d8	8.531	113	318579	30.270	ng/ul	0.00
21) Nitrobenzene-d5	8.966	128	148060	34.273	ng/ul	0.00
24) 2-Nitrophenol-d4	9.689	143	161792	33.411	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.235	165	291129	31.052	ng/ul	0.00
31) 4-Chloroaniline-d4	10.734	131	401883	33.759	ng/ul	0.00
46) Dimethylphthalate-d6	13.854	166	1119319	34.273	ng/ul	0.00
49) Acenaphthylene-d8	14.142	160	1230589	33.054	ng/ul	0.00
54) 4-Nitrophenol-d4	14.683	143	153042m	33.073	ng/ul	0.00
60) Fluorene-d10	15.447	176	992501	34.372	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.576	200	166323	27.463	ng/ul	0.00
73) Anthracene-d10	17.303	188	1770540	35.306	ng/ul	0.00
81) Pyrene-d10	19.600	212	2000424	34.185	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.271	264	1925496	33.504	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
Data File : BG063683.D
Acq On : 16 Dec 2024 11:12
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Manual IntegrationsAPPROVED

Quant Time: Dec 17 02:03:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 23:59:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/18/2024
Supervised By :mohammad ahmed 12/18/2024

