

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
 Data File : BG063683.D
 Acq On : 16 Dec 2024 11:12
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG063683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.684	96	101	111	rBV	490841	834932	16.18%	1.643%
2	5.153	349	351	352	rBV	9465	9034	0.18%	0.018%
3	5.617	429	430	433	rBV2	8756	8853	0.17%	0.017%
4	5.758	451	454	457	rBV3	8879	14968	0.29%	0.029%
5	6.034	499	501	504	rBV3	8187	8072	0.16%	0.016%
6	6.187	525	527	528	rBV2	13191	11514	0.22%	0.023%
7	6.463	572	574	578	rVB4	8241	7324	0.14%	0.014%
8	6.657	604	607	609	rBV3	9865	11979	0.23%	0.024%
9	6.810	632	633	636	rBV3	8247	7263	0.14%	0.014%
10	6.998	659	665	674	rBV	681869	1149168	22.27%	2.261%
11	7.144	684	690	698	rVB	543585	893802	17.32%	1.758%
12	7.350	719	725	732	rBV	659473	1086090	21.04%	2.137%
13	7.503	749	751	755	rBV3	9382	10681	0.21%	0.021%
14	7.744	790	792	795	rVB2	9579	9147	0.18%	0.018%
15	7.808	796	803	810	rVV	546189	924390	17.91%	1.819%
16	7.961	826	829	831	rVB	9736	10212	0.20%	0.020%
17	7.985	831	833	835	rBV	9785	7079	0.14%	0.014%
18	8.014	835	838	841	rBV3	9532	14006	0.27%	0.028%
19	8.531	916	926	934	rBV	830721	1487746	28.83%	2.927%
20	8.901	987	989	992	rVB3	8145	7536	0.15%	0.015%
21	8.966	992	1000	1012	rBV	674086	1188626	23.03%	2.338%
22	9.125	1025	1027	1030	rVB3	9846	8155	0.16%	0.016%
23	9.465	1083	1085	1087	rBV2	6450	7950	0.15%	0.016%
24	9.553	1096	1100	1102	rBV3	10244	12020	0.23%	0.024%
25	9.689	1115	1123	1132	rBV	550044	994037	19.26%	1.956%
26	10.065	1183	1187	1188	rBV	9372	8275	0.16%	0.016%
27	10.235	1208	1216	1230	rBV	765913	1411700	27.35%	2.777%
28	10.452	1252	1253	1256	rVB2	9367	7499	0.15%	0.015%
29	10.494	1256	1260	1262	rBV	8392	8054	0.16%	0.016%
30	10.599	1267	1278	1289	rBV	778130	1375625	26.65%	2.706%
31	10.682	1289	1292	1294	rBV4	7244	9354	0.18%	0.018%
32	10.740	1294	1302	1313	rBV	741516	1441453	27.93%	2.836%
33	10.928	1332	1334	1337	rVB4	6969	7804	0.15%	0.015%
34	11.175	1374	1376	1381	rBV6	9010	10911	0.21%	0.021%
35	11.310	1395	1399	1401	rBV3	7149	11392	0.22%	0.022%
36	11.381	1408	1411	1414	rBV	8546	8704	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
 Data File : BG063683.D
 Acq On : 16 Dec 2024 11:12
 Operator : RC/JU
 Sample : PB165588BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK588

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
 Title : SVOA CALIBRATION

37	11.510	1431	1433	1436	rBV2	8377	8858	0.17%	0.017%
38	11.686	1460	1463	1465	rBV2	6212	7218	0.14%	0.014%
39	11.739	1469	1472	1474	rVB	8524	9296	0.18%	0.018%
40	11.798	1478	1482	1484	rBV3	6724	7383	0.14%	0.015%
41	12.039	1519	1523	1527	rBV2	12042	20904	0.41%	0.041%
42	12.086	1527	1531	1534	rVV3	8602	12277	0.24%	0.024%
43	12.197	1549	1550	1557	rVB4	13219	26087	0.51%	0.051%
44	12.344	1572	1575	1577	rVB2	8364	10031	0.19%	0.020%
45	12.368	1577	1579	1581	rBV	8099	7671	0.15%	0.015%
46	12.615	1617	1621	1624	rBV3	10400	10765	0.21%	0.021%
47	12.656	1624	1628	1631	rVB3	6304	8530	0.17%	0.017%
48	12.996	1680	1686	1689	rBV2	9394	15848	0.31%	0.031%
49	13.038	1691	1693	1697	rVV4	8515	9678	0.19%	0.019%
50	13.073	1697	1699	1701	rVV	8633	7328	0.14%	0.014%
51	13.155	1711	1713	1716	rBV2	6567	8344	0.16%	0.016%
52	13.226	1723	1725	1727	rBV2	7036	7492	0.15%	0.015%
53	13.320	1739	1741	1745	rVB2	9266	9746	0.19%	0.019%
54	13.355	1745	1747	1750	rBV3	7498	9584	0.19%	0.019%
55	13.449	1760	1763	1765	rVB2	7938	7673	0.15%	0.015%
56	13.649	1795	1797	1801	rVB2	8932	8078	0.16%	0.016%
57	13.854	1826	1832	1841	rBV	1726441	2479730	48.04%	4.878%
58	13.995	1854	1856	1862	rVB6	6464	8052	0.16%	0.016%
59	14.142	1874	1881	1888	rBV2	1852353	2873504	55.67%	5.653%
60	14.448	1925	1933	1942	rVB	1378336	2165740	41.96%	4.261%
61	14.512	1942	1944	1949	rBV3	8195	9982	0.19%	0.020%
62	14.683	1966	1973	1986	rBV	522321	1090218	21.12%	2.145%
63	15.235	2065	2067	2070	rVB2	8325	7275	0.14%	0.014%
64	15.270	2070	2073	2075	rBV4	6920	8842	0.17%	0.017%
65	15.370	2086	2090	2093	rBV5	11437	18549	0.36%	0.036%
66	15.447	2096	2103	2112	rBV	2580950	3826766	74.14%	7.529%
67	15.576	2119	2125	2138	rBV	737256	1162914	22.53%	2.288%
68	15.687	2142	2144	2151	rVB5	24372	31788	0.62%	0.063%
69	15.846	2169	2171	2175	rVB2	10948	8745	0.17%	0.017%
70	15.946	2186	2188	2193	rVB5	9820	12596	0.24%	0.025%
71	16.234	2229	2237	2239	rBV7	11387	20657	0.40%	0.041%
72	16.387	2259	2263	2267	rVB5	9365	13988	0.27%	0.028%
73	16.680	2311	2313	2314	rBV2	9290	8099	0.16%	0.016%
74	16.769	2325	2328	2331	rBV5	11542	13398	0.26%	0.026%
75	16.892	2348	2349	2353	rVB3	9097	8903	0.17%	0.018%
76	17.203	2395	2402	2412	rBV2	1926444	2898594	56.16%	5.703%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
Data File : BG063683.D
Acq On : 16 Dec 2024 11:12
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Title : SVOA CALIBRATION

77	17.303	2412	2419	2432	rVV	2968513	4548852	88.13%	8.949%
78	19.600	2804	2810	2817	rBV	3580952	5161289	100.00%	10.154%
79	21.451	3120	3125	3135	rVB2	1847167	2921572	56.61%	5.748%
80	24.271	3598	3605	3620	rVB2	1912427	4853022	94.03%	9.548%
81	24.471	3633	3639	3653	rVB	1333496	3438610	66.62%	6.765%




Sum of corrected areas: 50829831

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
Data File : BG063683.D
Acq On : 16 Dec 2024 11:12
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

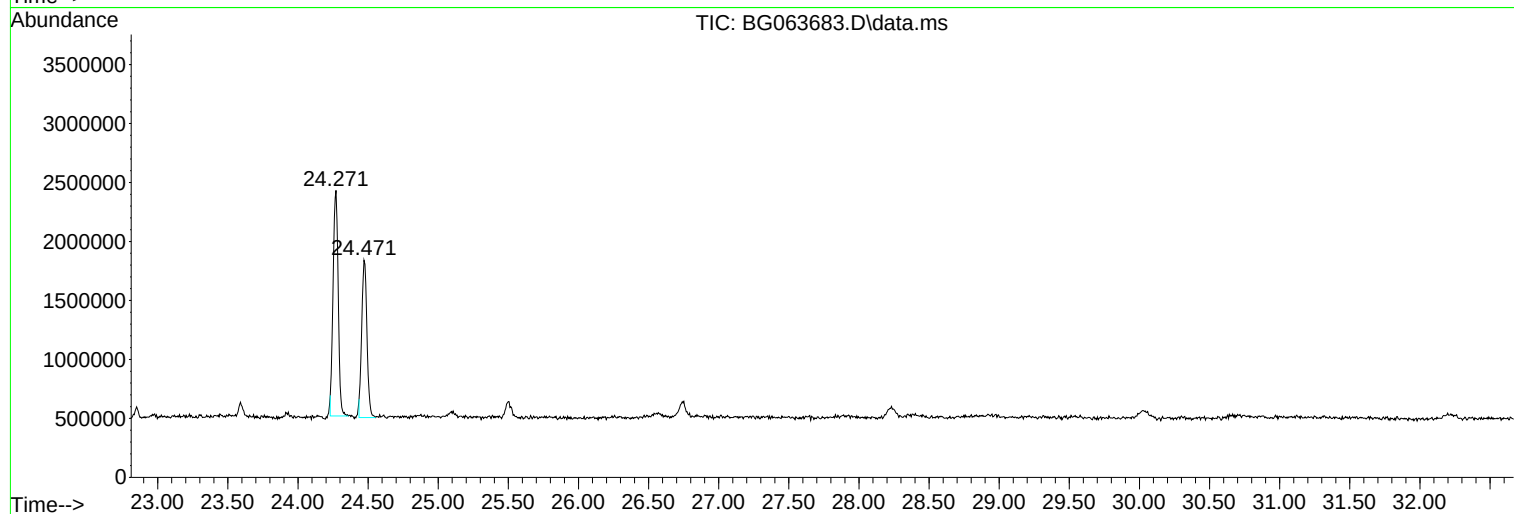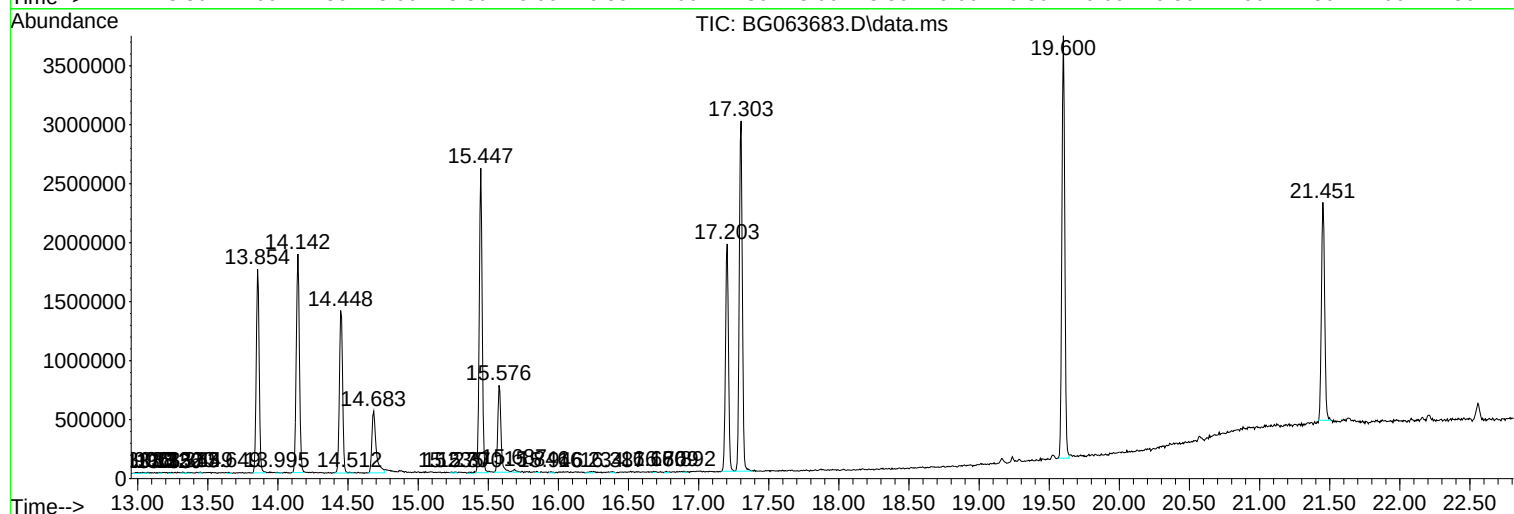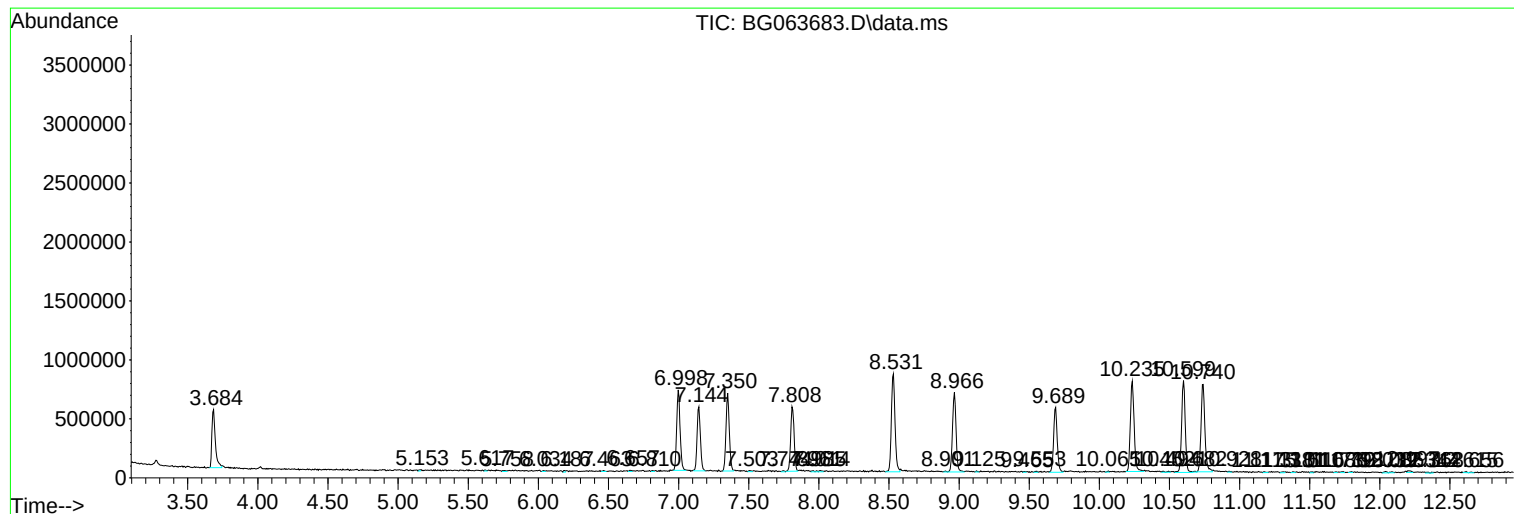

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
Data File : BG063683.D
Acq On : 16 Dec 2024 11:12
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121624\
Data File : BG063683.D
Acq On : 16 Dec 2024 11:12
Operator : RC/JU
Sample : PB165588BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK588

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc