


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122118\
 Data File : BG038780.D
 Acq On : 21 Dec 2018 8:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

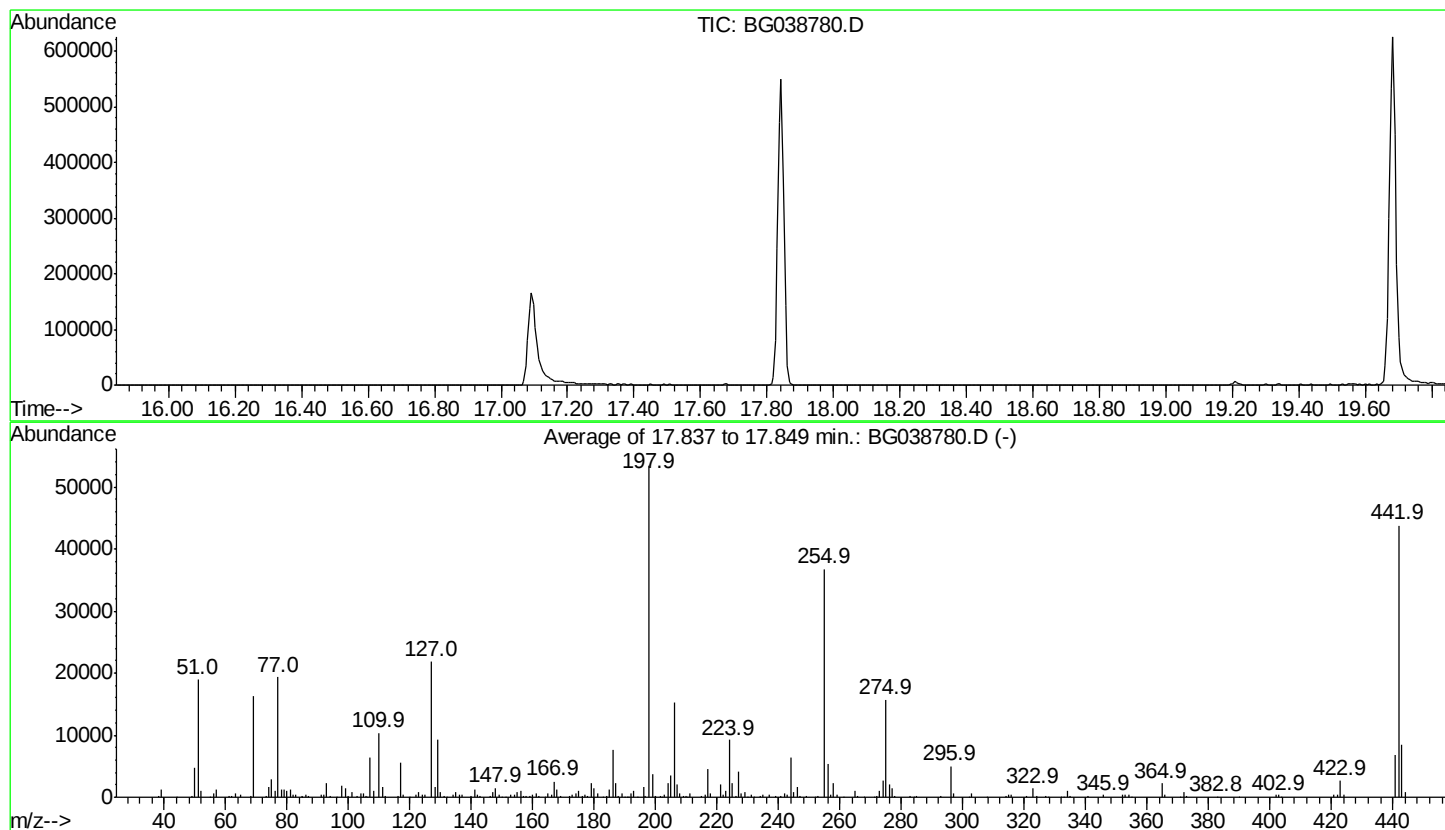

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	18900	PASS
68	69	0.00	2	1.3	206	PASS
69	198	0.00	100	30.5	16311	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.9	21833	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53424	PASS
199	198	5	9	6.9	3692	PASS
275	198	10	60	29.5	15742	PASS
365	198	1	100	4.1	2194	PASS
441	198	0.01	100	12.7	6764	PASS
442	198	50	100	81.9	43768	PASS
443	442	15	24	19.5	8547	PASS