


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG122118\
 Data File : BG038788.D
 Acq On : 21 Dec 2018 16:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

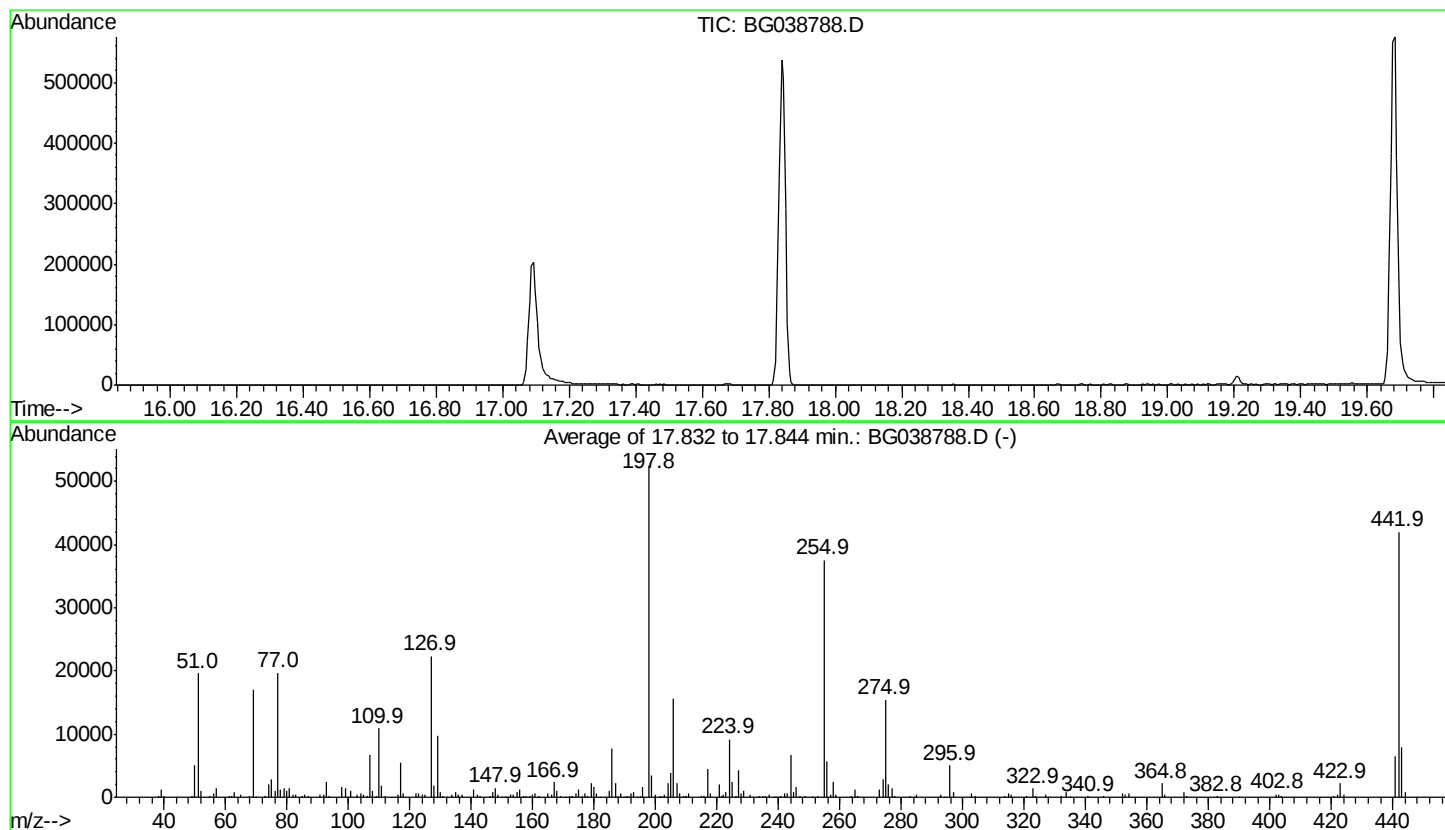

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	19650	PASS
68	69	0.00	2	1.4	238	PASS
69	198	0.00	100	32.5	17078	PASS
70	69	0.00	2	0.4	69	PASS
127	198	10	80	42.6	22362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52485	PASS
199	198	5	9	6.6	3464	PASS
275	198	10	60	29.4	15450	PASS
365	198	1	100	4.1	2160	PASS
441	198	0.01	100	12.4	6524	PASS
442	198	50	100	79.9	41954	PASS
443	442	15	24	19.1	8000	PASS