


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122118\
 Data File : BG038807.D
 Acq On : 22 Dec 2018 8:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG121218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 12 15:26:27 2018

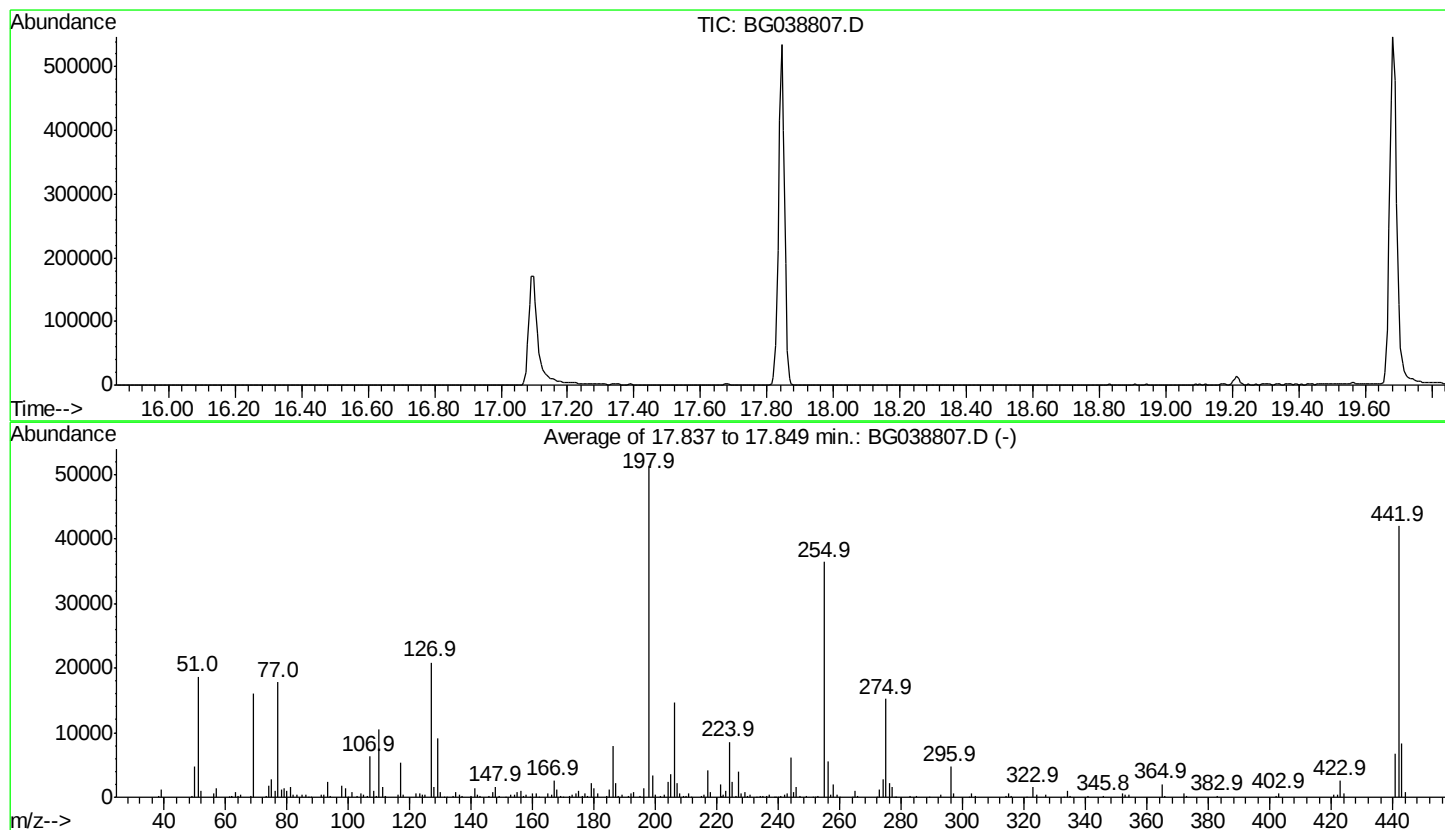

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	18640	PASS
68	69	0.00	2	1.4	228	PASS
69	198	0.00	100	31.4	16118	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	20821	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51333	PASS
199	198	5	9	6.6	3385	PASS
275	198	10	60	29.7	15250	PASS
365	198	1	100	4.1	2081	PASS
441	198	0.01	100	13.1	6737	PASS
442	198	50	100	81.8	42010	PASS
443	442	15	24	19.7	8293	PASS