

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080515\
 Data File : BG018278.D
 Acq On : 5 Aug 2015 19:42
 Operator : UM/TP
 Sample : PB84843BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080515.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.800	17	19	22	rBV3	2120	1756	0.18%	0.020%
2	2.906	33	37	39	rBV2	4619	6345	0.66%	0.073%
3	3.247	93	95	98	rBV2	2899	2740	0.28%	0.032%
4	3.458	129	131	134	rBV2	2078	2182	0.23%	0.025%
5	3.652	162	164	166	rVB2	2332	2117	0.22%	0.024%
6	3.764	181	183	187	rBV2	2089	3382	0.35%	0.039%
7	3.793	187	188	194	rVB2	2910	3485	0.36%	0.040%
8	4.087	236	238	241	rBV2	2509	2154	0.22%	0.025%
9	4.122	241	244	246	rVB2	2196	1960	0.20%	0.023%
10	4.533	313	314	316	rBV	2157	1800	0.19%	0.021%
11	4.610	325	327	330	rBV2	1787	2489	0.26%	0.029%
12	4.798	354	359	364	rVB3	1802	3144	0.32%	0.036%
13	4.956	384	386	388	rBV2	1983	2033	0.21%	0.023%
14	5.268	438	439	442	rVB	2127	2042	0.21%	0.024%
15	5.432	465	467	471	rVB	1944	2051	0.21%	0.024%
16	5.538	480	485	486	rBV2	1245	1821	0.19%	0.021%
17	5.726	514	517	521	rBV	2035	2437	0.25%	0.028%
18	5.844	535	537	541	rBV	1830	2091	0.22%	0.024%
19	5.920	548	550	553	rVV	2588	2193	0.23%	0.025%
20	5.973	557	559	560	rBV2	2650	1752	0.18%	0.020%
21	6.008	561	565	568	rVV3	2119	2566	0.27%	0.030%
22	6.061	571	574	576	rVV2	1639	1805	0.19%	0.021%
23	6.096	576	580	583	rVB3	1787	2037	0.21%	0.023%
24	6.249	602	606	607	rBV2	1592	2034	0.21%	0.023%
25	6.314	614	617	620	rBV	1428	2095	0.22%	0.024%
26	6.637	665	672	678	rBV	121534	182606	18.86%	2.106%
27	6.778	690	696	704	rVB	80982	129295	13.36%	1.491%
28	6.966	723	728	735	rVV	125684	203470	21.02%	2.347%
29	7.042	738	741	743	rVV	2746	2663	0.28%	0.031%
30	7.195	765	767	770	rVB	2641	2124	0.22%	0.024%
31	7.430	801	807	814	rBV	105978	164649	17.01%	1.899%
32	7.594	832	835	837	rBV	1808	1756	0.18%	0.020%
33	7.730	851	858	859	rBV	1065	1855	0.19%	0.021%
34	7.976	898	900	902	rVB	1978	2012	0.21%	0.023%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080515\
 Data File : BG018278.D
 Acq On : 5 Aug 2015 19:42
 Operator : UM/TP
 Sample : PB84843BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080515.M
 Title : SVOA CALIBRATION

35	8.164	924	932	939	rBV	155897	247692	25.59%	2.857%
36	8.329	957	960	963	rBV	2009	2057	0.21%	0.024%
37	8.587	998	1004	1012	rVV	124992	202472	20.92%	2.335%
38	8.652	1012	1015	1020	rVB2	1595	2621	0.27%	0.030%
39	9.034	1078	1080	1086	rVB	2081	3216	0.33%	0.037%
40	9.122	1093	1095	1097	rVB	2398	1931	0.20%	0.022%
41	9.310	1120	1127	1136	rBV	120340	195178	20.16%	2.251%
42	9.856	1210	1220	1229	rBV2	164529	277165	28.63%	3.197%
43	9.998	1242	1244	1250	rVB2	1982	1834	0.19%	0.021%
44	10.144	1264	1269	1271	rVB	1325	1972	0.20%	0.023%
45	10.215	1275	1281	1288	rVV	142435	230461	23.81%	2.658%
46	10.362	1300	1306	1316	rVB	166860	267093	27.59%	3.081%
47	10.703	1360	1364	1365	rVB	1636	1943	0.20%	0.022%
48	10.738	1367	1370	1372	rVV	2137	1812	0.19%	0.021%
49	10.961	1407	1408	1413	rBV	1430	2170	0.22%	0.025%
50	11.731	1536	1539	1541	rBV	1985	2073	0.21%	0.024%
51	12.724	1706	1708	1711	rBV	2266	2669	0.28%	0.031%
52	13.529	1839	1845	1854	rVV	353838	496584	51.30%	5.728%
53	13.623	1857	1861	1863	rBV	1803	2245	0.23%	0.026%
54	13.799	1885	1891	1899	rBV	327294	498716	51.52%	5.752%
55	14.116	1938	1945	1952	rBV2	229224	344608	35.60%	3.975%
56	14.269	1969	1971	1975	rVB2	1713	1965	0.20%	0.023%
57	14.369	1983	1988	1994	rBV	138085	208823	21.57%	2.409%
58	15.115	2109	2115	2124	rVB	486928	653265	67.49%	7.535%
59	15.262	2134	2140	2152	rBV	158664	232009	23.97%	2.676%
60	15.544	2184	2188	2191	rVB	2371	2513	0.26%	0.029%
61	15.609	2197	2199	2204	rVB	1338	1942	0.20%	0.022%
62	15.855	2239	2241	2244	rVB	2194	2518	0.26%	0.029%
63	15.891	2244	2247	2249	rBV	1393	1830	0.19%	0.021%
64	15.908	2249	2250	2253	rVB	3063	2623	0.27%	0.030%
65	15.949	2253	2257	2258	rBV2	2651	3720	0.38%	0.043%
66	15.990	2263	2264	2268	rBV	2114	1898	0.20%	0.022%
67	16.032	2268	2271	2274	rBV	1561	1849	0.19%	0.021%
68	16.343	2321	2324	2325	rBV	2858	2802	0.29%	0.032%
69	16.872	2406	2414	2420	rBV	365517	483796	49.98%	5.580%
70	16.972	2425	2431	2441	rVB	608721	819712	84.68%	9.455%
71	17.095	2450	2452	2455	rVB2	2000	2044	0.21%	0.024%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080515\
Data File : BG018278.D
Acq On : 5 Aug 2015 19:42
Operator : UM/TP
Sample : PB84843BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080515.M
Title : SVOA CALIBRATION

72	17.154	2459	2462	2463	rBV	2202	2646	0.27%	0.031%
73	17.224	2472	2474	2476	rBV	3545	3155	0.33%	0.036%
74	17.307	2486	2488	2490	rVB2	2189	1797	0.19%	0.021%
75	17.600	2535	2538	2540	rVB2	2175	2581	0.27%	0.030%
76	17.624	2540	2542	2543	rBV2	1906	1836	0.19%	0.021%
77	17.747	2558	2563	2564	rBV2	2127	2636	0.27%	0.030%
78	17.818	2573	2575	2579	rBV	2007	2384	0.25%	0.027%
79	17.906	2589	2590	2594	rVB2	2886	1782	0.18%	0.021%
80	17.953	2594	2598	2600	rBV2	2157	2360	0.24%	0.027%
81	18.094	2620	2622	2624	rBV	1816	2045	0.21%	0.024%
82	18.211	2640	2642	2644	rBV	3230	2720	0.28%	0.031%
83	18.317	2658	2660	2663	rBV	1853	2160	0.22%	0.025%
84	18.347	2663	2665	2668	rVB	3349	3420	0.35%	0.039%
85	18.399	2670	2674	2677	rBV3	2425	3936	0.41%	0.045%
86	18.435	2678	2680	2683	rVV2	2084	1888	0.20%	0.022%
87	18.582	2701	2705	2706	rBV3	2772	2912	0.30%	0.034%
88	18.676	2719	2721	2722	rVB	3187	1861	0.19%	0.021%
89	18.764	2734	2736	2739	rBV3	1967	2032	0.21%	0.023%
90	18.793	2739	2741	2744	rBV4	3323	3513	0.36%	0.041%
91	18.864	2752	2753	2756	rVV3	2637	1782	0.18%	0.021%
92	18.969	2770	2771	2773	rBV2	2839	1850	0.19%	0.021%
93	18.993	2773	2775	2777	rBV3	2803	2838	0.29%	0.033%
94	19.022	2779	2780	2782	rBV2	3626	2497	0.26%	0.029%
95	19.169	2803	2805	2808	rVB2	5796	5291	0.55%	0.061%
96	19.281	2819	2824	2829	rBV	708586	968008	100.00%	11.165%
97	20.086	2959	2961	2962	rBV2	5455	3153	0.33%	0.036%
98	21.079	3126	3130	3136	rVB	451606	560853	57.94%	6.469%
99	23.100	3468	3474	3484	rVB	396543	736232	76.06%	8.492%
100	23.241	3492	3498	3504	rVB	209439	378814	39.13%	4.369%


Sum of corrected areas: 8669744

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080515\
Data File : BG018278.D
Acq On : 5 Aug 2015 19:42
Operator : UM/TP
Sample : PB84843BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080515.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

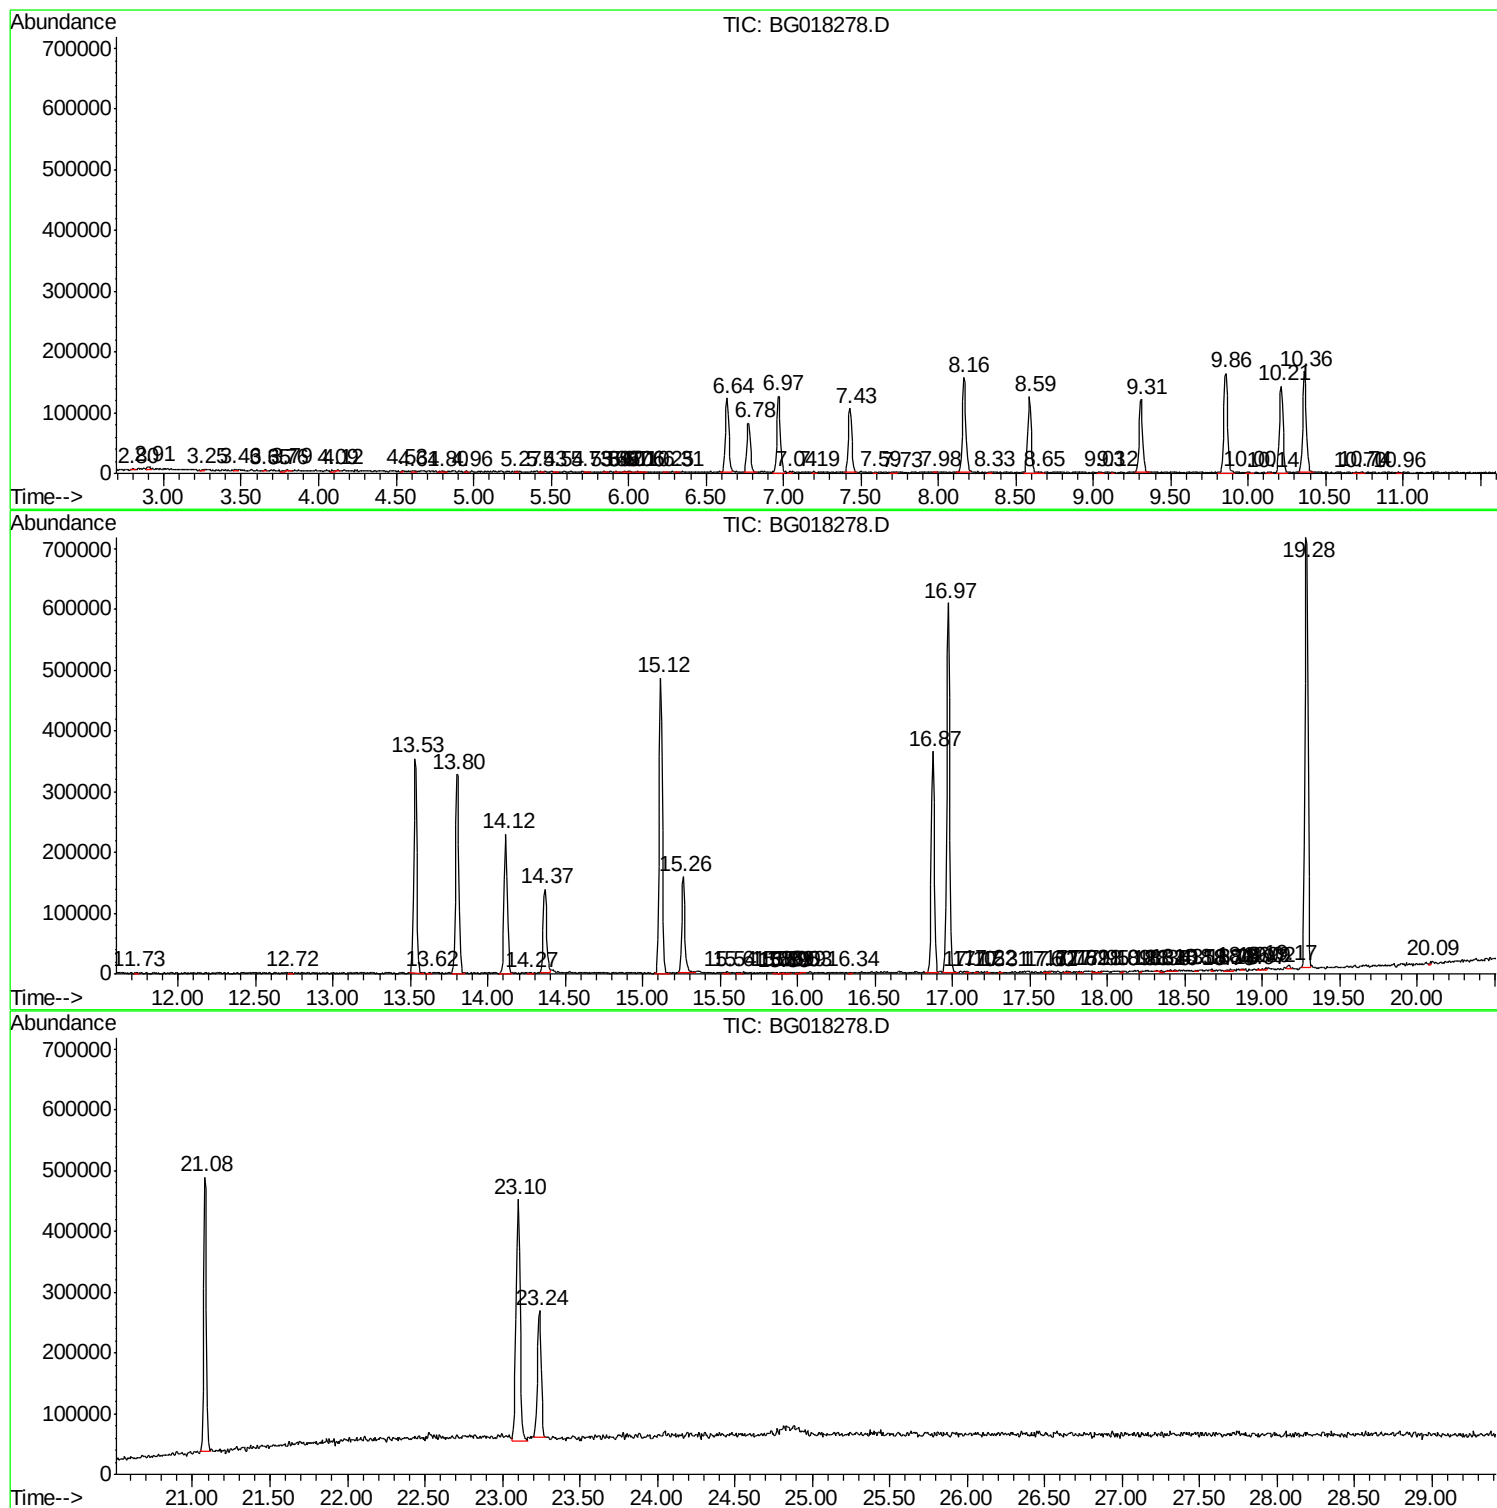

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG080515\
Data_File : BG018278.D
Acq_On : 5_Aug_2015_ 19:422
Operator : UM/TPP
Sample : PB84843BLL
Misc :
ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
SBLK43

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080515.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
