
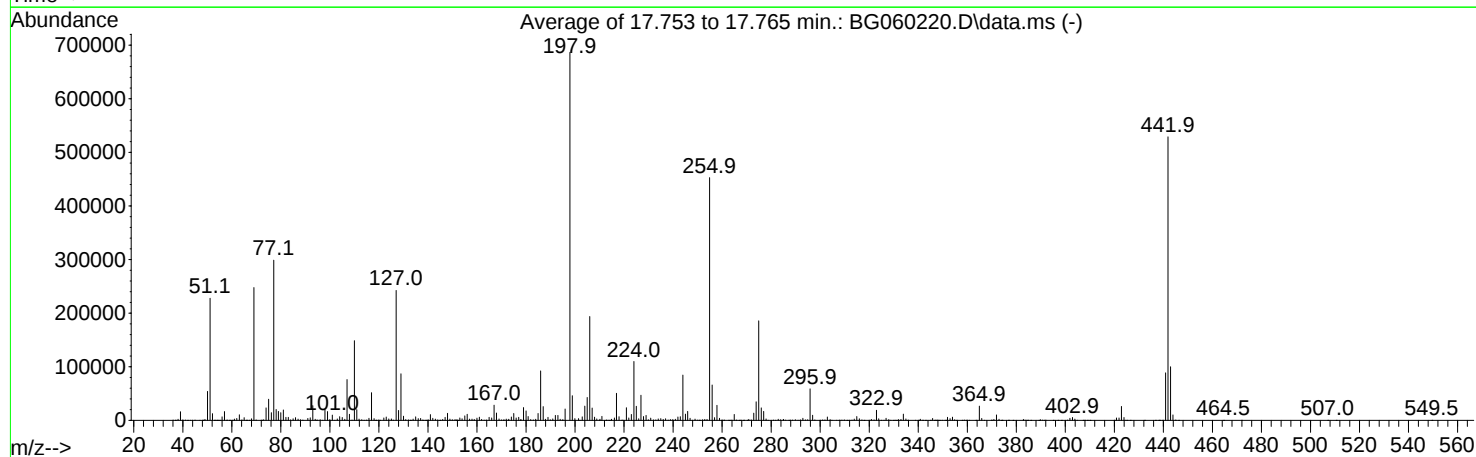


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010324\
Data File : BG060220.D
Acq On : 3 Jan 2024 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

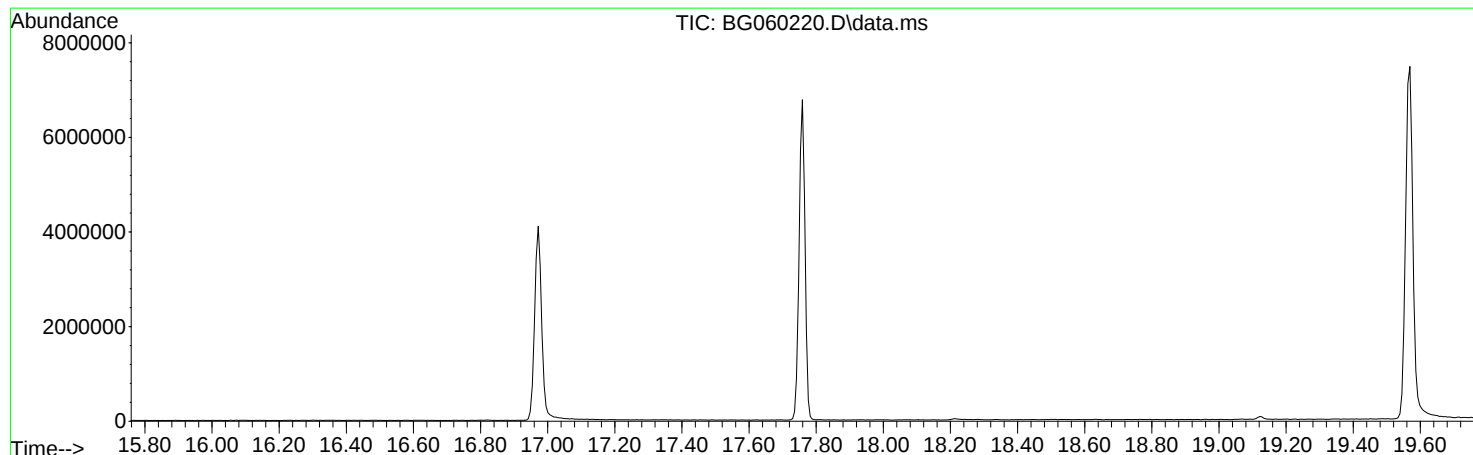

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	227831	PASS
68	69	0.00	2	1.2	2971	PASS
69	198	0.00	100	36.1	247916	PASS
70	69	0.00	2	0.3	811	PASS
127	198	10	80	35.3	242443	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	686293	PASS
199	198	5	9	6.7	46067	PASS
275	198	10	60	27.1	185749	PASS
365	198	1	100	3.9	26611	PASS
441	198	0.01	100	12.9	88712	PASS
442	442	50	100	100.0	528917	PASS
443	442	15	24	18.9	100029	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2024	BNA_G	<u>BG060220.D</u>
Compound Name	Response	Retention Time
DDT	2039906	20.797
DDD	146875	20.35
DDE	928	19.839
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
147803	2187709	6.76

Instrument :
BNA_G
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010324\  
Data File : BG060220.D  
Acq On    : 3 Jan 2024 10:09  
Operator  : MA/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 04 01:01:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

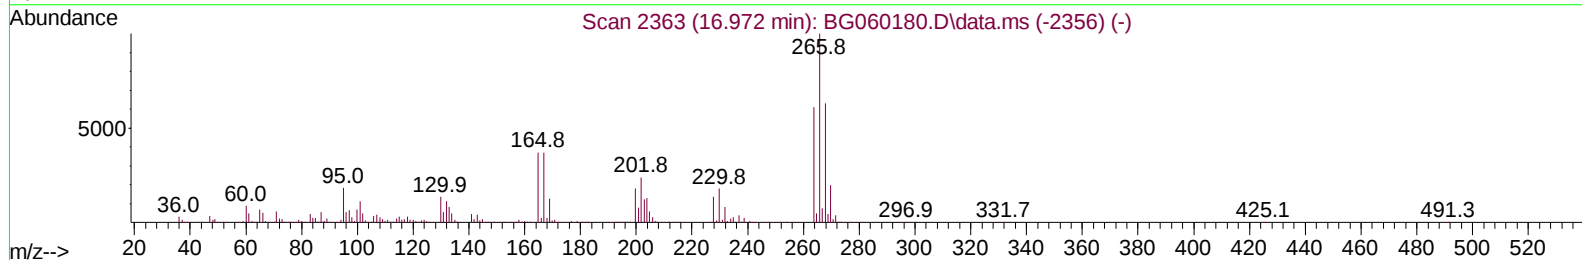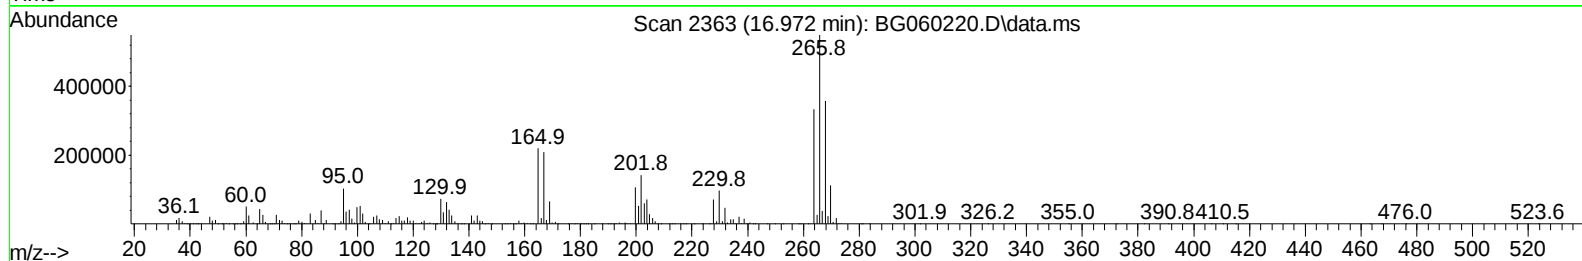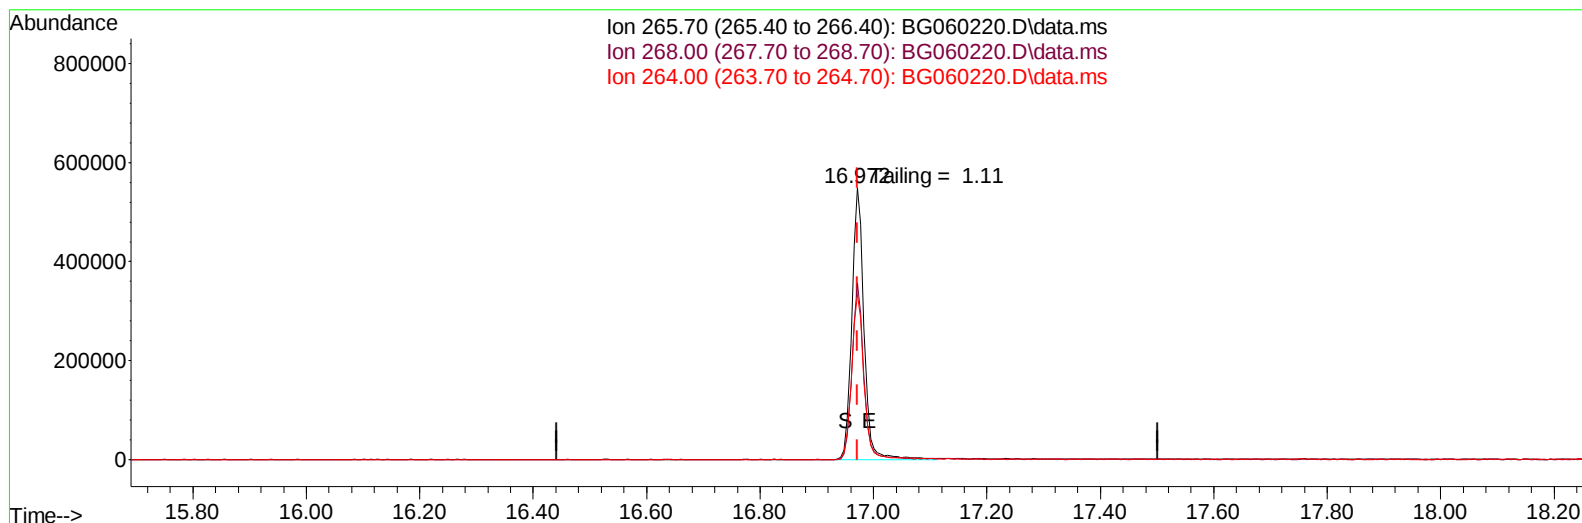

TIC: BG060220.D\data.ms

(70) Pentachlorophenol (C)

16.972min (-0.000) 36919.74 ng




response **825430**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	69.18
264.00	65.80	60.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010324\
Data File : BG060220.D
Acq On : 3 Jan 2024 10:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 04 01:01:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

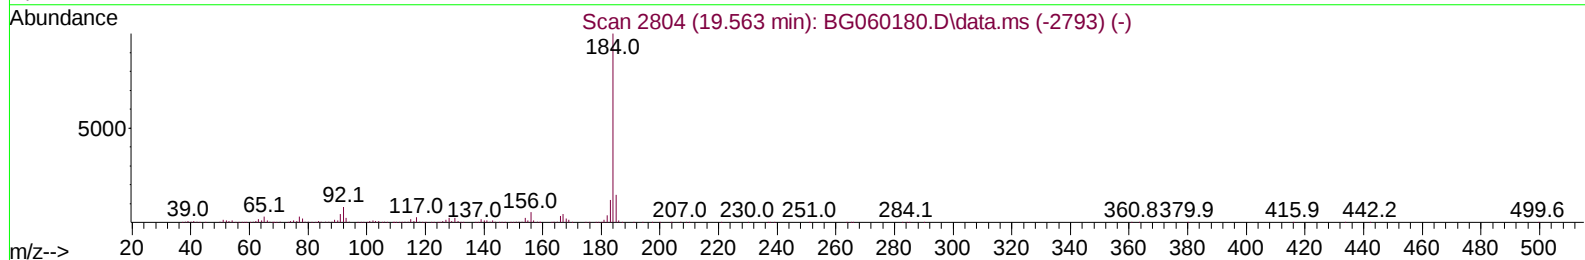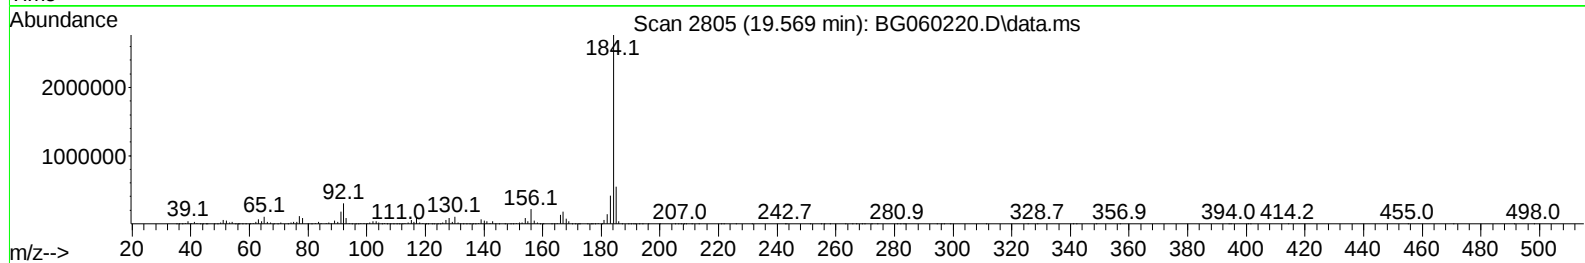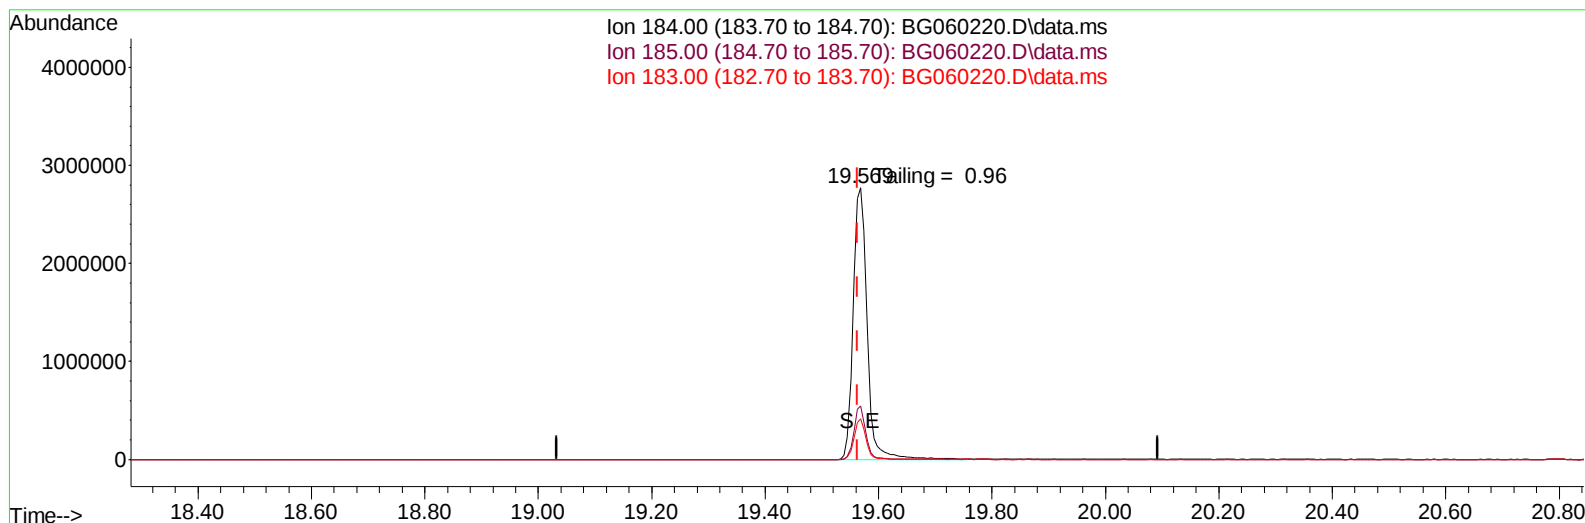

TIC: BG060220.D\data.ms

(77) Benzidine

19.569min (+ 0.006) 1829619.08 ng

response 4759942

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	19.69#
183.00	11.80	15.05#
0.00	0.00	0.00