
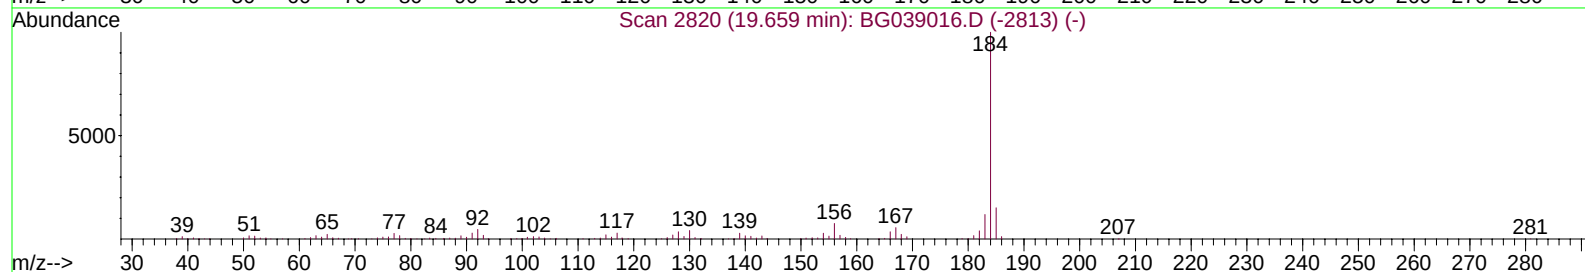
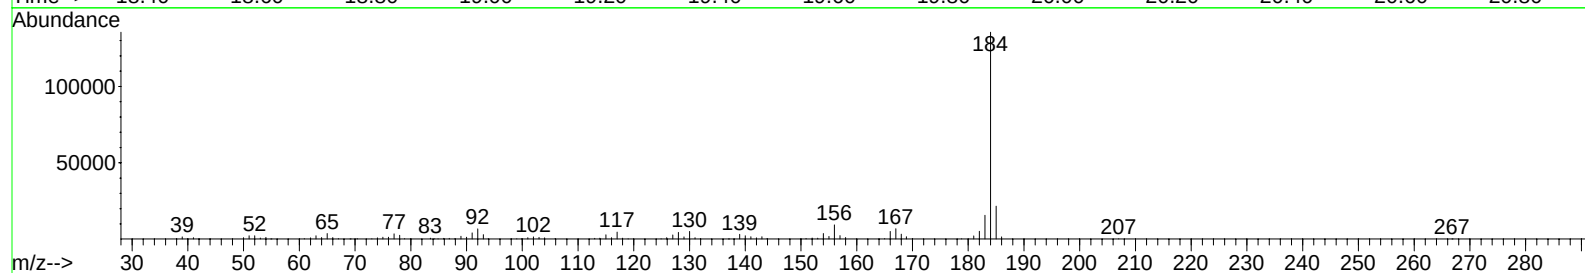


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012219\
 Data File : BG039247.D
 Acq On : 22 Jan 2019 10:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 17:50:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 18 04:20:14 2019
 Response via : Initial Calibration

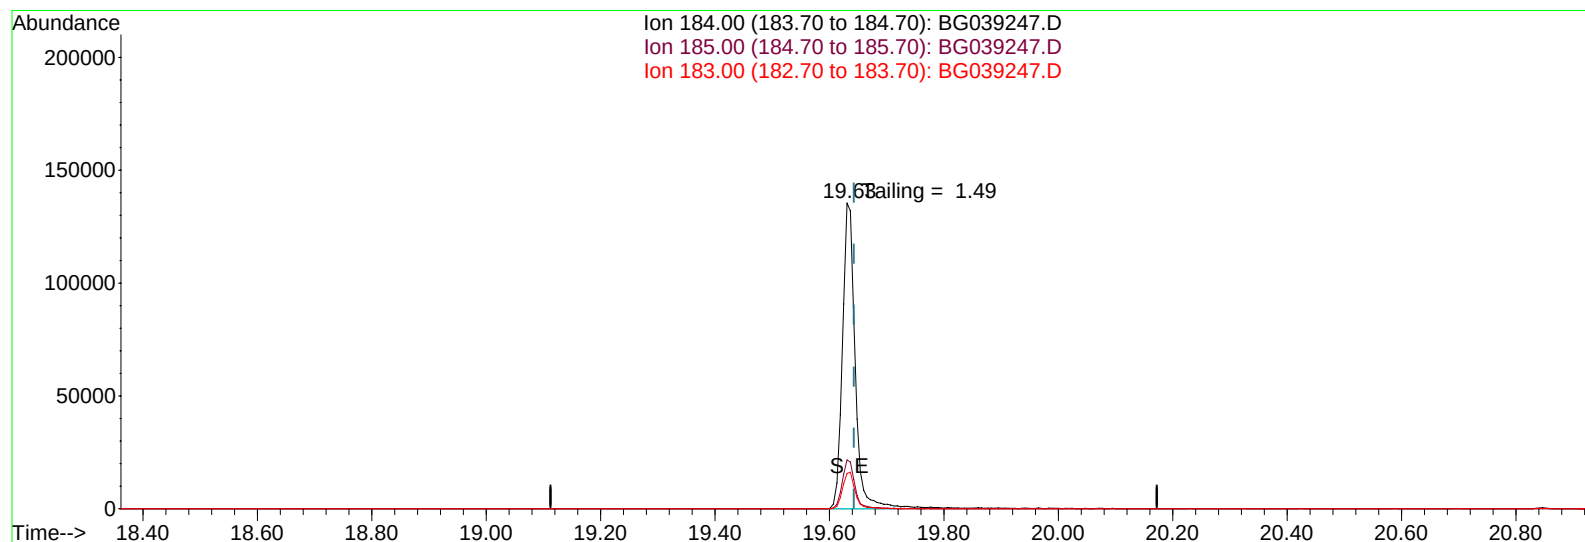

TIC: BG039247.D

(77) Benzidine




19.631min (-0.012) 0.00ng

response 209818

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	15.94
183.00	11.90	11.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG012219\
Data File : BG039247.D
Acq On : 22 Jan 2019 10:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 17:50:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 18 04:20:14 2019
Response via : Initial Calibration

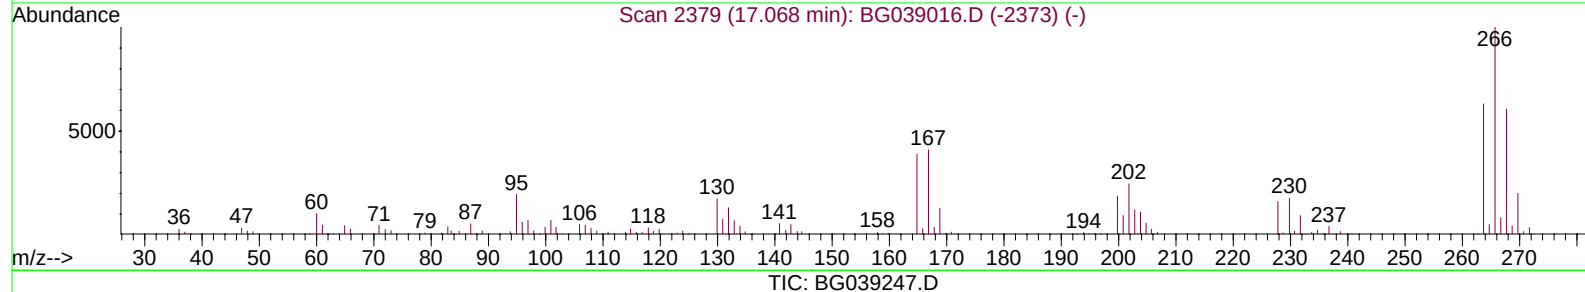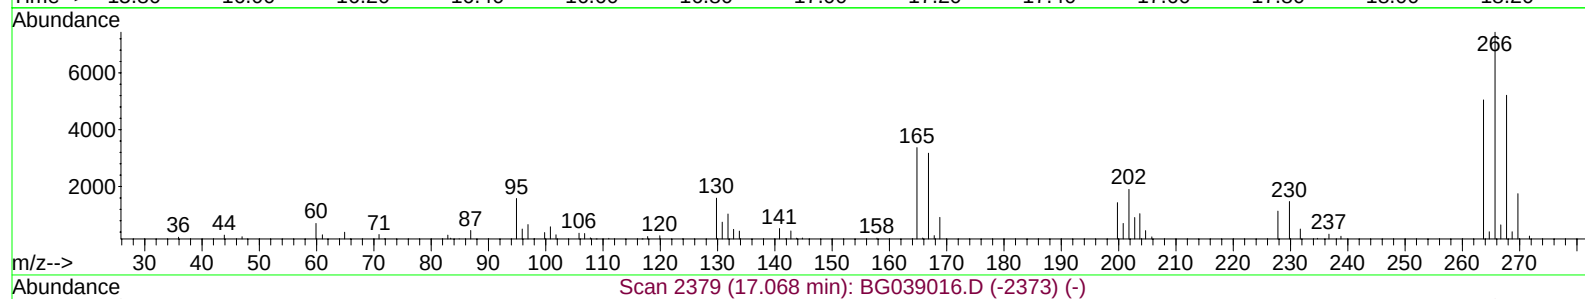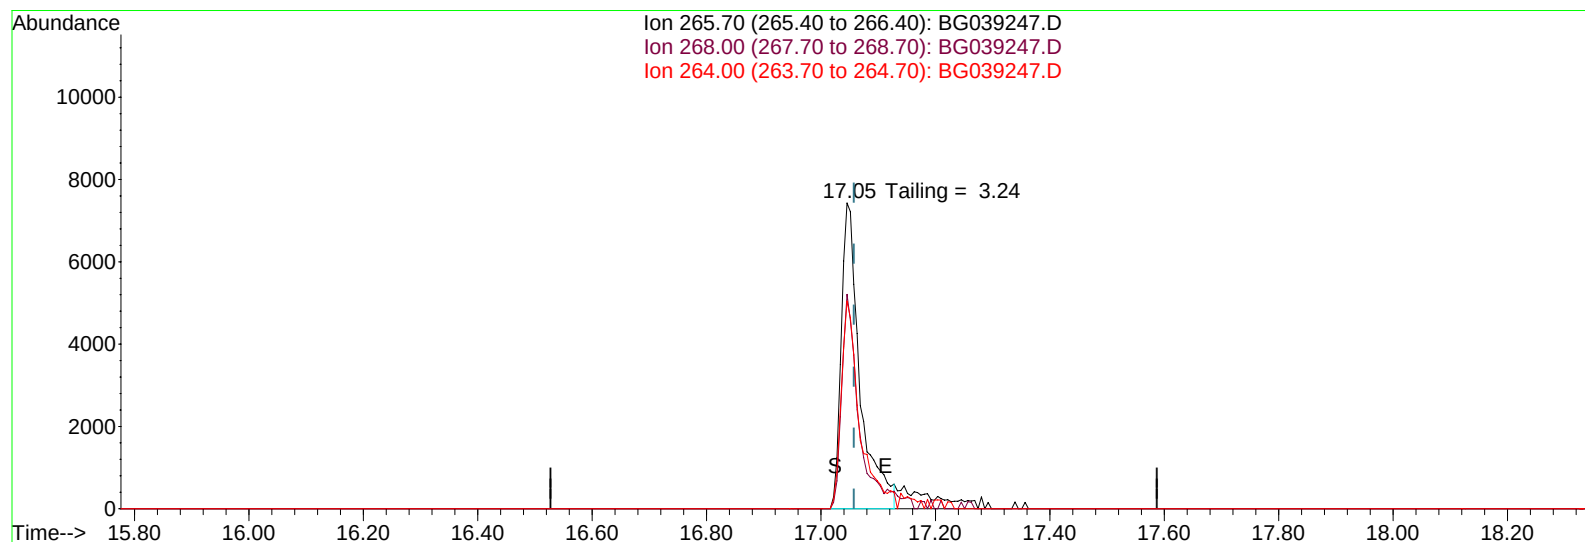

(70) Pentachlorophenol (C)

17.045min (-0.012) 10780.74ng

response 17820

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	75.64
264.00	68.20	73.43
0.00	0.00	0.00