


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012219\
 Data File : BG039247.D
 Acq On : 22 Jan 2019 10:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 18 04:20:14 2019

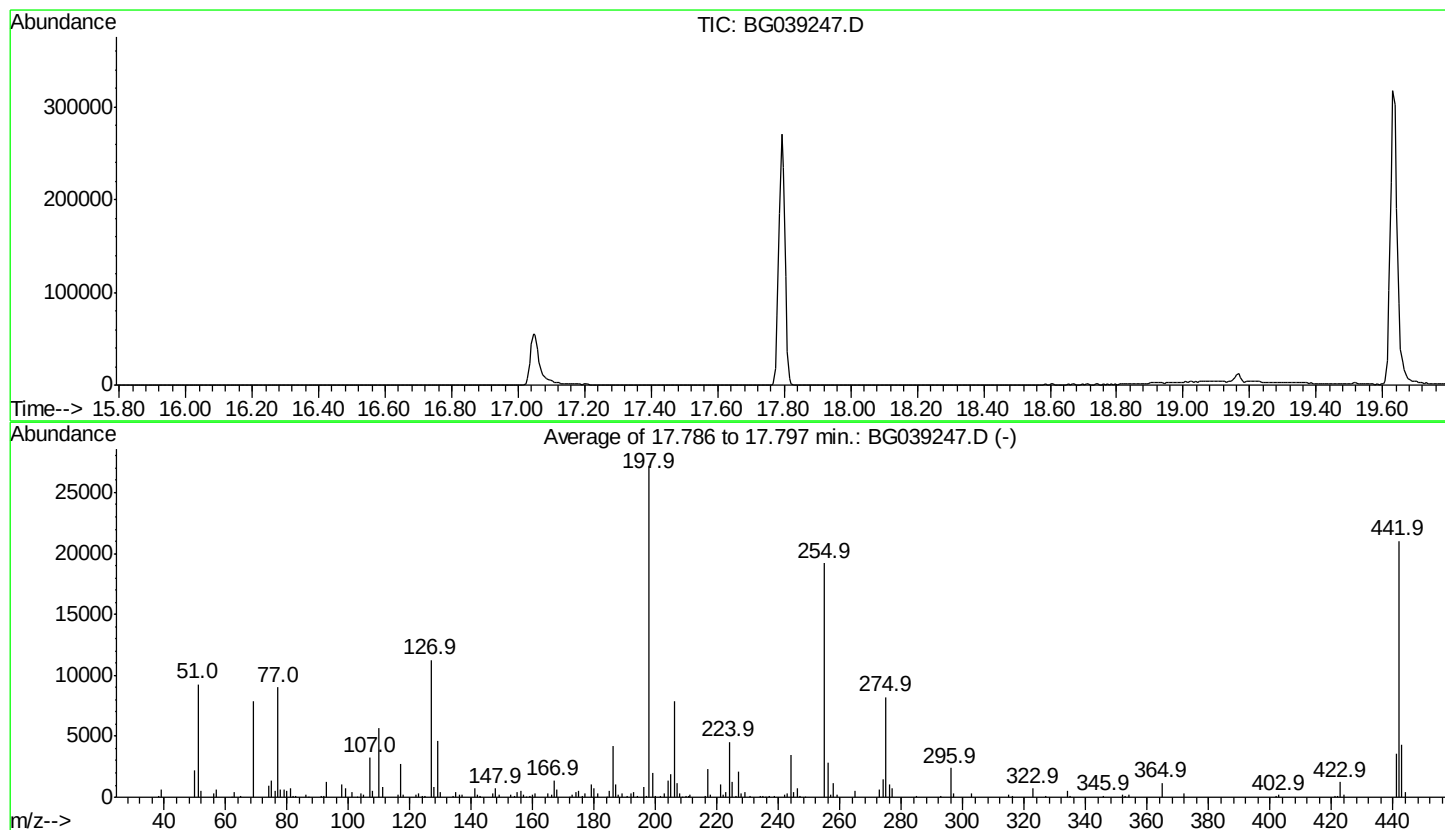

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	9263	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.1	7910	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.4	11269	PASS
197	198	0.00	2	0.4	122	PASS
198	198	100	100	100.0	27202	PASS
199	198	5	9	7.3	1973	PASS
275	198	10	60	30.3	8232	PASS
365	198	1	100	4.4	1196	PASS
441	198	0.01	100	13.0	3546	PASS
442	198	50	100	77.4	21048	PASS
443	442	15	24	20.7	4361	PASS