


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG052020\
 Data File : BG045432.D
 Acq On : 20 May 2020 8:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG051520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 20 14:43:36 2020

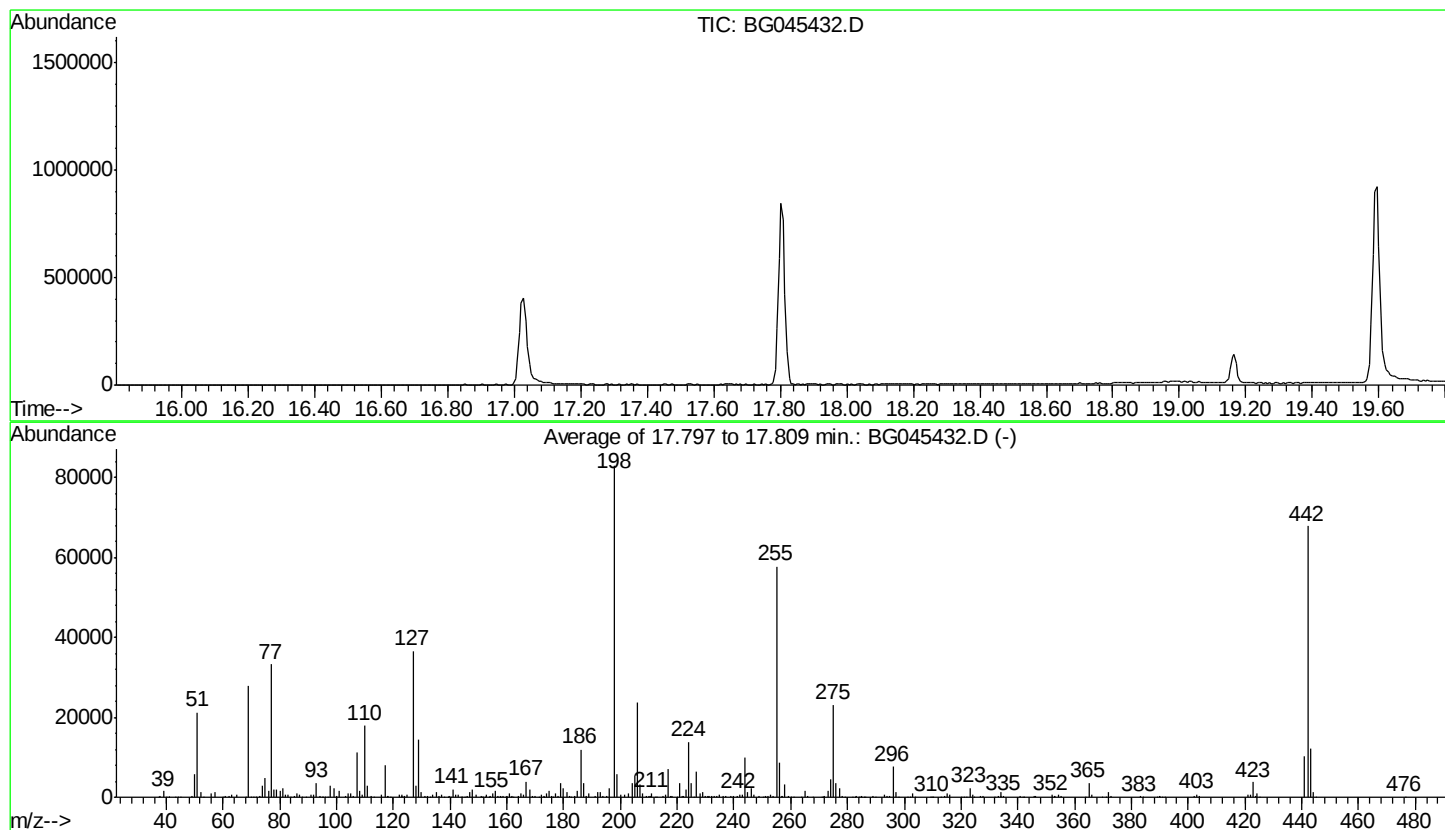

AutoFind: Scans 2504, 2505, 2506; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.6	21221	PASS
68	69	0.00	2	0.6	169	PASS
69	198	0.00	100	33.6	27877	PASS
70	69	0.00	2	0.2	57	PASS
127	198	10	80	44.1	36634	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83026	PASS
199	198	5	9	7.0	5791	PASS
275	198	10	60	27.9	23189	PASS
365	198	1	100	4.4	3616	PASS
441	198	0.01	100	12.3	10225	PASS
442	198	50	100	81.7	67829	PASS
443	442	15	24	18.1	12268	PASS