

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042191.D
 Acq On : 13 Aug 2019 21:41
 Operator : HP/JU
 Sample : K4281-05
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Quant Time: Aug 14 05:04:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 14 02:56:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	74521	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	304127	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	208765	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	423638	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	414987	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	484004	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul	
46) Acenaphthylene-d8	14.69	160	92866	5.02	ng/ul	0.31
51) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
57) Fluorene-d10	15.71	176	249	0.02	ng/ul	0.03
62) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
70) Anthracene-d10	17.44	188	423638	20.84	ng/ul	-0.10
78) Pyrene-d10	0.00	212	0	0.00	ng/ul	
89) Benzo(a)pyrene-d12	24.99	264	484004	19.14	ng/ul	0.23


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.69	163	44566	2.772	ng/ul#	1
45) 2,6-Dinitrotoluene	14.69	165	27408	7.838	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042191.D
Acq On : 13 Aug 2019 21:41
Operator : HP/JU
Sample : K4281-05
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Time: Aug 14 05:04:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 02:56:59 2019
Response via : Initial Calibration

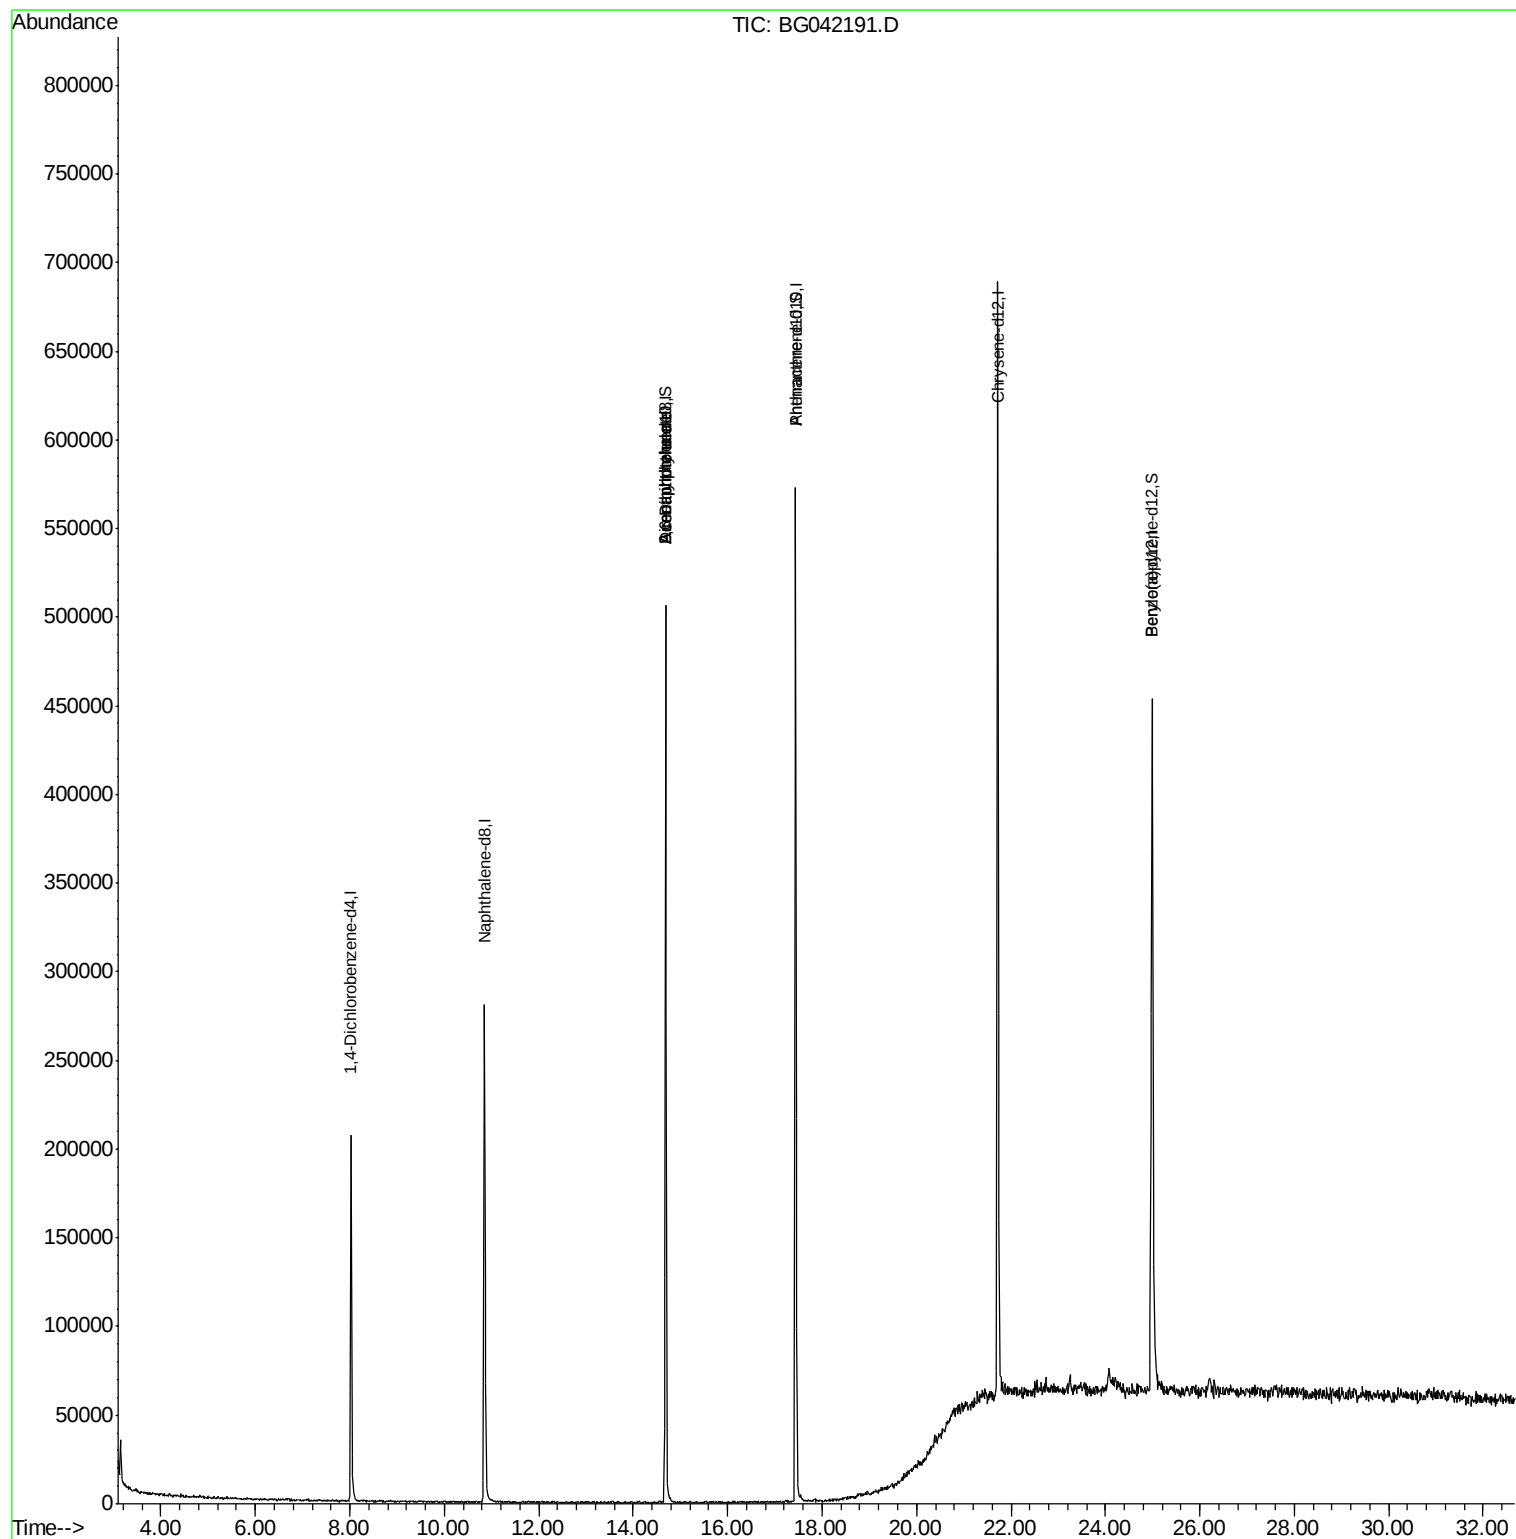


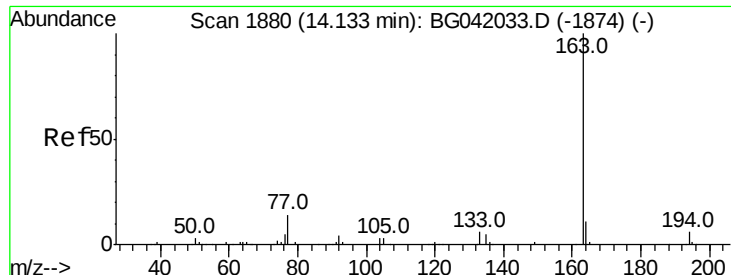




#44
Dimethylphthalate
Concen: 2.772 ng/ul
RT: 14.69 min Scan# 1974
Delta R.T. 0.56 min
Lab File: BG042191.D
Acq: 13 Aug 2019 21:41

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Tot Ion:163 Resp: 44566
Ion Ratio Lower Upper
163 100
194 0.0 4.2 6.2#
164 489.6 7.8 11.8#

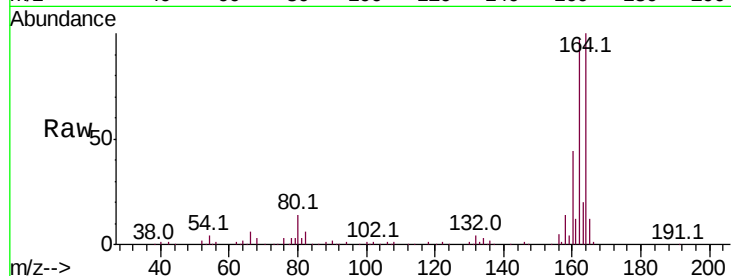


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

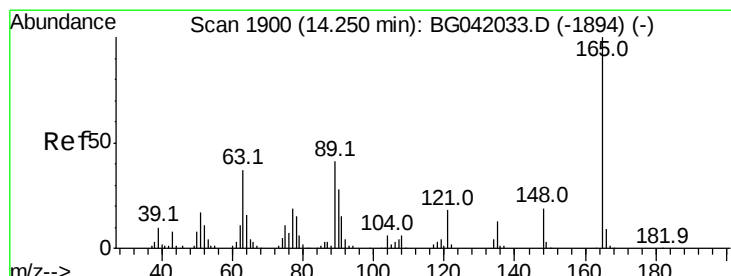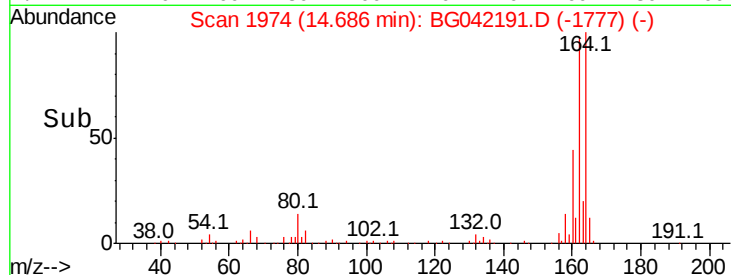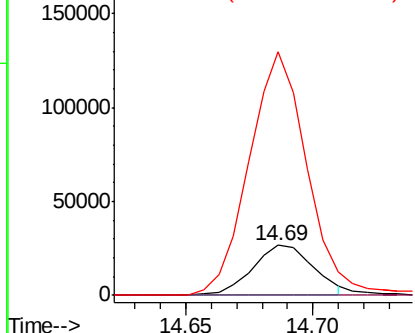

#45
2,6-Dinitrotoluene
Concen: 7.838 ng/ul
RT: 14.69 min Scan# 1974
Delta R.T. 0.43 min
Lab File: BG042191.D
Acq: 13 Aug 2019 21:41

Tgt Ion:165 Resp: 27408
Ion Ratio Lower Upper
165 100
89 0.0 36.8 55.2#
121 0.0 15.6 23.4#

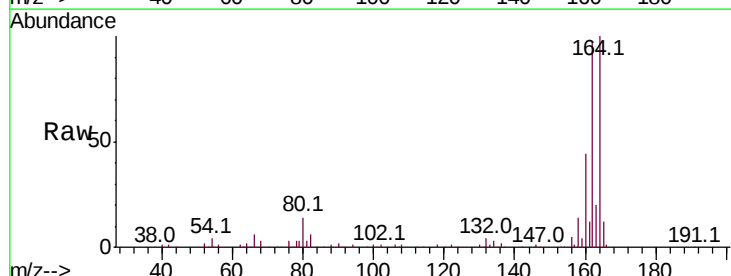

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 89.00 (88.70 to 89.70): BG
Ion 121.00 (120.70 to 121.70): E

