

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042154.D
 Acq On : 12 Aug 2019 20:17
 Operator : HP/JU
 Sample : K4161-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ETOE6

Quant Time: Aug 13 12:37:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 13 04:44:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	101259	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	416712	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	282330	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	579332	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	595363	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	670977	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	9995	4.32	ng/uL	0.00
5) Phenol-d5	7.18	99	66328	8.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	114024	25.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	179409	26.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	118700	17.79	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	105705	33.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	130792	35.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	238529	32.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	26048	3.19	ng/ul	0.00
43) Dimethylphthalate-d6	14.09	166	724766	33.10	ng/ul	0.00
46) Acenaphthylene-d8	14.37	160	829763	33.17	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	29597	8.05	ng/ul	0.00
57) Fluorene-d10	15.68	176	631977	32.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	122405	32.93	ng/ul	0.00
70) Anthracene-d10	17.54	188	956956	34.43	ng/ul	0.00
78) Pyrene-d10	19.82	212	1087809	32.74	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	1264165	36.07	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	14.13	163	27572	1.268	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042154.D
Acq On : 12 Aug 2019 20:17
Operator : HP/JU
Sample : K4161-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
ETOE6

Quant Time: Aug 13 12:37:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 13 04:44:41 2019
Response via : Initial Calibration

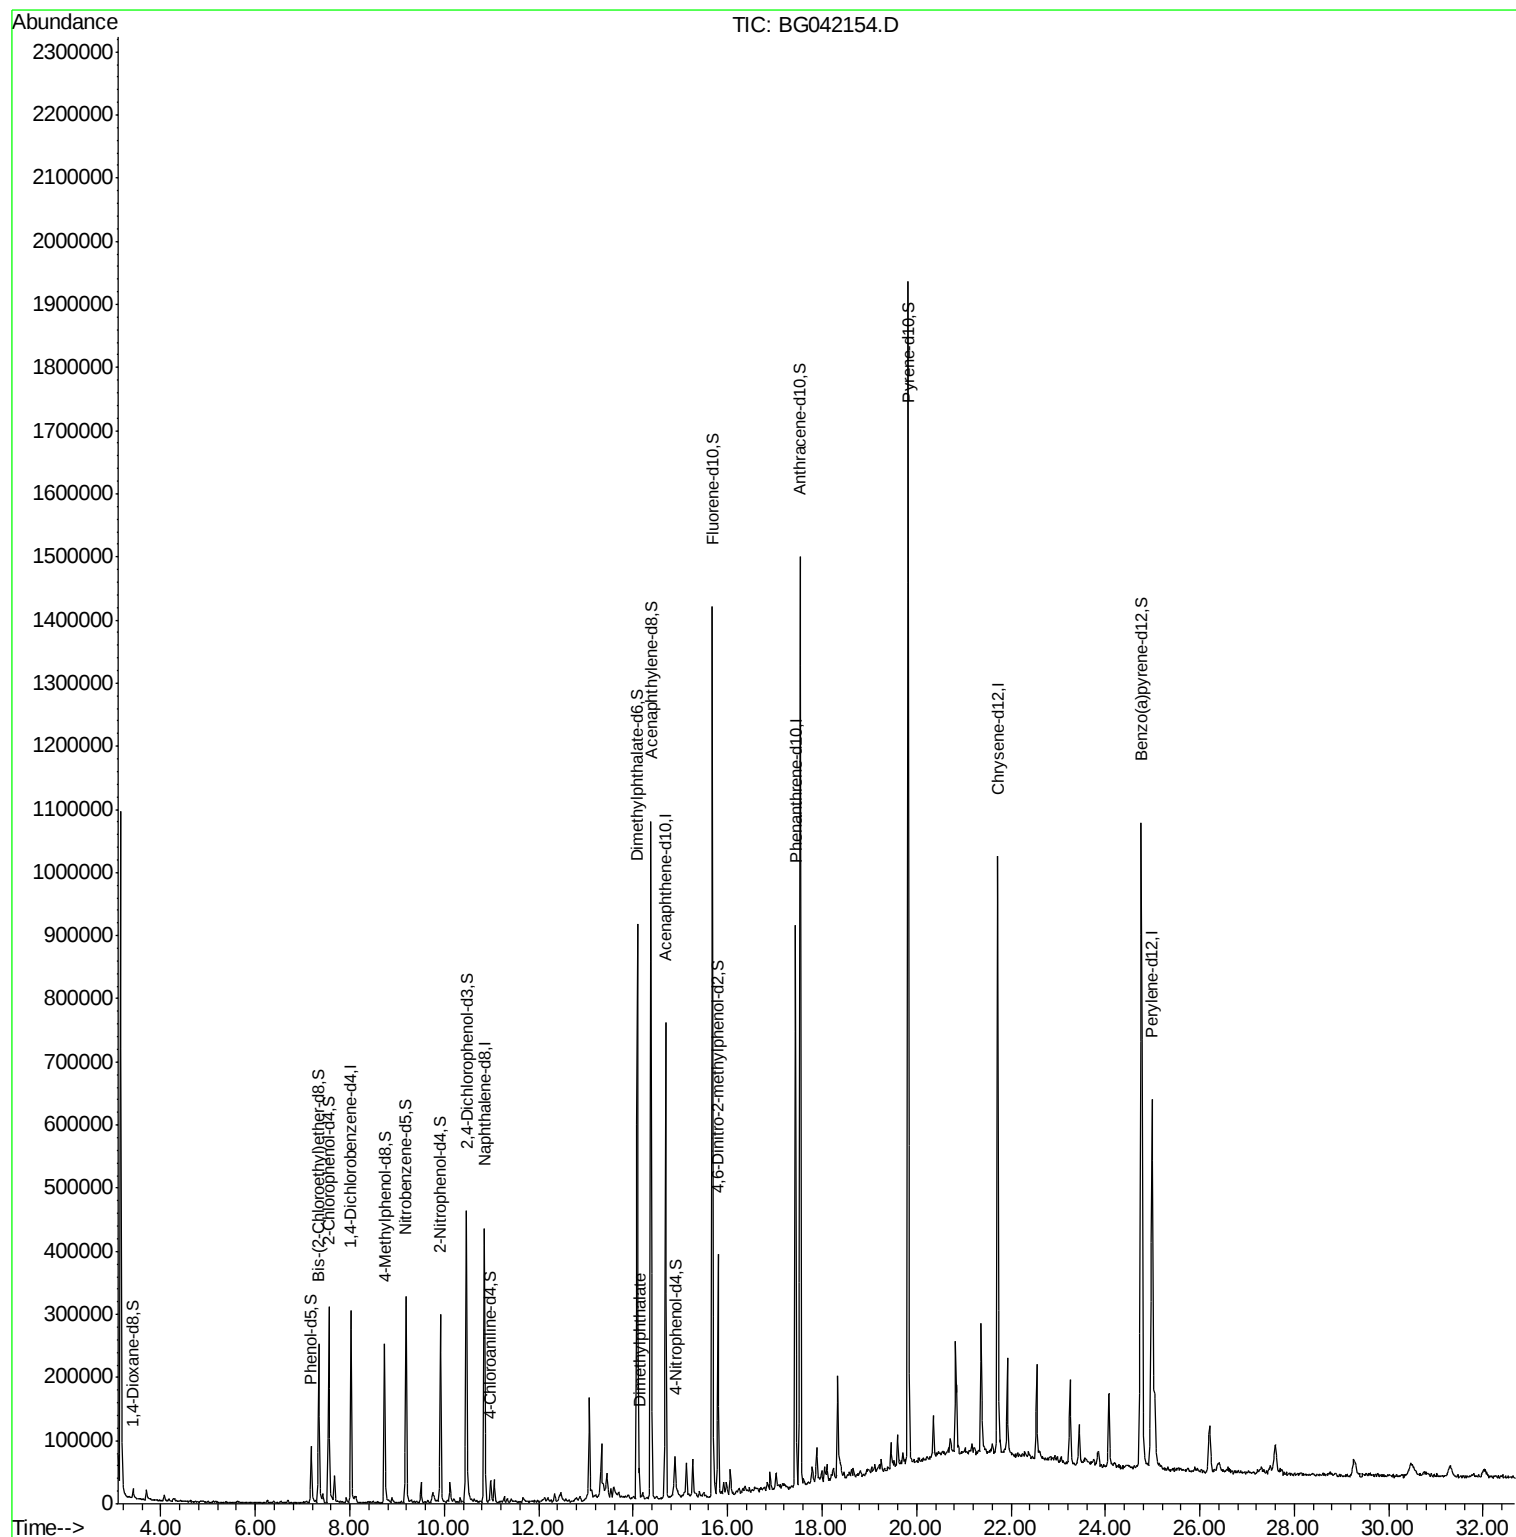

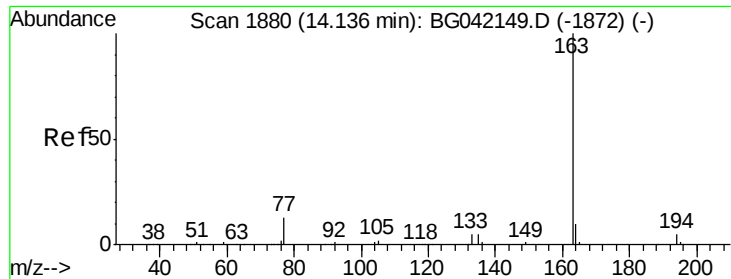

#44

Dimethylphthalate

Concen: 1.268 ng/ul

RT: 14.13 min Scan# 1879

Delta R.T. -0.00 min

Lab File: BG042154.D

Acq: 12 Aug 2019 20:17

Instrument :

BNA_G

ClientSampleId :

ETOE6


Tot Ion:163 Resp: 27572

Ion Ratio Lower Upper

163 100

194 5.7 4.2 6.2

164 11.4 7.8 11.8

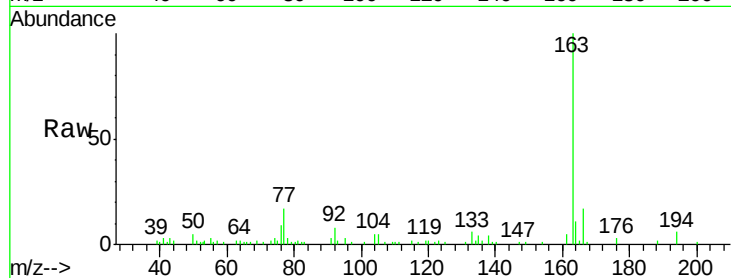

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

