

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042171.D
 Acq On : 13 Aug 2019 8:48
 Operator : HP/JU
 Sample : K4117-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JLLD8

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:50:50 AM

Quant Time: Aug 13 13:39:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 13 04:44:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	79485	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	330624	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.68	164	228771	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.43	188	490906m	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	493106	20.00	ng/ul	0.00
85) Perylene-d12	24.98	264	516691	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	6667	3.67	ng/uL	0.00
5) Phenol-d5	7.18	99	155976	25.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	77497	22.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	142019	26.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	131603	25.13	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	69377	27.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	86352	29.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	162098	27.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	194491	30.05	ng/ul	0.00
43) Dimethylphthalate-d6	14.09	166	482818	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.37	160	564824	27.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.88	143	55363	18.58	ng/ul	0.00
57) Fluorene-d10	15.68	176	430716	27.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	53437m	16.97	ng/ul	0.00
70) Anthracene-d10	17.53	188	662836	28.14	ng/ul	0.00
78) Pyrene-d10	19.82	212	748623	27.21	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	799432	29.62	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.13	163	201074	11.414	ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042171.D
Acq On : 13 Aug 2019 8:48
Operator : HP/JU
Sample : K4117-01
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JLLD8

Manual Integrations
APPROVED

mohammad
8/14/2019 2:50:50 AM

Quant Time: Aug 13 13:39:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 13 04:44:41 2019
Response via : Initial Calibration

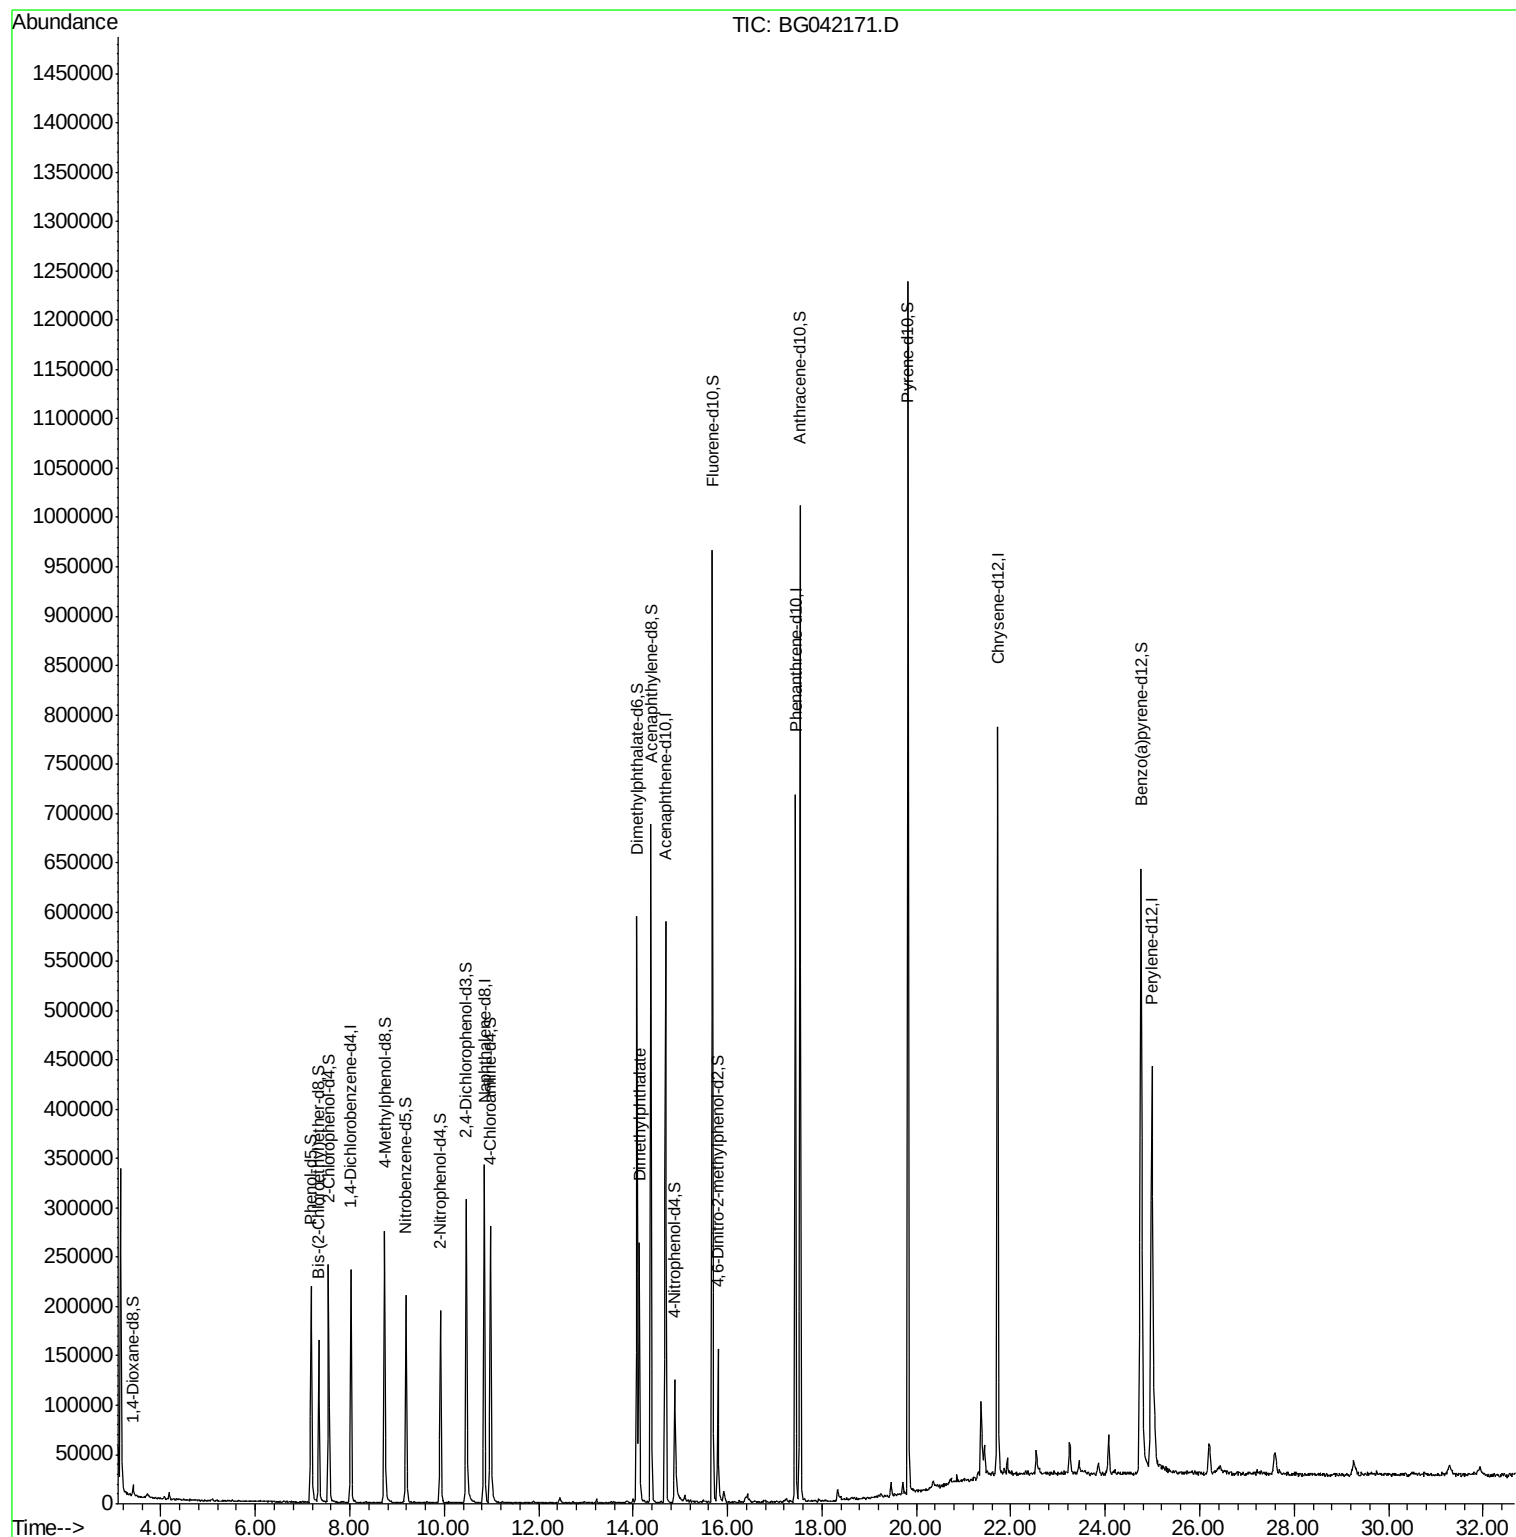

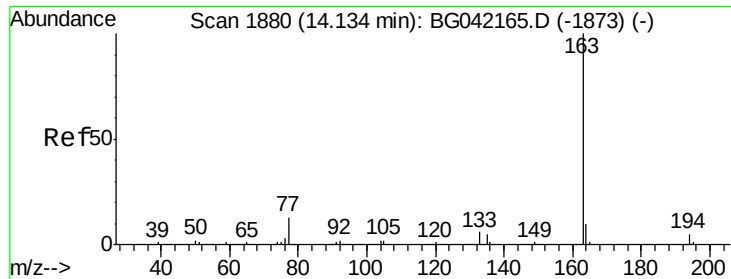

#44
 Dimethylphthalate
 Concen: 11.414 ng/ul
 RT: 14.13 min Scan# 1880
 Delta R.T. 0.00 min
 Lab File: BG042171.D
 Acq: 13 Aug 2019 8:48

Instrument :
 BNA_G
 ClientSampleId :
 JLLD8

Tot Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	5.1	4.2	6.2
164	11.3	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 8/14/2019 2:50:50 AM

