

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042174.D
 Acq On : 13 Aug 2019 10:44
 Operator : HP/JU
 Sample : K4117-07
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JLLF5

Quant Time: Aug 13 13:27:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 13 04:44:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	81211	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	332052	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.68	164	231466	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.43	188	493091	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	504879	20.00	ng/ul	0.00
85) Perylene-d12	24.98	264	530601	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	7177	3.87	ng/uL	0.00
5) Phenol-d5	7.18	99	157993	24.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	78982	22.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	144622	26.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	135543	25.33	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	70771	28.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	86140	29.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	164325	28.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	198776	30.57	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	492006	27.41	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	576211	28.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.88	143	54488	18.08	ng/ul	0.00
57) Fluorene-d10	15.68	176	439881	27.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.79	200	54999	17.38	ng/ul	0.00
70) Anthracene-d10	17.53	188	674007	28.49	ng/ul	0.00
78) Pyrene-d10	19.82	212	764436	27.13	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	823339	29.70	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.13	163	193100	10.834	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042174.D
Acq On : 13 Aug 2019 10:44
Operator : HP/JU
Sample : K4117-07
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JLLF5

Quant Time: Aug 13 13:27:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 13 04:44:41 2019
Response via : Initial Calibration

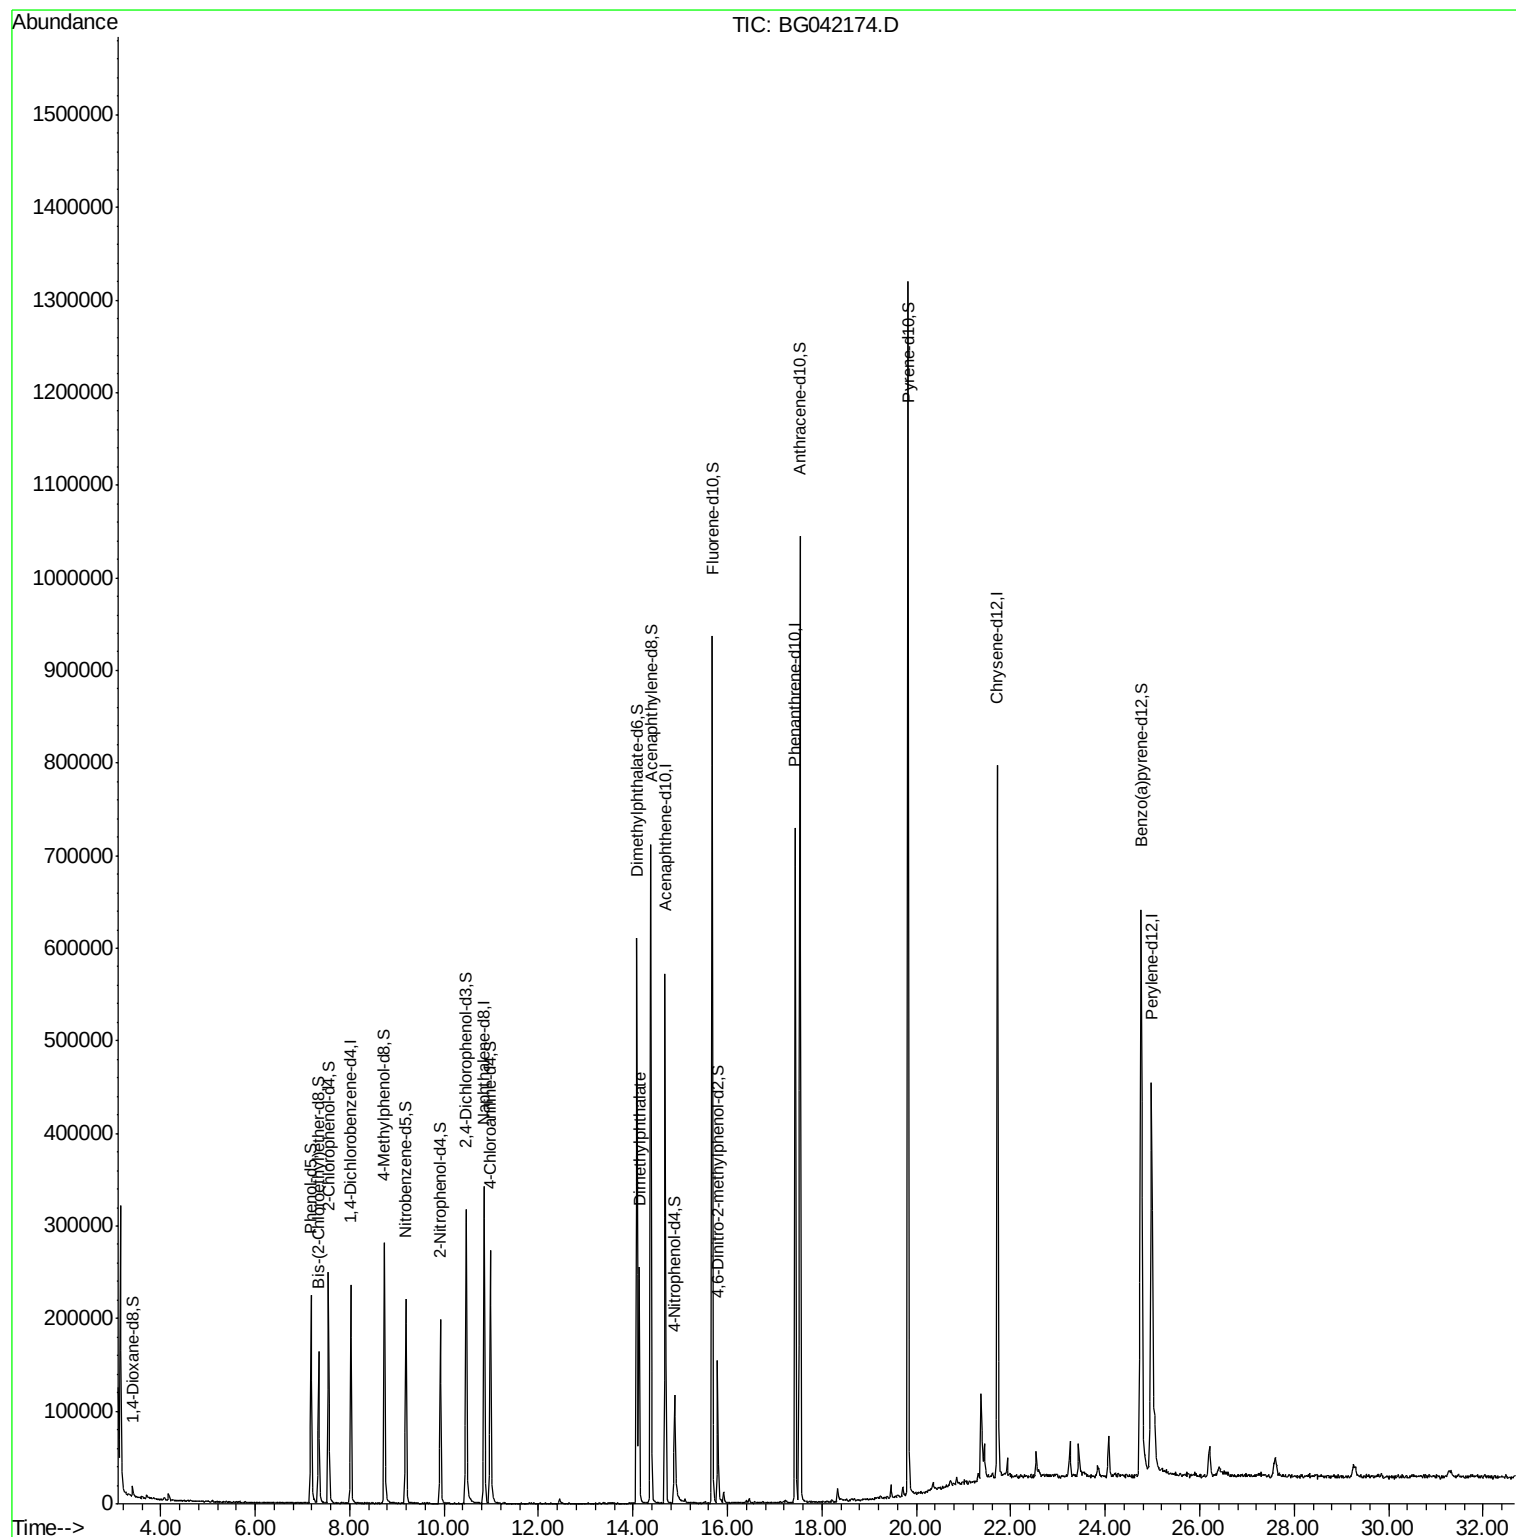

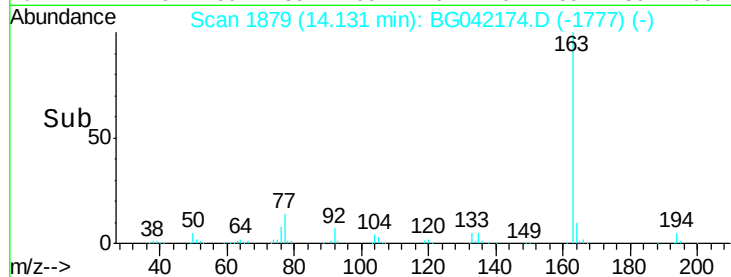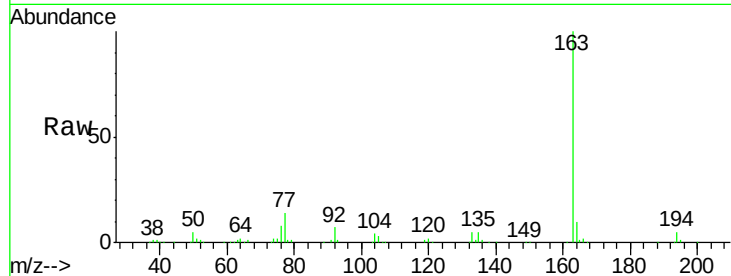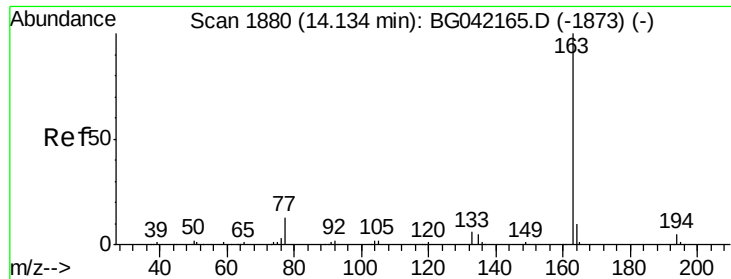

#44

Dimethylphthalate

Concen: 10.834 ng/ul

RT: 14.13 min Scan# 1879

Delta R.T. 0.00 min

Lab File: BG042174.D

Acq: 13 Aug 2019 10:44

Instrument :

BNA_G

ClientSampleId :

JLLF5

Tot Ion:163 Resp: 193100

Ion Ratio Lower Upper

163 100

194 4.9 4.2 6.2

164 10.3 7.8 11.8

