

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042176.D
 Acq On : 13 Aug 2019 12:01
 Operator : HP/JU
 Sample : K4117-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JLLF7

Quant Time: Aug 13 13:23:25 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 13 04:44:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	80826	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	334284	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.68	164	231899	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	496137	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	503711	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	522770	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	7275	3.94	ng/uL	0.00
5) Phenol-d5	7.18	99	153556	24.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	79151	22.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	142724	26.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	130325	24.47	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	68223	27.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	86594	29.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	163031	27.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	193100	29.50	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	477426	26.55	ng/ul	0.00
46) Acenaphthylene-d8	14.37	160	561055	27.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.88	143	55154	18.26	ng/ul	0.00
57) Fluorene-d10	15.68	176	430498	26.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	56947	17.89	ng/ul	0.00
70) Anthracene-d10	17.54	188	660577	27.75	ng/ul	0.00
78) Pyrene-d10	19.82	212	750291	26.69	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	788935	28.89	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.13	163	247592	13.865	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042176.D
Acq On : 13 Aug 2019 12:01
Operator : HP/JU
Sample : K4117-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JLLF7

Quant Time: Aug 13 13:23:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 13 04:44:41 2019
Response via : Initial Calibration

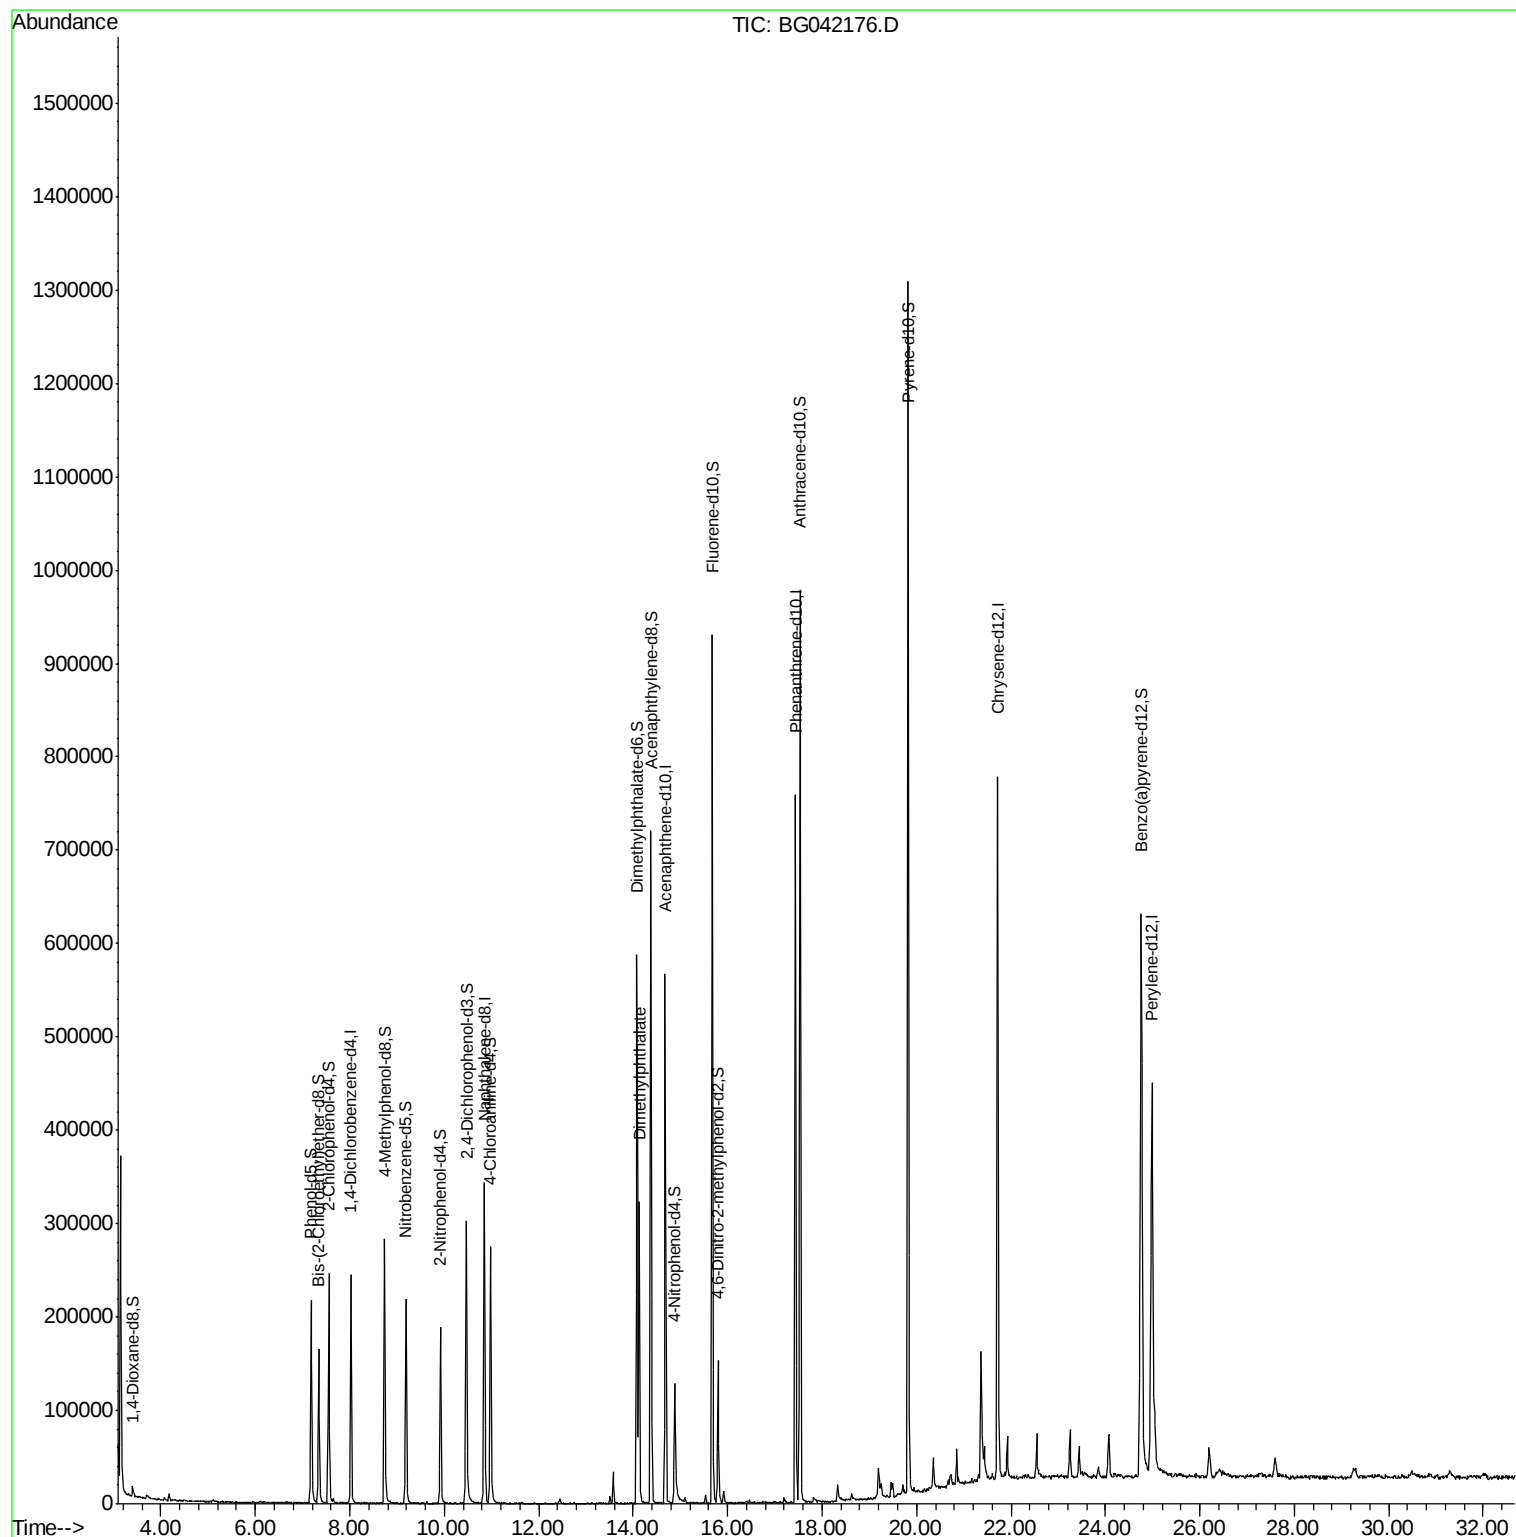

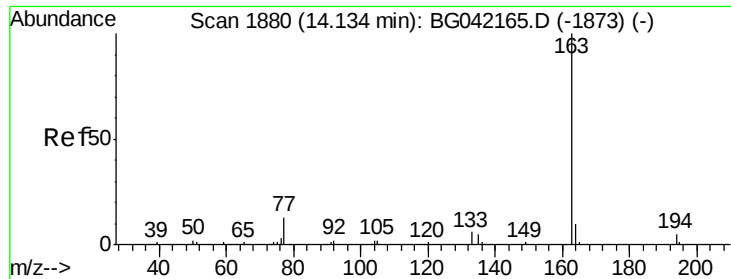

#44

Dimethylphthalate

Concen: 13.865 ng/ul

RT: 14.13 min Scan# 1879

Delta R.T. -0.00 min

Lab File: BG042176.D

Acq: 13 Aug 2019 12:01

Instrument :

BNA_G

ClientSampleId :

JLLF7


Tot Ion:163 Resp: 247592

Ion Ratio Lower Upper

163 100

194 4.8 4.2 6.2

164 10.7 7.8 11.8

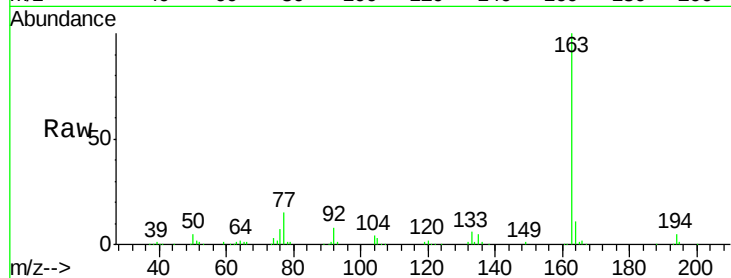

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

