

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042177.D
 Acq On : 13 Aug 2019 12:39
 Operator : HP/JU
 Sample : K4117-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JLLF8

Quant Time: Aug 13 13:21:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 13 04:44:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.02	152	82274	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	341311	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	235294	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	500251	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	505507	20.00	ng/ul	0.00
85) Perylene-d12	24.98	264	525039	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.40	96	4057	2.16	ng/uL	0.00
5) Phenol-d5	7.18	99	101983	15.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	52457	14.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	92939	16.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	77910	14.37	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	44995	17.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	56568	18.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	102569	17.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	122223	18.29	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	347386	19.04	ng/ul	0.00
46) Acenaphthylene-d8	14.37	160	396753	19.03	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	36666	11.97	ng/ul	0.00
57) Fluorene-d10	15.68	176	310074	19.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	33670	10.49	ng/ul	0.00
70) Anthracene-d10	17.54	188	477118	19.88	ng/ul	0.00
78) Pyrene-d10	19.82	212	572439	20.29	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.76	264	596583	21.75	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	14.13	163	137784	7.604	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042177.D
Acq On : 13 Aug 2019 12:39
Operator : HP/JU
Sample : K4117-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JLLF8

Quant Time: Aug 13 13:21:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 13 04:44:41 2019
Response via : Initial Calibration

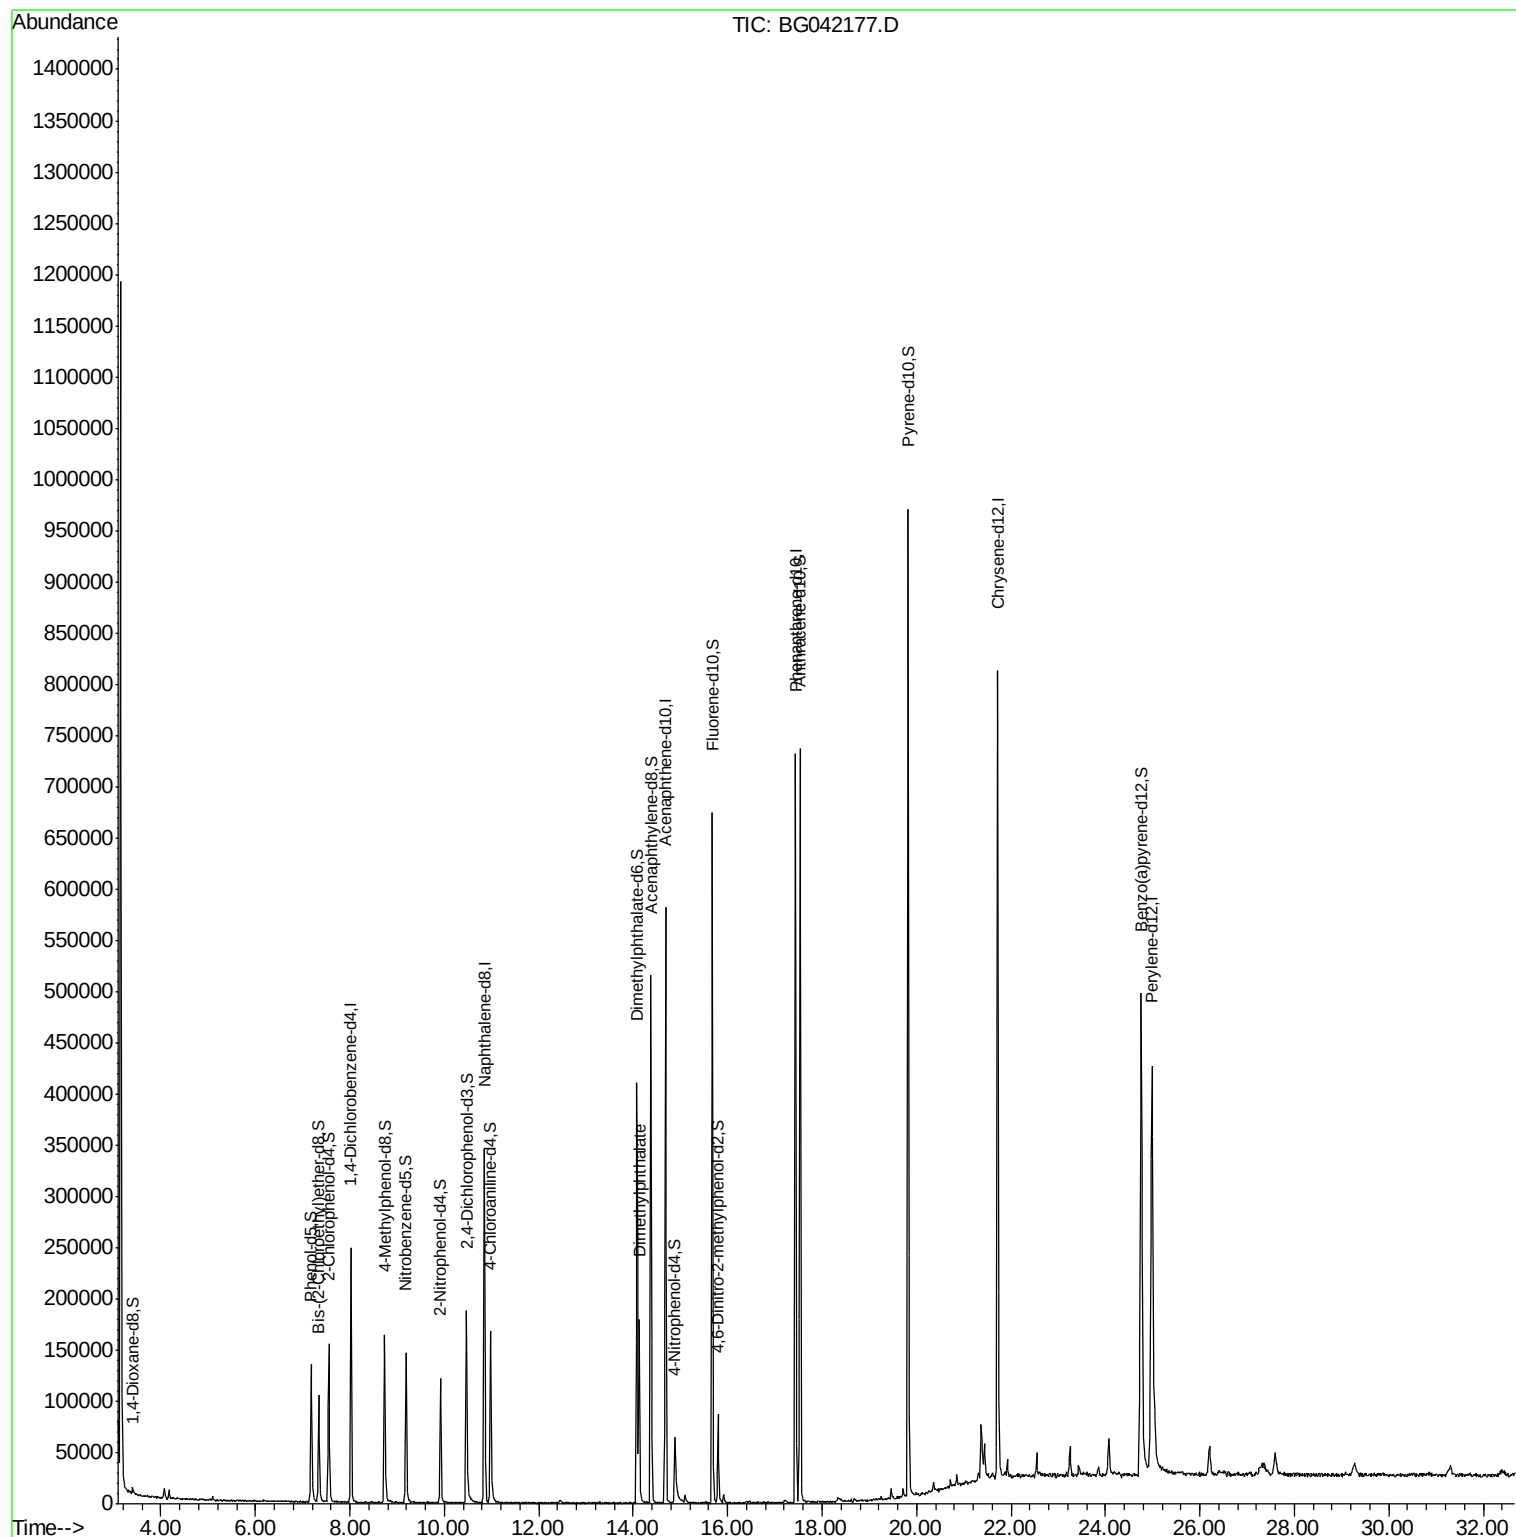

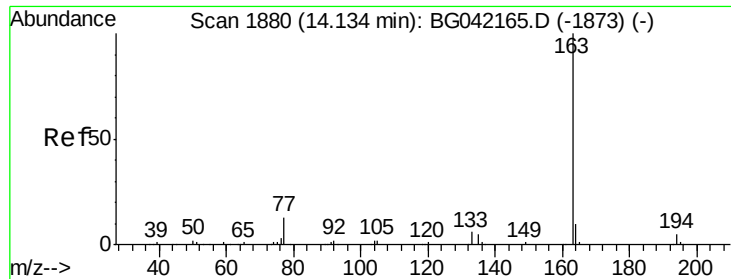

#44

Dimethylphthalate

Concen: 7.604 ng/ul

RT: 14.13 min Scan# 1879

Delta R.T. -0.00 min

Lab File: BG042177.D

Acq: 13 Aug 2019 12:39

Instrument :

BNA_G

ClientSampleId :

JLLF8

Tot Ion:163 Resp: 137784

Ion Ratio Lower Upper

163 100

194 4.6 4.2 6.2

164 11.0 7.8 11.8

