

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
 Data File : BG042186.D
 Acq On : 13 Aug 2019 18:28
 Operator : HP/JU
 Sample : K4215-12
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 ETOC3

Manual Integrations
 APPROVED

mohammad
 8/20/2019 8:35:57 AM

Quant Time: Aug 14 05:45:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 14 02:56:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	79220	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	321773	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.69	164	220304	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.44	188	447588	20.00	ng/ul	0.00
77) Chrysene-d12	21.72	240	431146	20.00	ng/ul	0.00
85) Perylene-d12	24.99	264	516583	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.41	96	4112	2.27	ng/uL	0.00
5) Phenol-d5	7.18	99	91605	14.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.34	67	46754	13.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	87503	16.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	75856	14.53	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	41245	17.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	51692	18.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	97083	17.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	107700	17.10	ng/ul	0.00
43) Dimethylphthalate-d6	14.08	166	321325	18.81	ng/ul	0.00
46) Acenaphthylene-d8	14.38	160	364710	18.69	ng/ul	0.00
51) 4-Nitrophenol-d4	14.89	143	33214	11.58	ng/ul	0.00
57) Fluorene-d10	15.68	176	283191	18.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.80	200	29758	10.36	ng/ul	0.00
70) Anthracene-d10	17.54	188	454050	21.14	ng/ul	0.00
78) Pyrene-d10	19.82	212	549177	22.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.77	264	643510	23.85	ng/ul	0.00

Target Compounds

					Ovalue	
6) Phenol	7.21	94	9705	1.512	ng/ul#	91
44) Dimethylphthalate	14.13	163	98378	5.799	ng/ul	98
69) Phenanthrene	17.48	178	29173	1.191	ng/ul	98
76) Fluoranthene	19.49	202	61693m	2.179	ng/ul	
79) Pyrene	19.85	202	55806	1.924	ng/ul#	95
82) Benzo(a)anthracene	21.70	228	40998	1.371	ng/ul	97
84) Chrysene	21.77	228	37622m	1.348	ng/ul	
87) Benzo(b)fluoranthene	23.95	252	61086	1.884	ng/ul	98
90) Benzo(a)pyrene	24.84	252	44218	1.431	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081219\
Data File : BG042186.D
Acq On : 13 Aug 2019 18:28
Operator : HP/JU
Sample : K4215-12
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
ETOC3

Quant Time: Aug 14 05:45:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 14 02:56:59 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
8/20/2019 8:35:57 AM

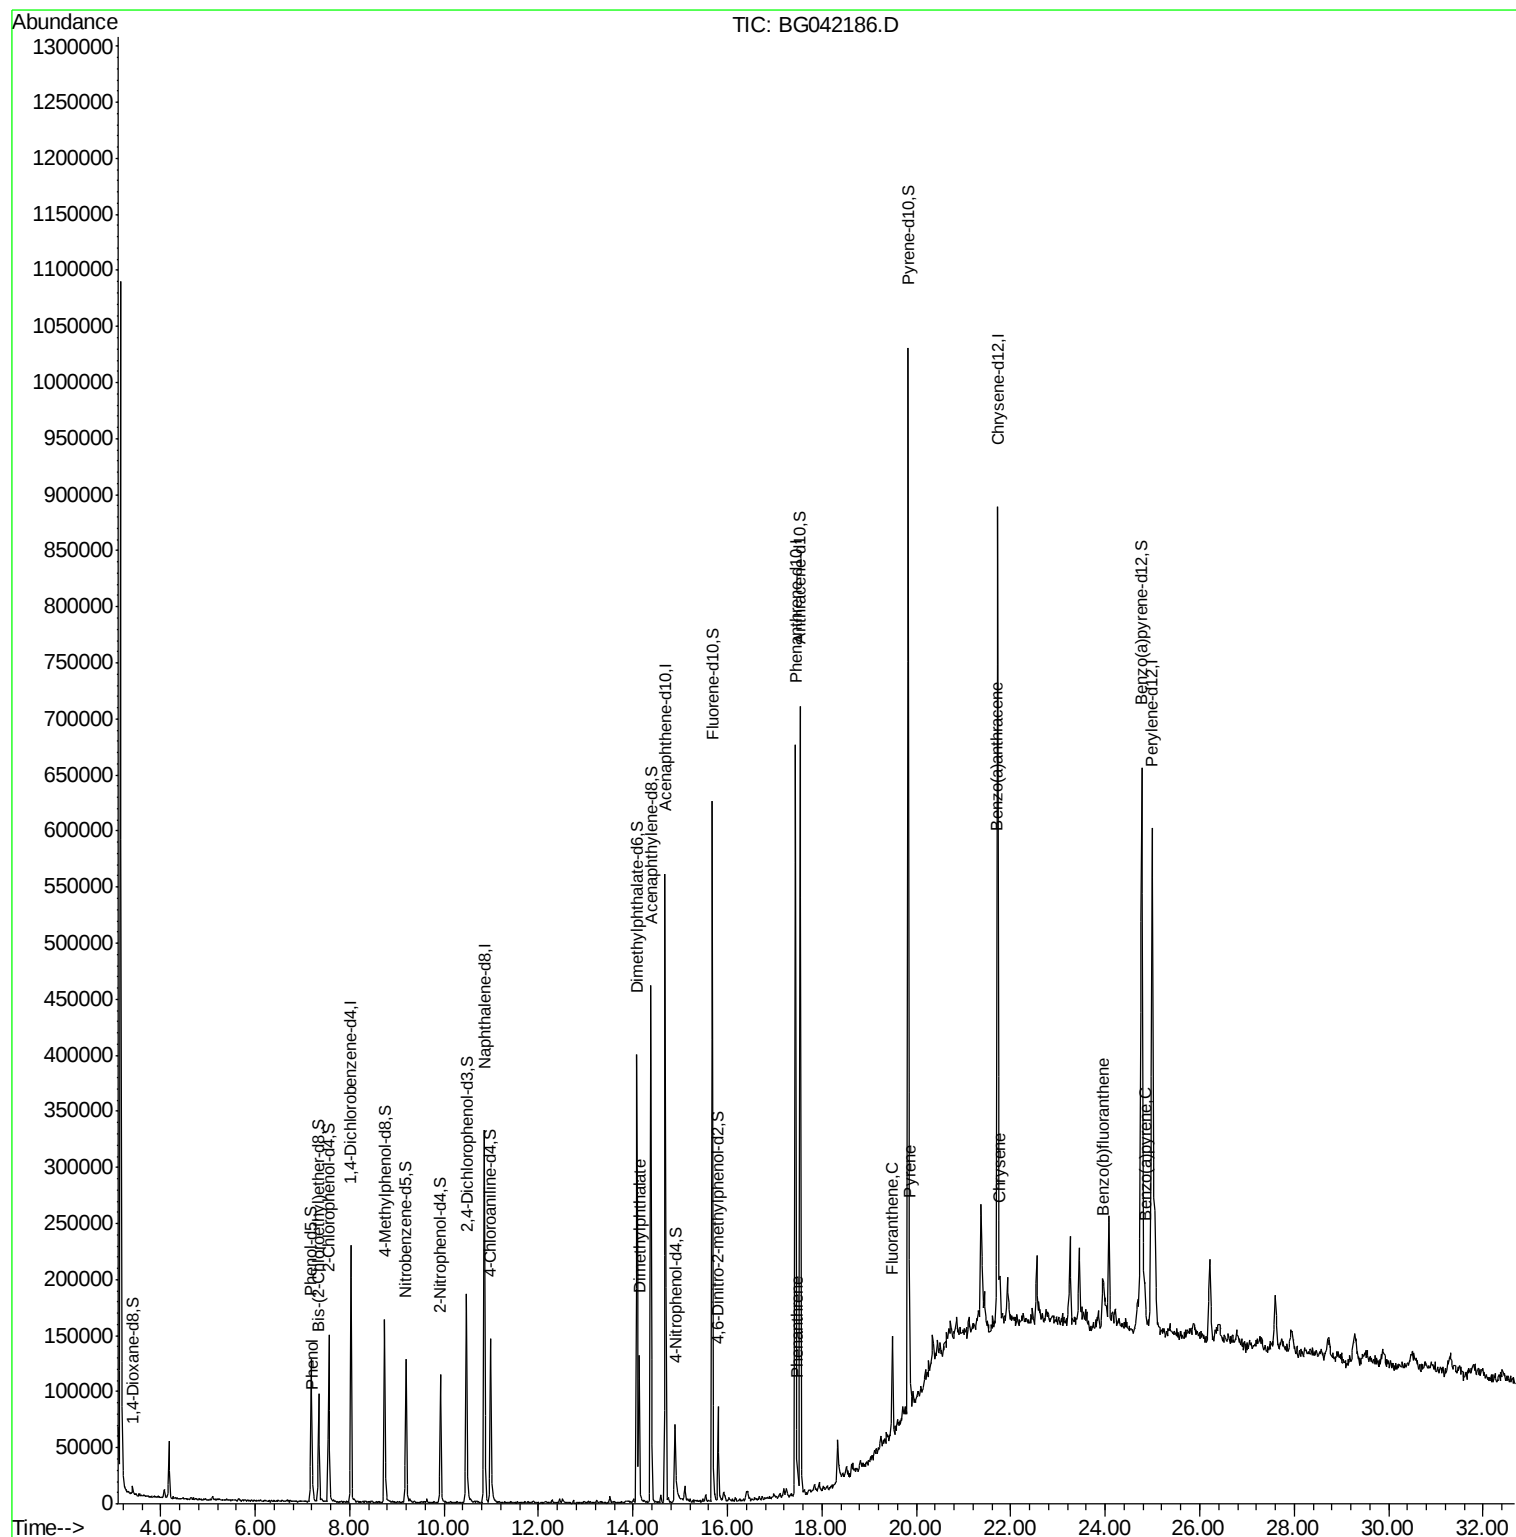

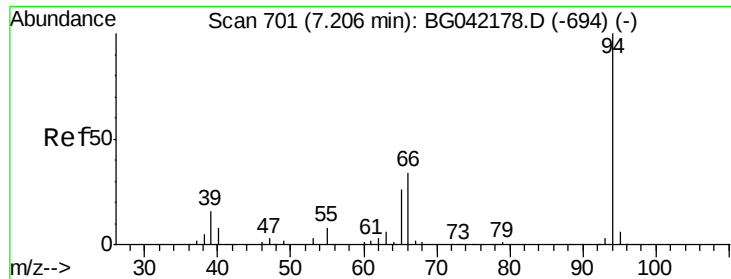

#6

Phenol





Concen: 1.512 ng/ul
 RT: 7.21 min Scan# 701
 Delta R.T. 0.00 min
 Lab File: BG042186.D
 Acq: 13 Aug 2019 18:28

Instrument :
 BNA_G
 ClientSampleId :
 ETOC3

Tot Ion	Ion	Ratio	Lower	Upper
94	100			
65	31.2	25.8	38.6	
66	48.7	31.8	47.8	

Manual Integrations
 APPROVED

mohammad
 8/20/2019 8:35:57 AM

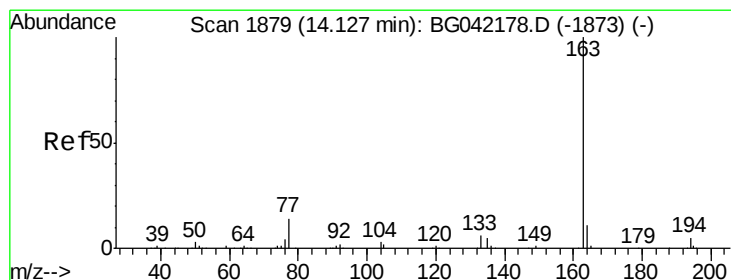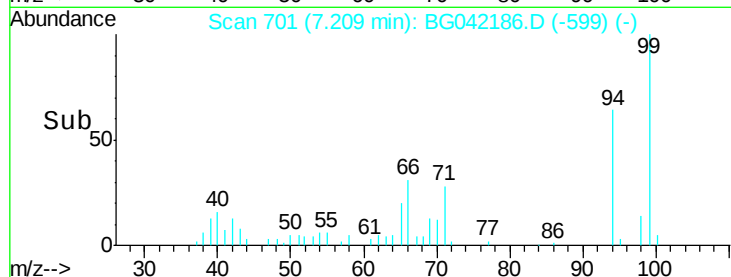
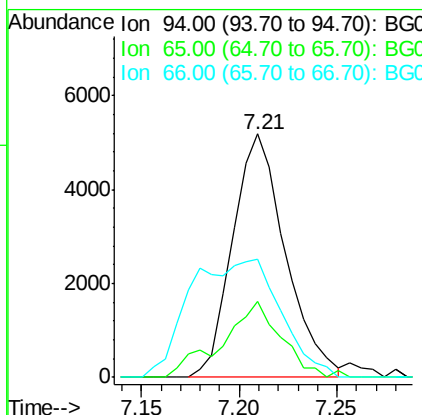
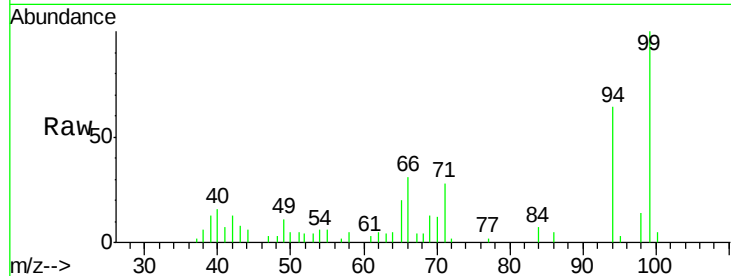



#44

Dimethylphthalate

Concen: 5.799 ng/ul
 RT: 14.13 min Scan# 1879
 Delta R.T. 0.00 min
 Lab File: BG042186.D
 Acq: 13 Aug 2019 18:28

Tgt Ion	Ion	Ratio	Lower	Upper
163	100			
194	4.5	4.2	6.2	
164	10.3	7.8	11.8	

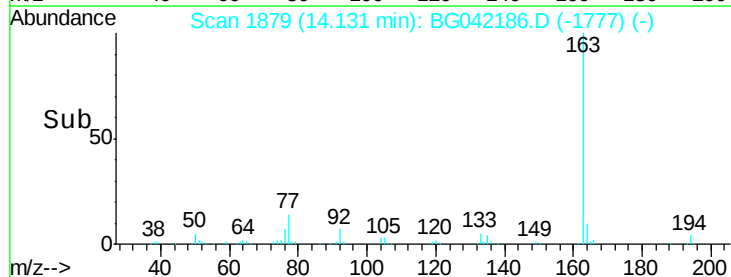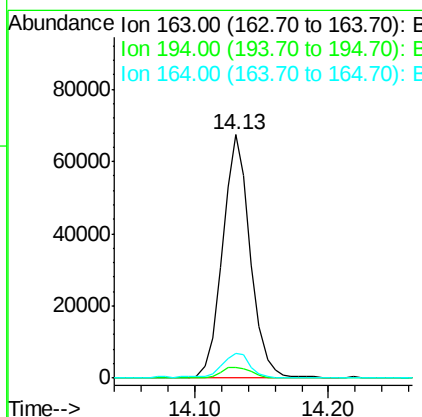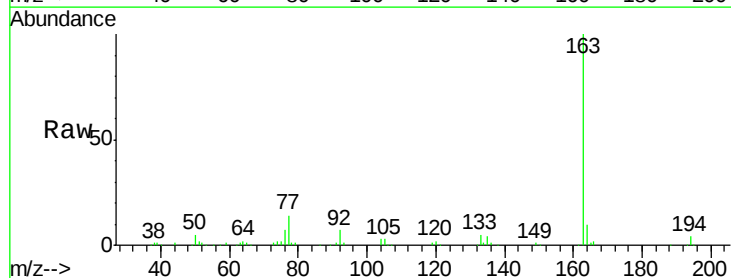

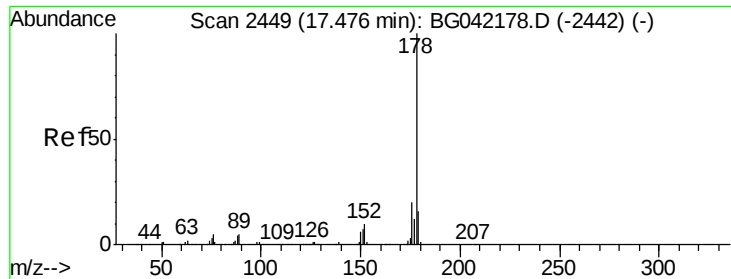





#69
Phenanthrene
Concen: 1.191 ng/ul
RT: 17.48 min Scan# 2449
Delta R.T. 0.00 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Instrument :
BNA_G
ClientSampled :
ETOC3

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.8	19.2
176	17.9	15.4	23.2




Manual Integrations
APPROVED


mohammad
8/20/2019 8:35:57 AM

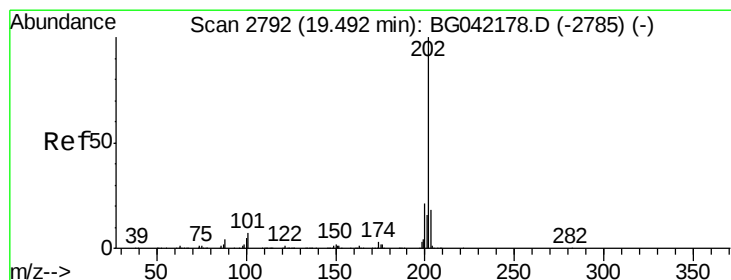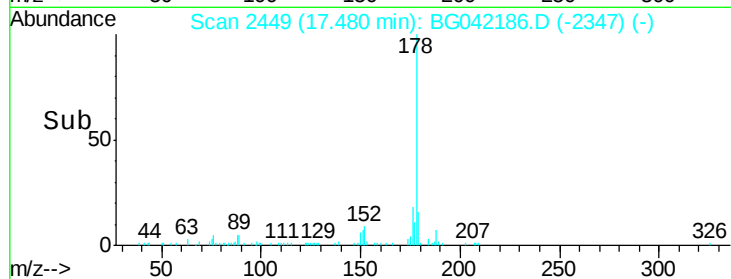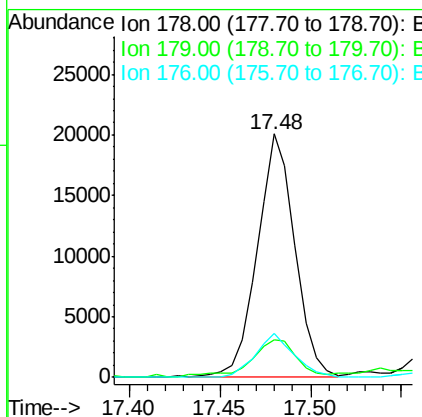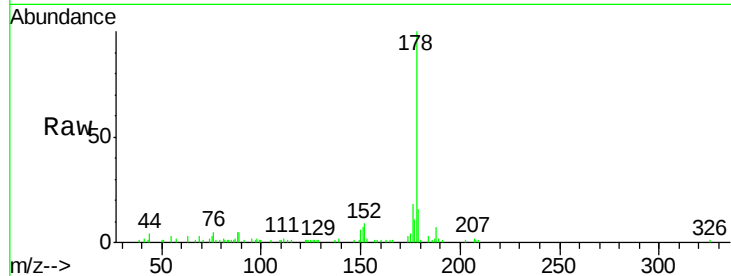

#76
Fluoranthene
Concen: 2.179 ng/ul m
RT: 19.49 min Scan# 2792
Delta R.T. 0.01 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Tgt Ion	Ratio	Lower	Upper
202	100		
101	7.7	6.7	10.1
100	5.1	5.3	7.9#

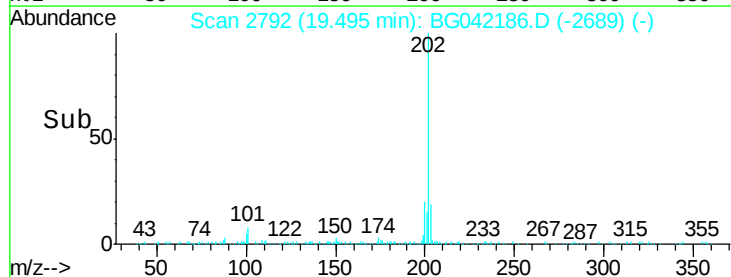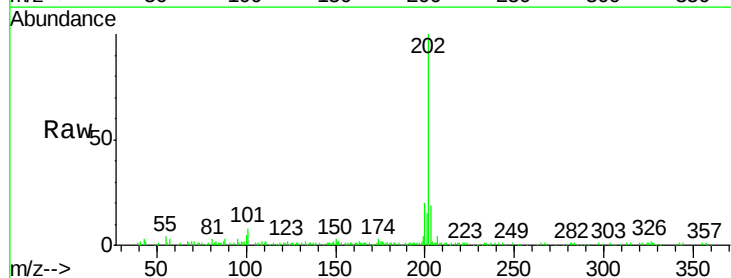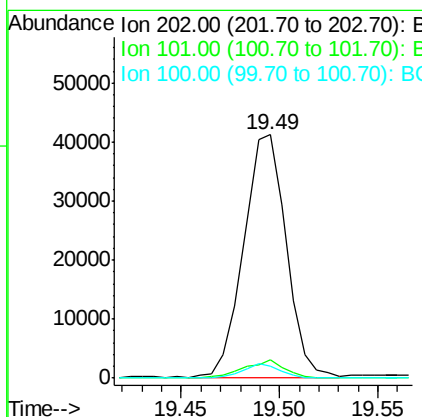

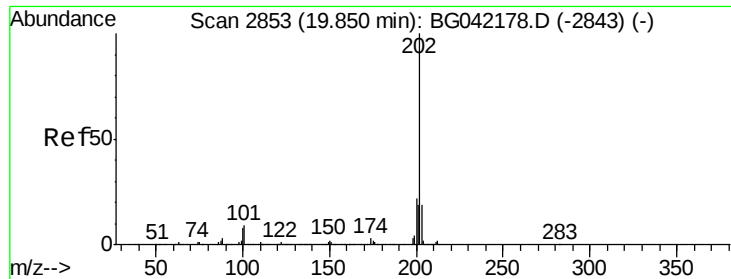





#79
Pvrene
Concen: 1.924 ng/ul
RT: 19.85 min Scan# 2853
Delta R.T. 0.00 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Instrument :
BNA_G
ClientSampled :
ETOC3

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	7.5	7.6	11.4#
100	6.8	6.5	9.7




Manual Integrations
APPROVED


mohammad
8/20/2019 8:35:57 AM

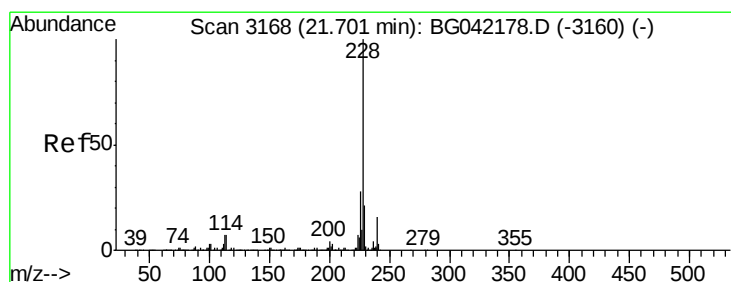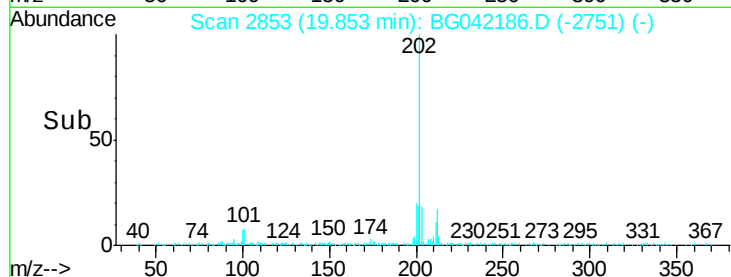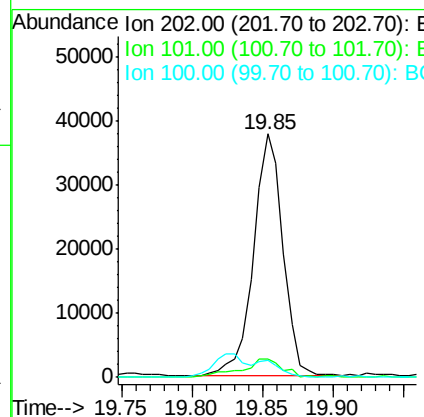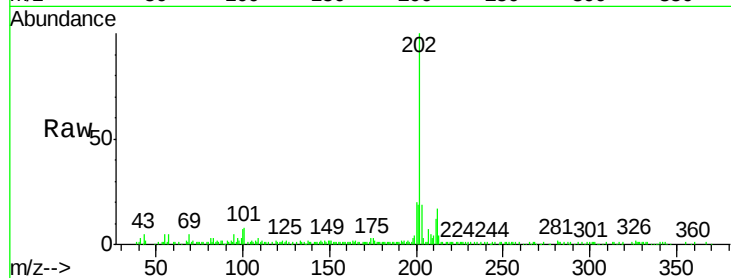

#82
Benzo(a)anthracene
Concen: 1.371 ng/ul
RT: 21.70 min Scan# 3168
Delta R.T. 0.00 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	20.6	17.0	25.6
226	31.2	23.3	34.9

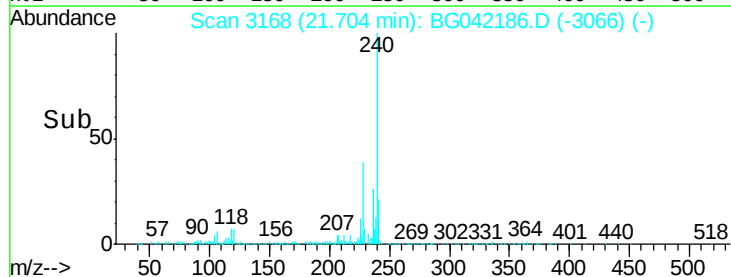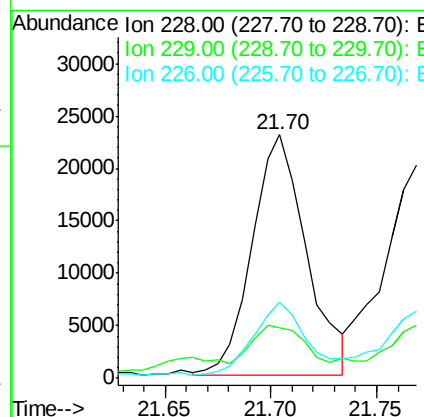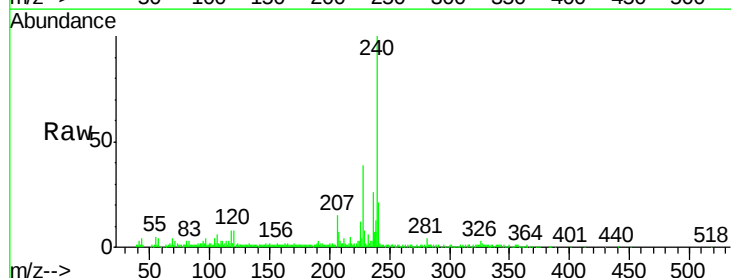

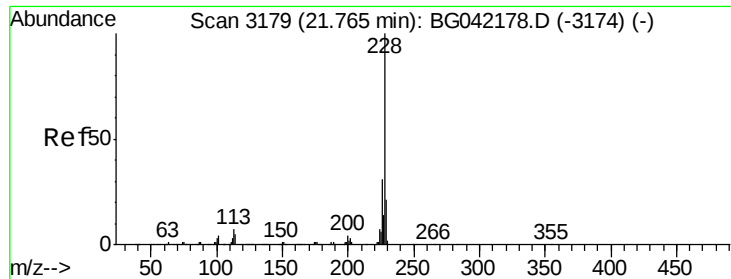





#84
Chrysene
Concen: 1.348 ng/ul m
RT: 21.77 min Scan# 3179
Delta R.T. 0.00 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Instrument :
BNA_G
ClientSampleId :
ETOC3

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.4	25.7	38.5
229	25.1	16.6	24.8




Manual Integrations
APPROVED


mohammad
8/20/2019 8:35:57 AM

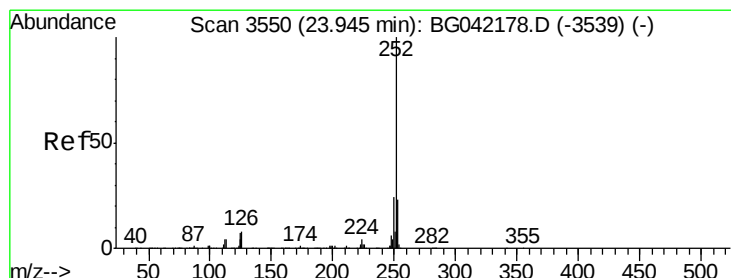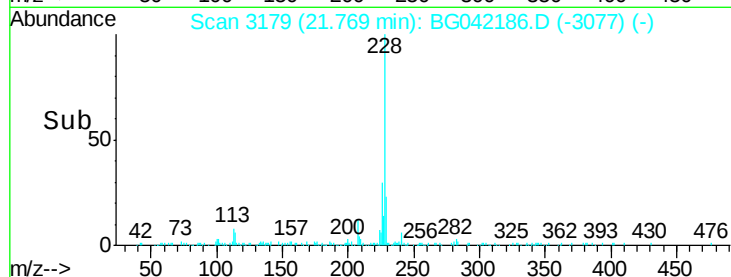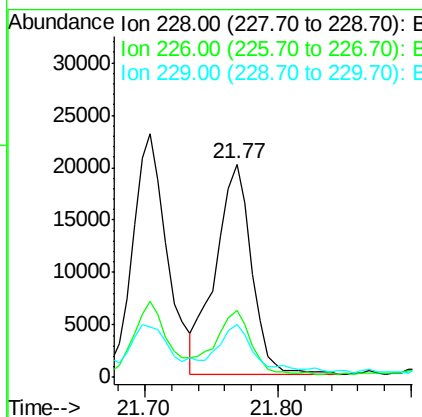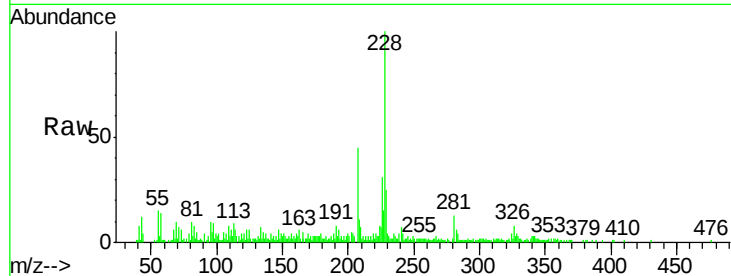

#87
Benzo(b)fluoranthene
Concen: 1.884 ng/ul
RT: 23.95 min Scan# 3551
Delta R.T. 0.01 min
Lab File: BG042186.D
Acq: 13 Aug 2019 18:28

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.0	18.4	27.6
125	8.5	5.8	8.8

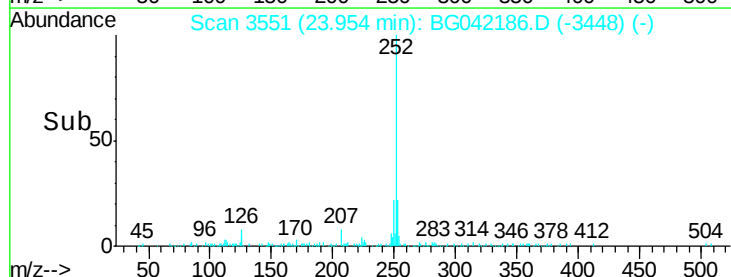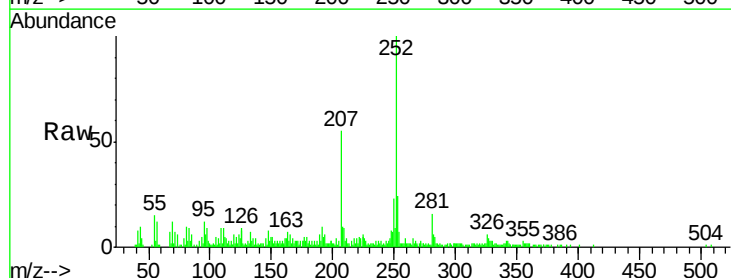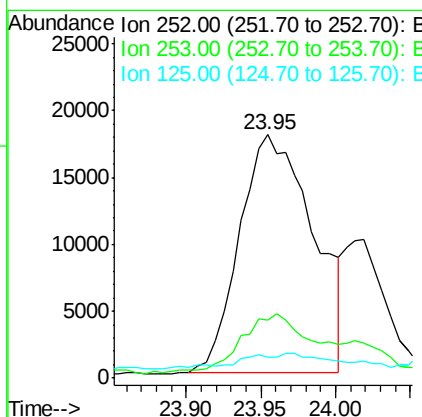

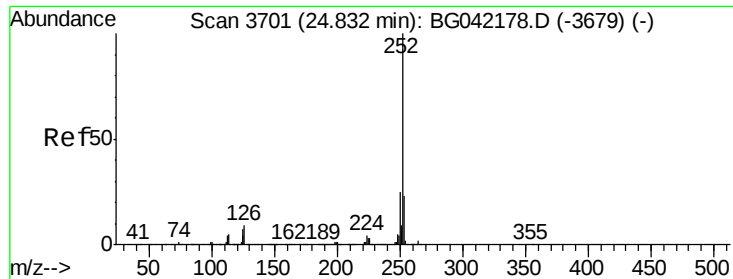

#90

Benzo(a)pyrene

Concen: 1.431 ng/ul

RT: 24.84 min Scan# 3701

Delta R.T. 0.00 min

Lab File: BG042186.D

Acq: 13 Aug 2019 18:28

Instrument :

BNA_G

ClientSampleId :

ETOC3

Tot Ion:	252	Resp:	44218
Ion Ratio	Lower	Upper	
252	100		
253	26.3	18.3	27.5
125	11.0	6.5	9.7#

Manual Integrations
APPROVED

mohammad
8/20/2019 8:35:57 AM

