

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081919\
 Data File : BG042351.D
 Acq On : 20 Aug 2019 10:01
 Operator : HP/JU
 Sample : k4385-33
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 21 03:20:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG081919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 19 13:40:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	67973	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	259061	20.00	ng	0.00
39) Acenaphthene-d10	14.66	164	185809	20.00	ng	0.00
64) Phenanthrene-d10	17.41	188	431879	20.00	ng	0.00
76) Chrysene-d12	21.69	240	451309	20.00	ng	0.00
87) Perylene-d12	24.93	264	521664	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.56	112	441171	131.50	ng	0.00
7) Phenol-d6	7.17	99	557517	122.36	ng	0.00
23) Nitrobenzene-d5	9.17	82	371525	100.87	ng	0.00
42) 2,4,6-Tribromophenol	16.16	330	363963	143.82	ng	0.00
45) 2-Fluorobiphenyl	13.28	172	1110143	101.10	ng	0.00
79) Terphenyl-d14	20.03	244	1925515	93.45	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.15	88	23907	16.524	ng	# 1
19) n-Nitroso-di-n-propylamine	9.17	70	46419	15.839	ng	# 71
50) Dimethylphthalate	14.11	163	46672	3.535	ng	# 99
51) 2,6-Dinitrotoluene	14.66	165	24592	7.958	ng	# 40
57) 2,4-Dinitrotoluene	14.66	165	24592	5.692	ng	# 38
67) 4-Bromophenyl-phenylether	16.16	248	25435	4.628	ng	# 1
77) Benzidine	20.03	184	27943	2.335	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG081919\
Data File : BG042351.D
Acq On : 20 Aug 2019 10:01
Operator : HP/JU
Sample : k4385-33
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 21 03:20:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG081919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 13:40:37 2019
Response via : Initial Calibration

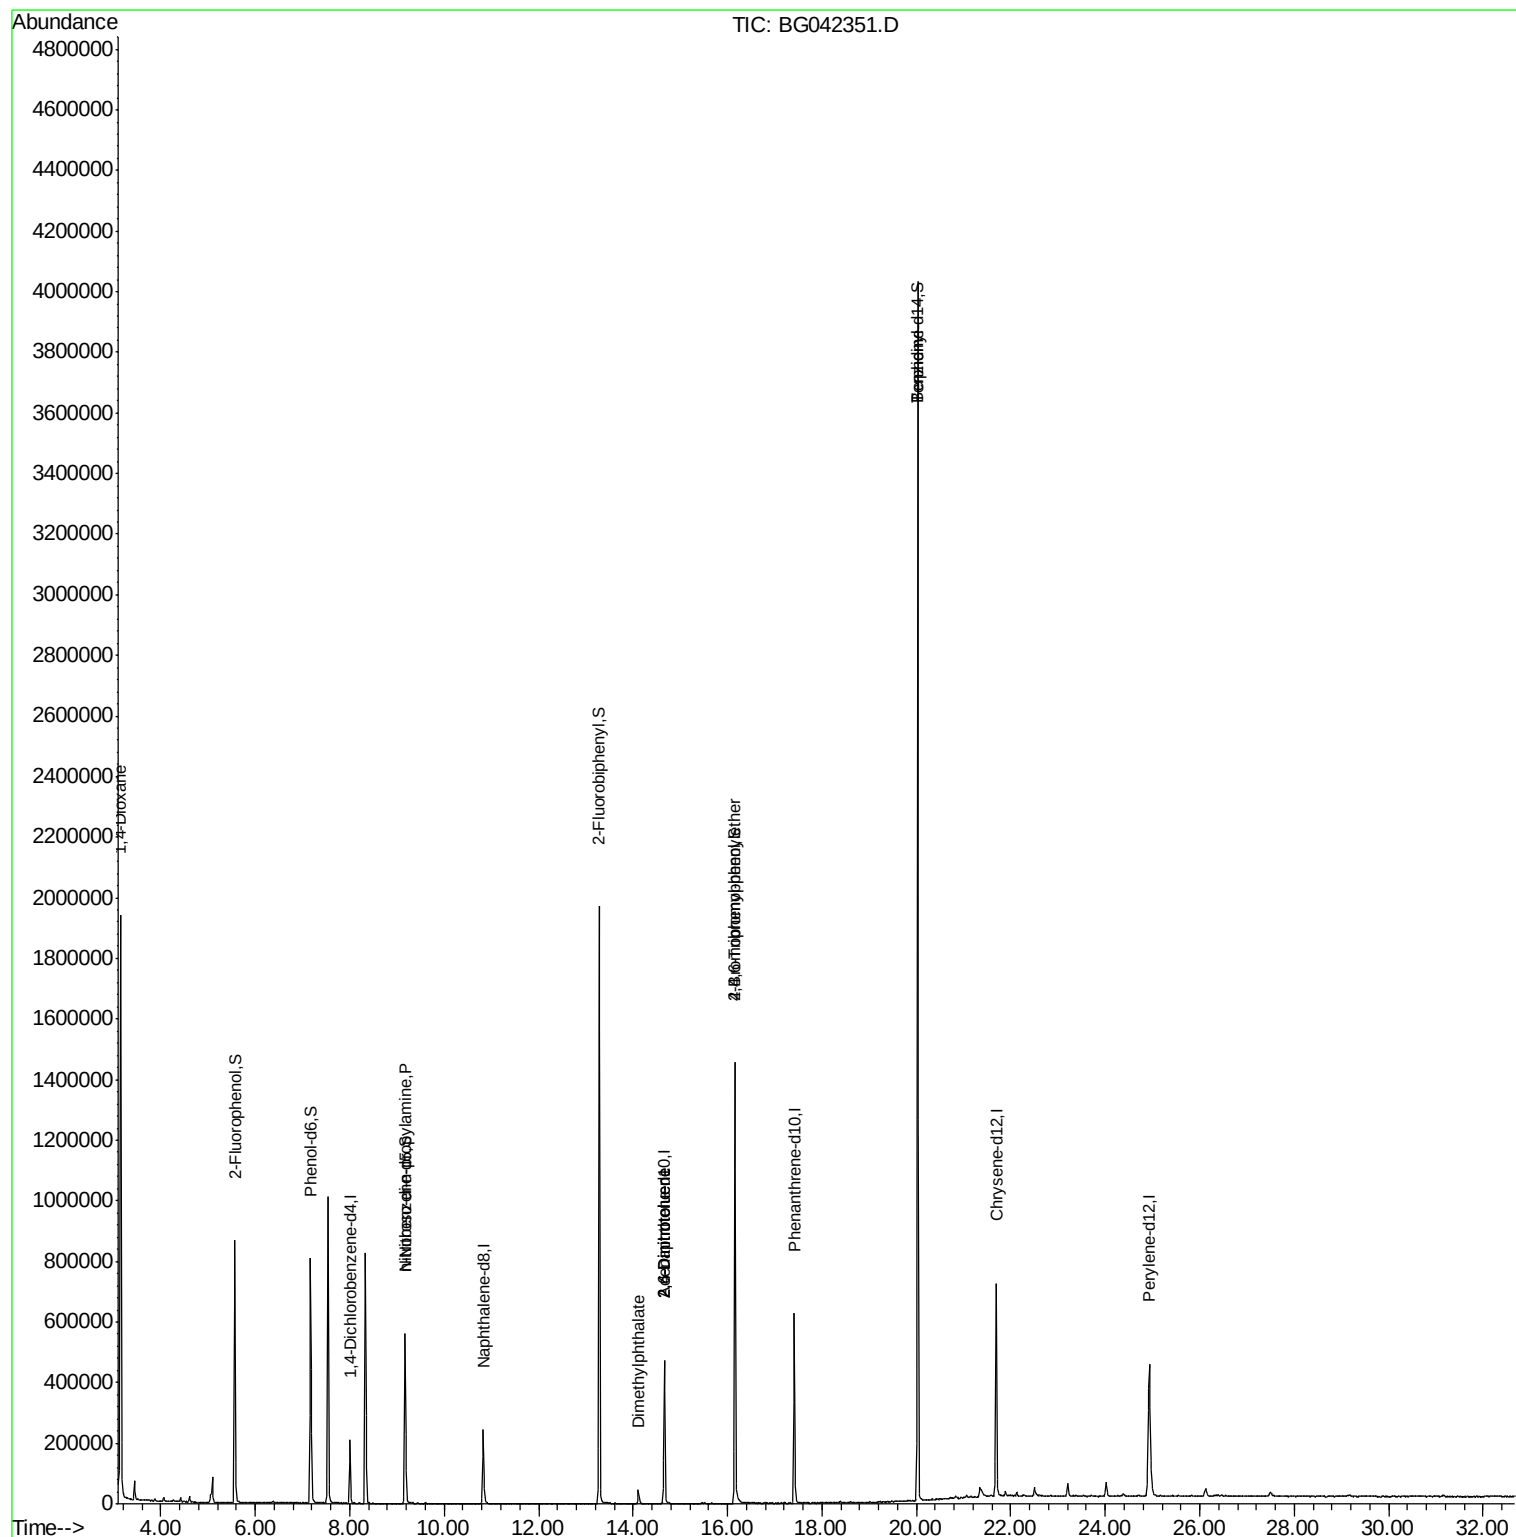




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.01 min Scan# 837
Delta R.T. 0.00 min
Lab File: BG042351.D
Acq: 20 Aug 2019 10:01

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 67973
Ion Ratio Lower Upper
152 100
150 155.6 124.3 186.5
115 48.4 40.5 60.7

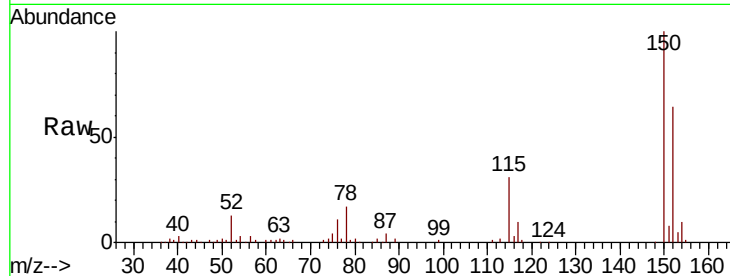


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

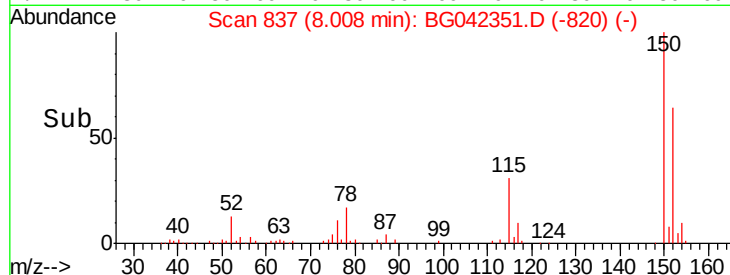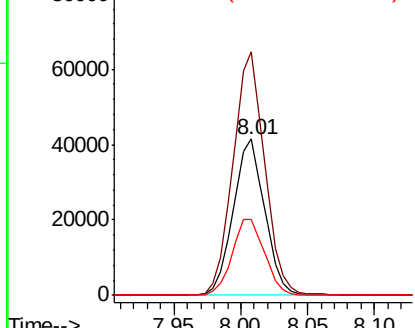



#2


1,4-Dioxane
Concen: 16.524 ng
RT: 3.15 min Scan# 10
Delta R.T. -0.28 min
Lab File: BG042351.D
Acq: 20 Aug 2019 10:01

Tgt Ion: 88 Resp: 23907
Ion Ratio Lower Upper
88 100
58 27.3 58.6 88.0#
43 2122.8 19.4 29.0#

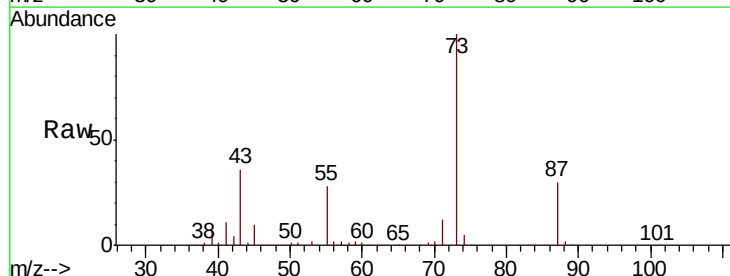

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 58.00 (57.70 to 58.70): BGC
Ion 43.00 (42.70 to 43.70): BGC

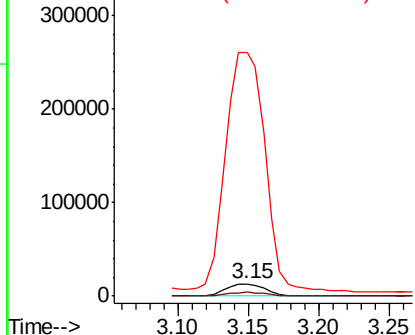

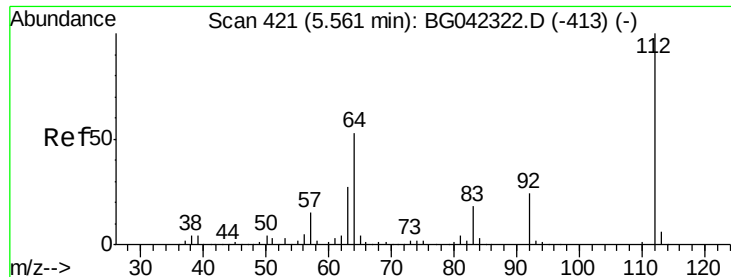

#5

2-Fluorophenol

Concen: 131.501 ng

RT: 5.56 min Scan# 421

Delta R.T. 0.00 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01

Instrument :

BNA_G

ClientSampleId :


Tot Ion:112 Resp: 441171

Ion Ratio Lower Upper




112 100

64 56.2 42.5 63.7

63 28.9 21.7 32.5

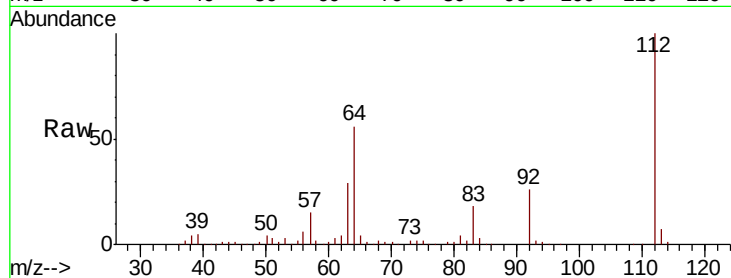

Abundance Ion 112.00 (111.70 to 112.70): BGC
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

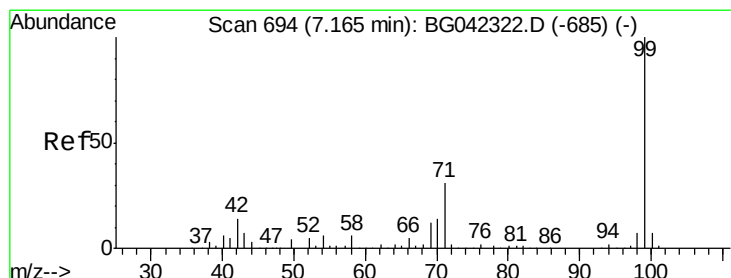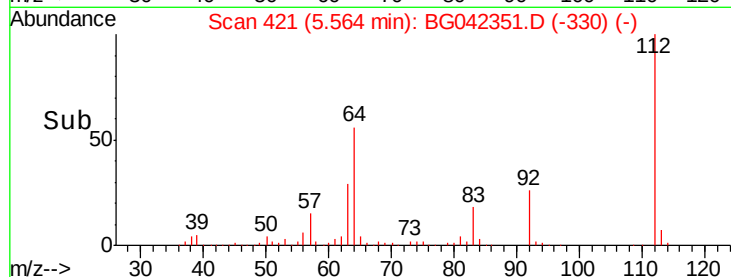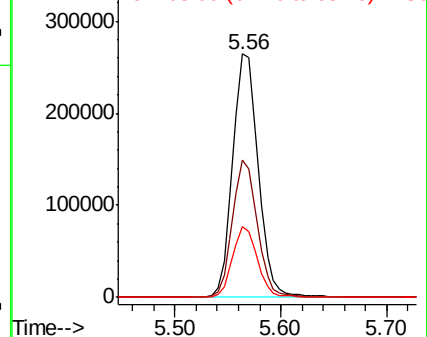

#7

Phenol-d6

Concen: 122.361 ng

RT: 7.17 min Scan# 695

Delta R.T. 0.01 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01


Tgt Ion: 99 Resp: 557517

Ion Ratio Lower Upper



99 100




42 13.9 11.4 17.0

71 31.2 25.1 37.7

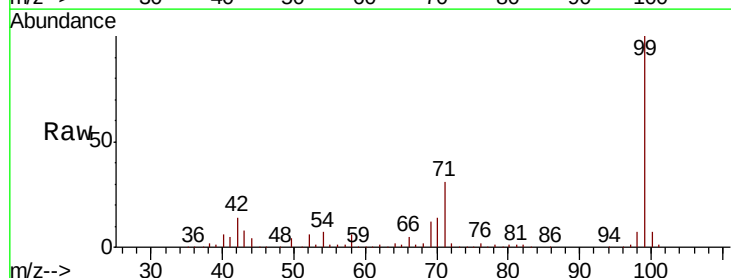

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC



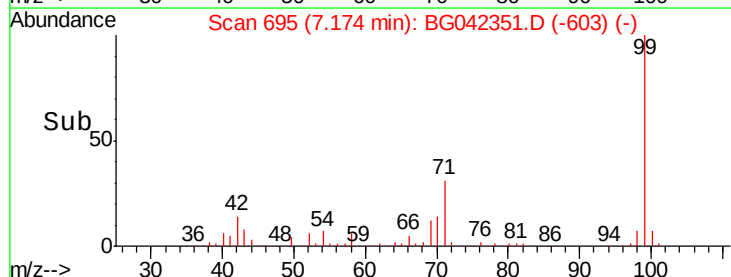
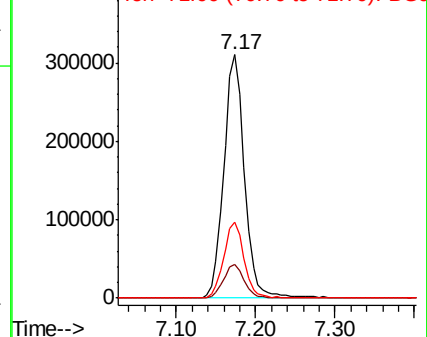


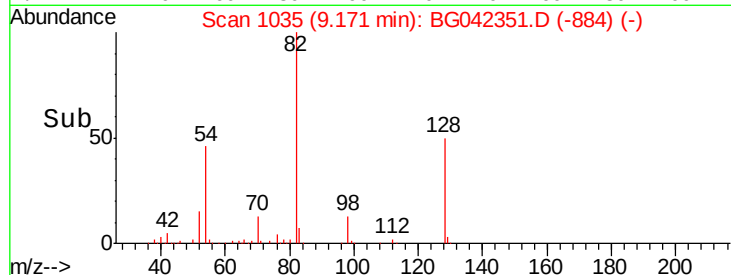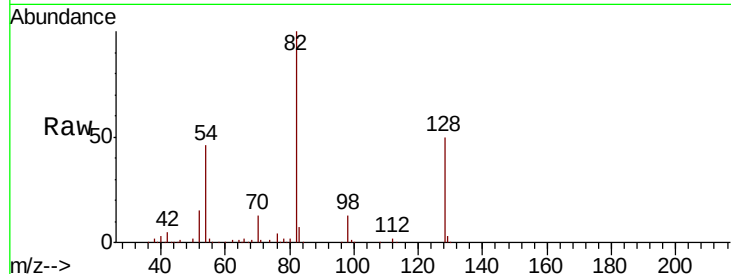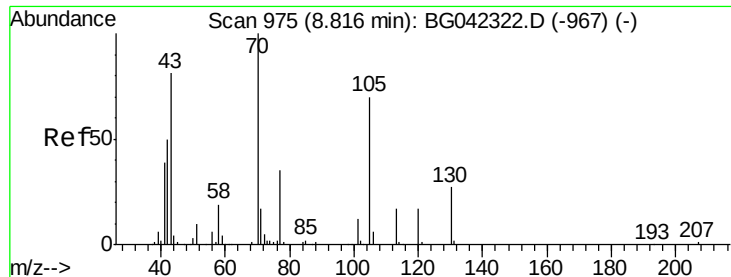

#19
n-Nitroso-di-n-propylamine
Concen: 15.839 ng
RT: 9.17 min Scan# 1035
Delta R.T. 0.36 min
Lab File: BG042351.D
Acq: 20 Aug 2019 10:01


Instrument :
BNA_G
ClientSampleId :


Tot Ion: 70 Resp: 46419
Ion Ratio Lower Upper
70 100
42 38.4 40.5 60.7#
101 0.0 9.3 13.9#
130 2.3 22.0 33.0#

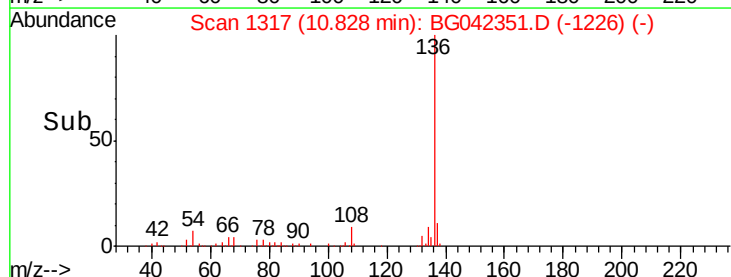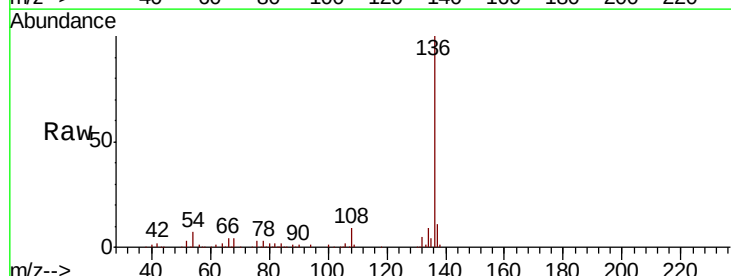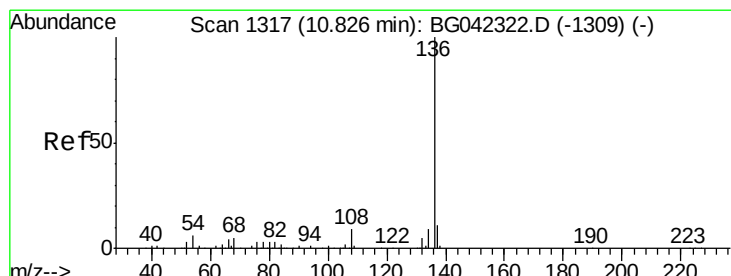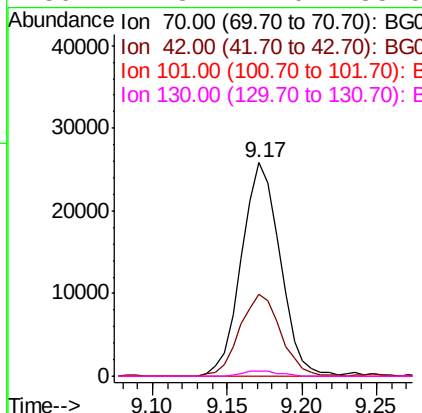

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.83 min Scan# 1317
Delta R.T. 0.00 min
Lab File: BG042351.D
Acq: 20 Aug 2019 10:01

Tgt Ion:136 Resp: 259061
Ion Ratio Lower Upper
136 100
137 11.2 8.4 12.6
54 6.8 5.0 7.4
68 4.3 3.8 5.8

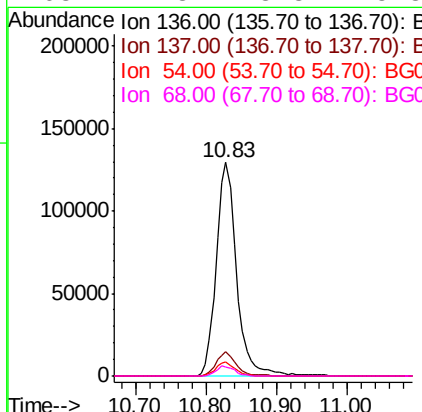







#23
 Nitrobenzene-d5
 Concen: 100.866 ng
 RT: 9.17 min Scan# 1035
 Delta R.T. -0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Instrument :
 BNA_G
 ClientSampled :

Tot Ion	82	Resp	371525
Ion Ratio	Lower	Upper	
82	100		
128	50.4	41.0	61.4
54	45.7	38.0	57.0

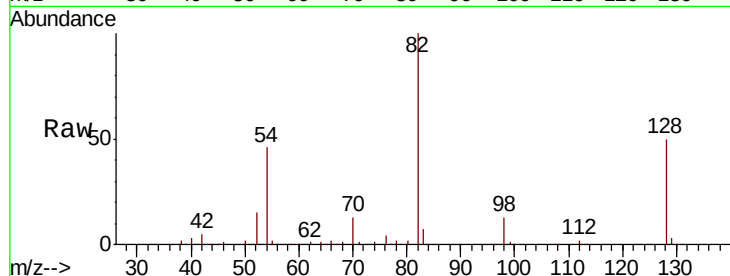


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

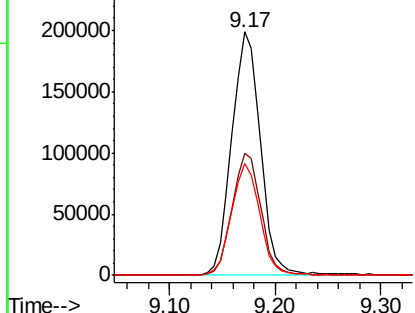




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. -0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Tgt Ion	164	Resp	185809
Ion Ratio	Lower	Upper	
164	100		
162	101.2	80.6	120.8
160	45.6	35.7	53.5



Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

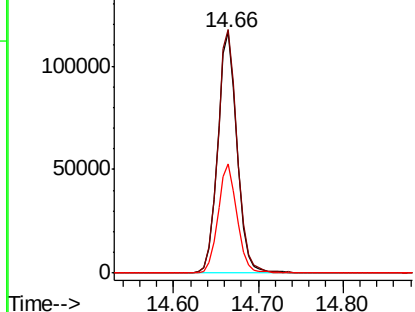




#42
 2,4,6-Tribromophenol
 Concen: 143.820 ng
 RT: 16.16 min Scan# 2224
 Delta R.T. 0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Instrument :
 BNA_G
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	98.4	76.9	115.3
141	28.8	21.8	32.6






Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

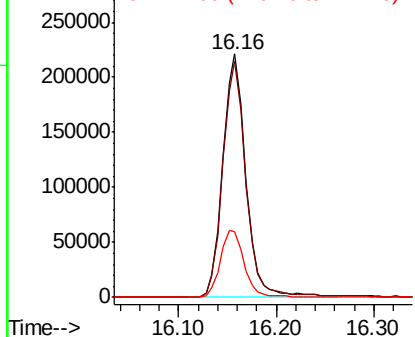

#45
 2-Fluorobiphenyl
 Concen: 101.100 ng
 RT: 13.28 min Scan# 1735
 Delta R.T. -0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	39.1	30.3	45.5
170	25.7	20.0	30.0






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

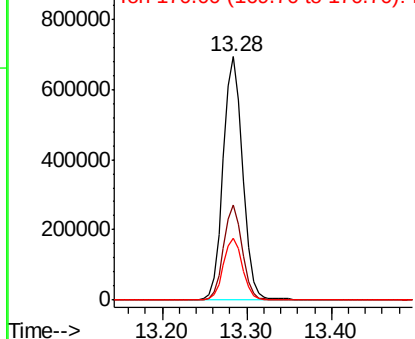



#50

Dimethylphthalate

Concen: 3.535 ng

RT: 14.11 min Scan# 1876

Delta R.T. -0.00 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01

Instrument :

BNA_G

ClientSampleId :


Tot Ion:163 Resp: 46672

Ion Ratio Lower Upper

163 100

194 4.4 4.2 6.2




164 10.6 8.8 13.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

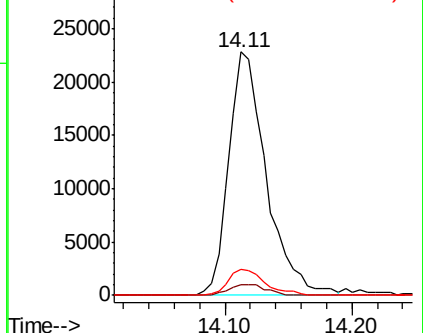

#51

2,6-Dinitrotoluene

Concen: 7.958 ng

RT: 14.66 min Scan# 1970

Delta R.T. 0.43 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01


Tgt Ion:165 Resp: 24592

Ion Ratio Lower Upper

165 100

63 1.4 28.2 42.2#



89 1.0 30.0 45.0#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

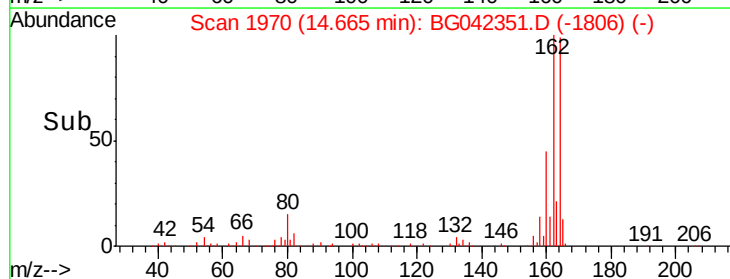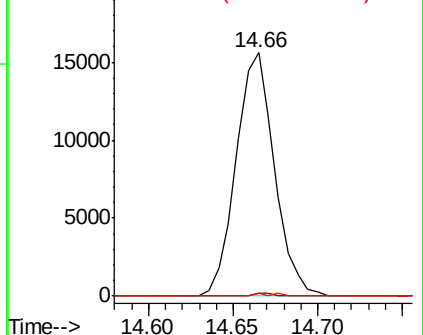


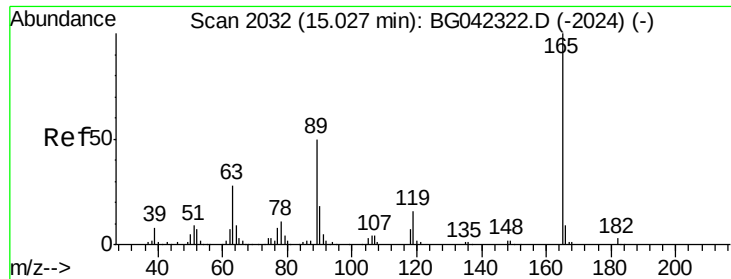

#57
 2,4-Dinitrotoluene
 Concen: 5.692 ng
 RT: 14.66 min Scan# 1970
 Delta R.T. -0.36 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Instrument :
 BNA_G
 ClientSampleID :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.4	22.4	33.6#
89	1.0	40.2	60.2#
182	0.0	2.6	3.8#



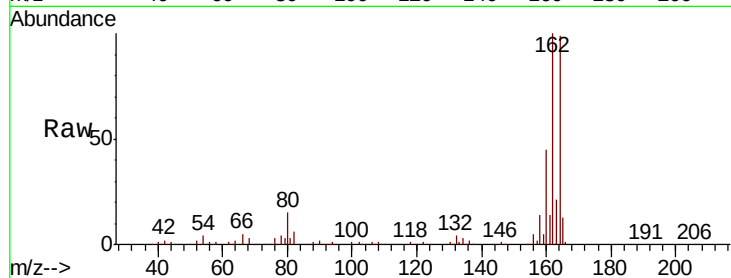


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

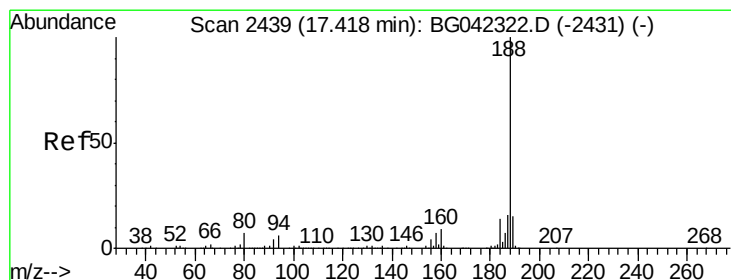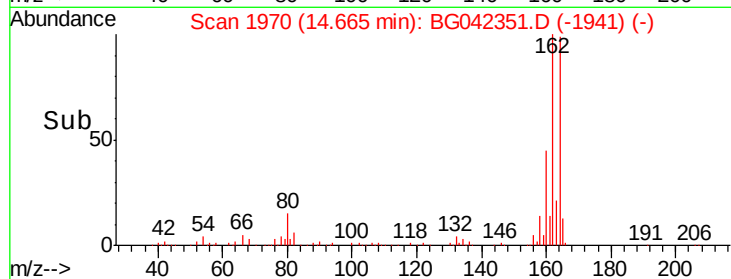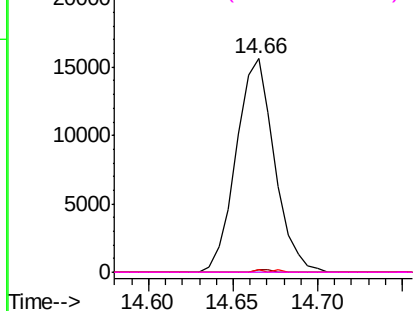

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2438
 Delta R.T. -0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01



Tgt Ion	Ratio	Lower	Upper
188	100		
94	6.2	4.9	7.3
80	7.1	5.4	8.0

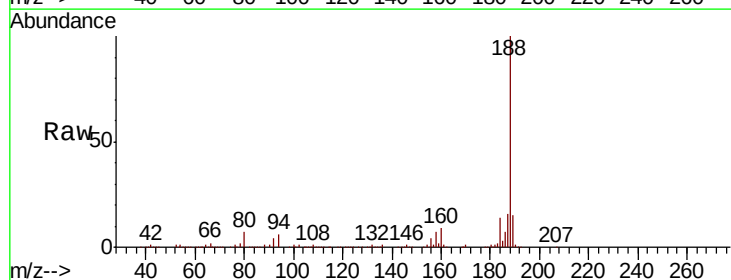


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

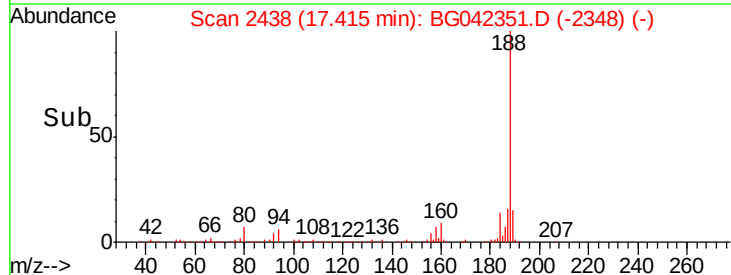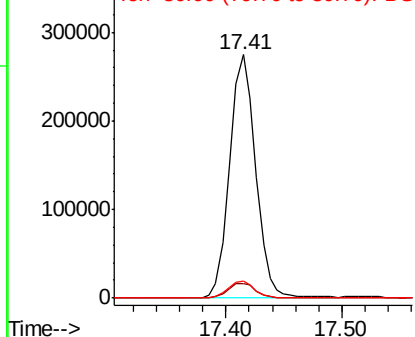


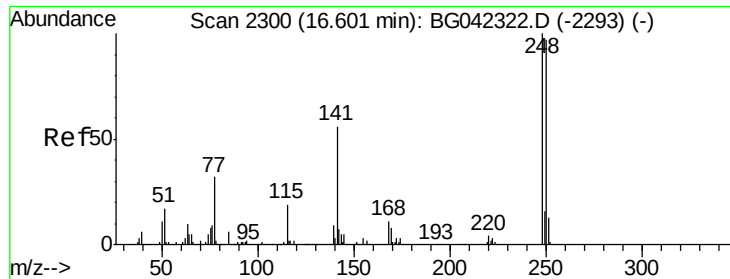

#67
 4-Bromophenyl-phenylether
 Concen: 4.628 ng
 RT: 16.16 min Scan# 2224
 Delta R.T. -0.44 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
248	100		
250	191.2	78.0	117.0#
141	371.8	44.9	67.3#






Abundance

Ion 248.00 (247.70 to 248.70): E


Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

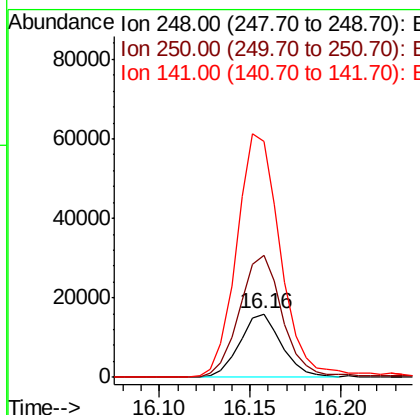

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.69 min Scan# 3166
 Delta R.T. -0.00 min
 Lab File: BG042351.D
 Acq: 20 Aug 2019 10:01

Tgt Ion	Ratio	Lower	Upper
240	100		
120	7.7	6.0	9.0
236	26.4	21.6	32.4






Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

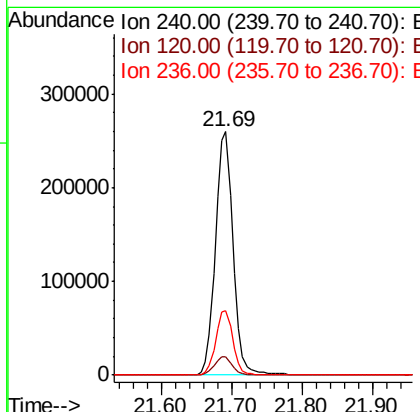



#77

Benzidine

Concen: 2.335 ng

RT: 20.03 min Scan# 2883

Delta R.T. 0.38 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 27943

Ion Ratio Lower Upper

184 100

185 16.7 11.8 17.6




183 8.9 10.6 15.8#



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

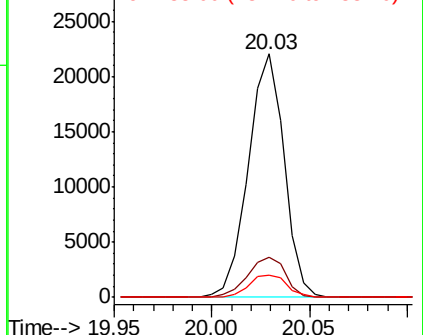

#79

Terphenyl-d14

Concen: 93.449 ng

RT: 20.03 min Scan# 2883

Delta R.T. -0.00 min

Lab File: BG042351.D

Acq: 20 Aug 2019 10:01


Tgt Ion:244 Resp: 1925515

Ion Ratio Lower Upper

244 100

212 8.7 6.4 9.6



122 10.0 6.6 10.0#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

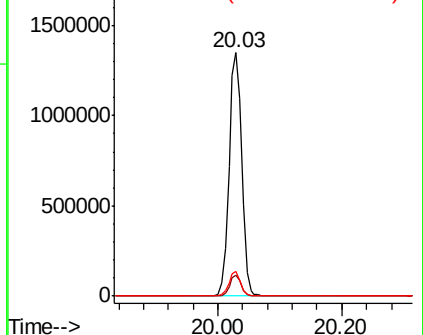


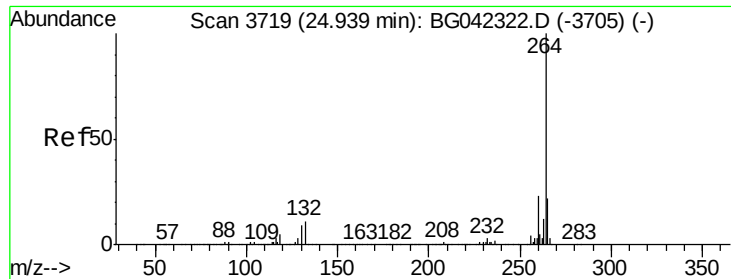

#87
Pervlene-d12
Concen: 20.000 ng
RT: 24.93 min Scan# 3717
Delta R.T. -0.01 min
Lab File: BG042351.D
Acq: 20 Aug 2019 10:01

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	18.4	27.6
265	21.6	17.4	26.0

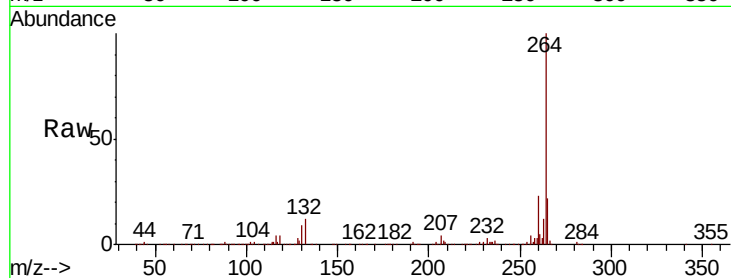

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

