


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG082119\
 Data File : BG042378.D
 Acq On : 21 Aug 2019 10:57
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG081919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 13:40:37 2019

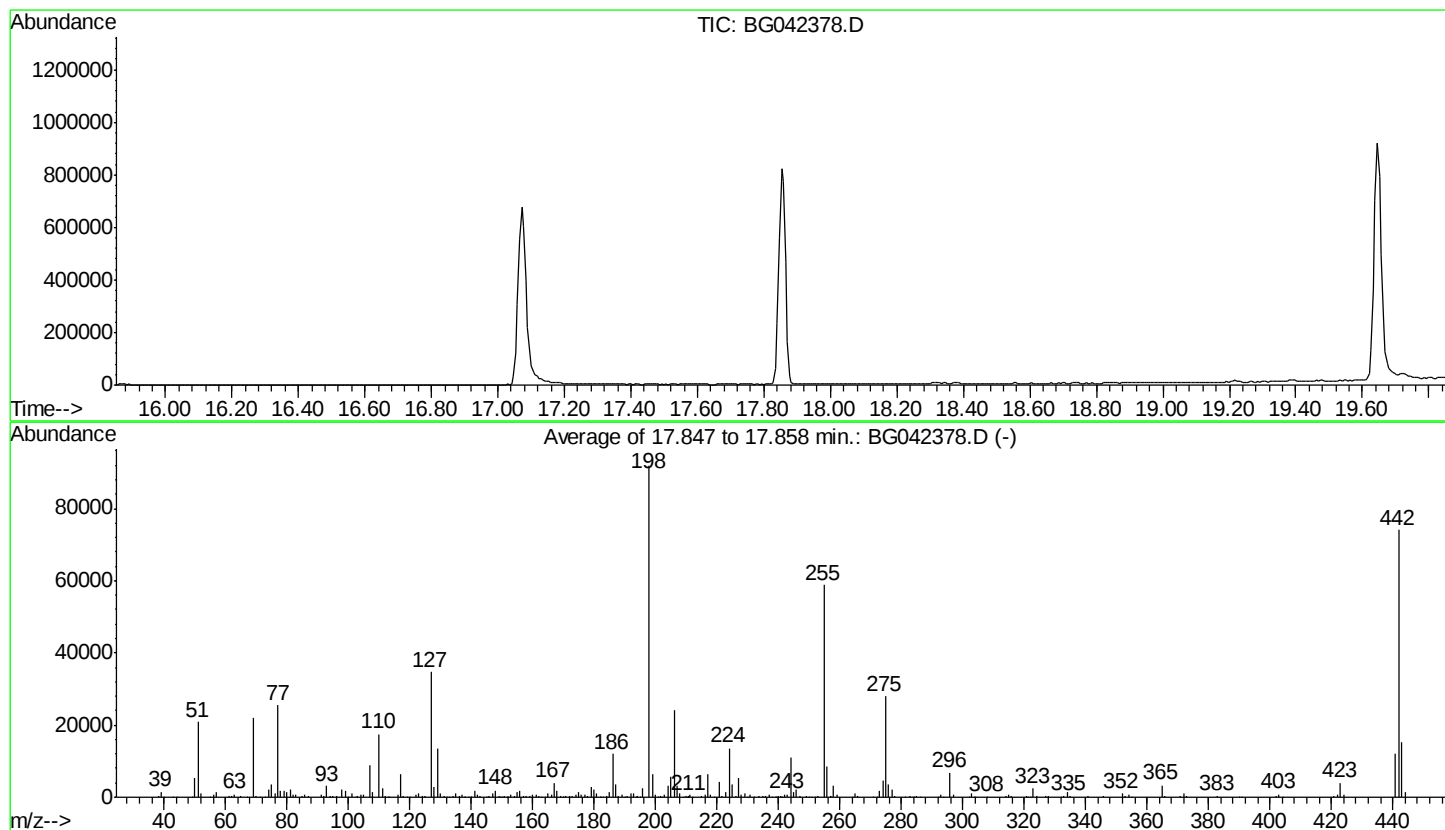

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	20797	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.8	21888	PASS
70	69	0.00	2	1.0	211	PASS
127	198	10	80	37.8	34709	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91898	PASS
199	198	5	9	6.9	6376	PASS
275	198	10	60	30.4	27981	PASS
365	198	1	100	3.5	3256	PASS
441	198	0.01	100	13.0	11932	PASS
442	198	50	100	80.6	74072	PASS
443	442	15	24	20.4	15090	PASS