
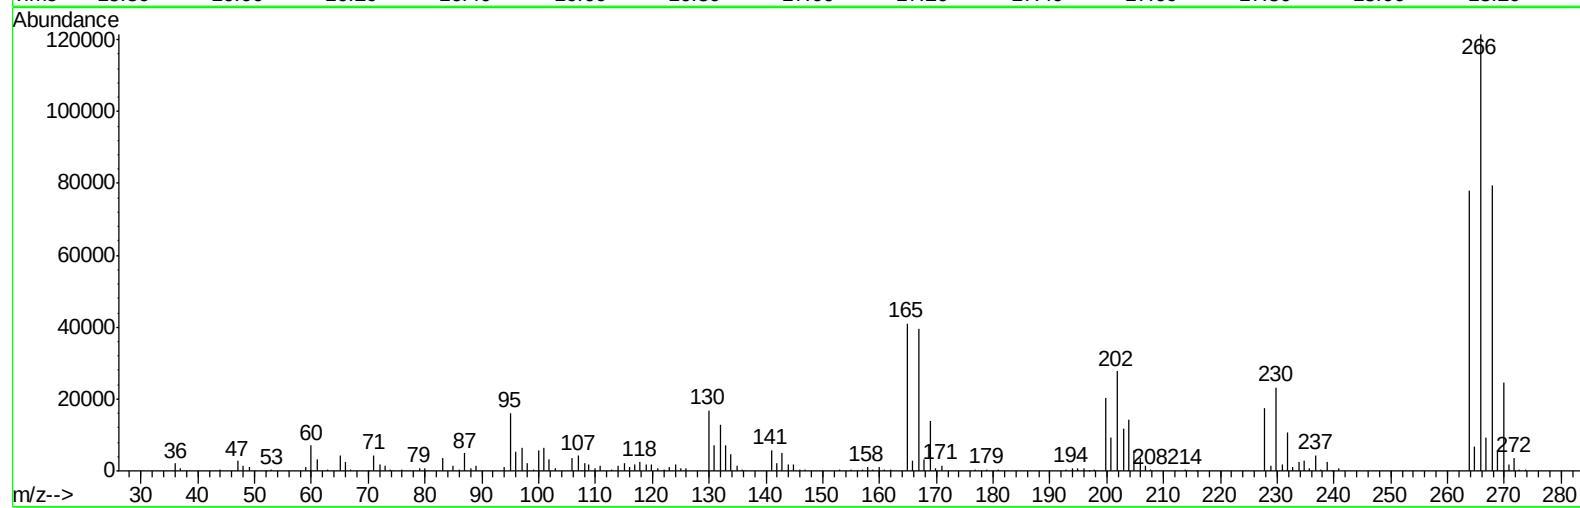


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083119\
Data File : BG042622.D
Acq On : 31 Aug 2019 6:53
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 01:10:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

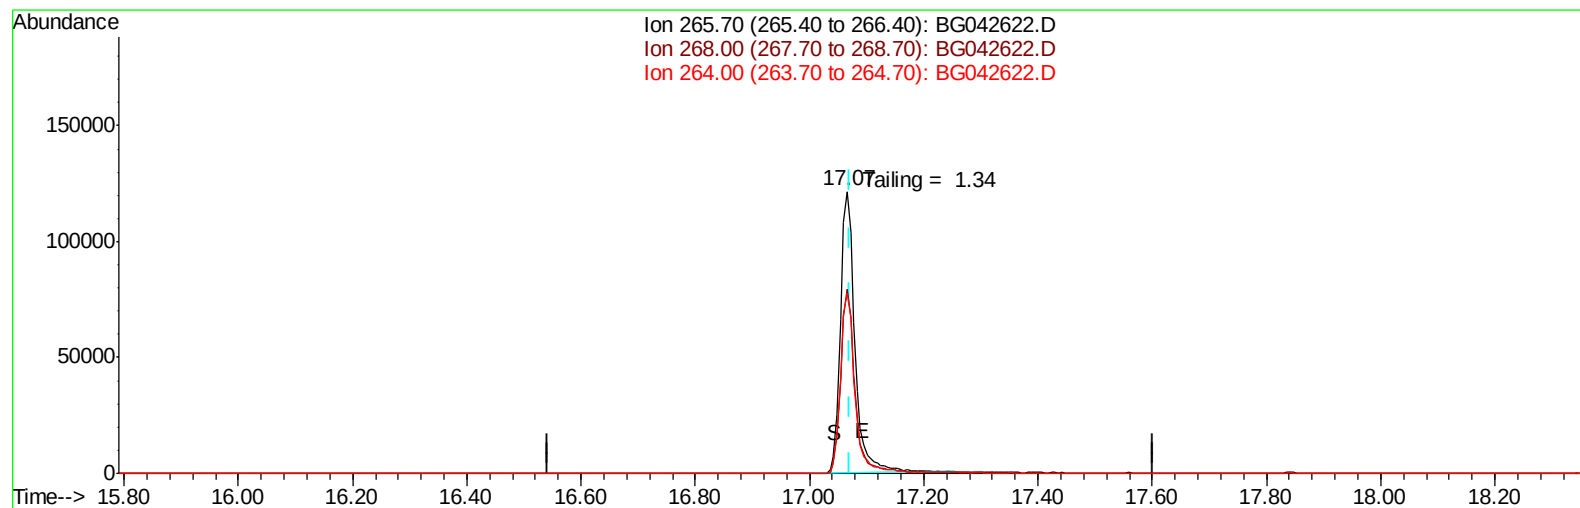

TIC: BG042622.D

(70) Pentachlorophenol (C)



17.066min (-0.006) 20174.84ng

response 218836

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	65.40
264.00	61.80	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083119\
Data File : BG042622.D
Acq On : 31 Aug 2019 6:53
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 01:10:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

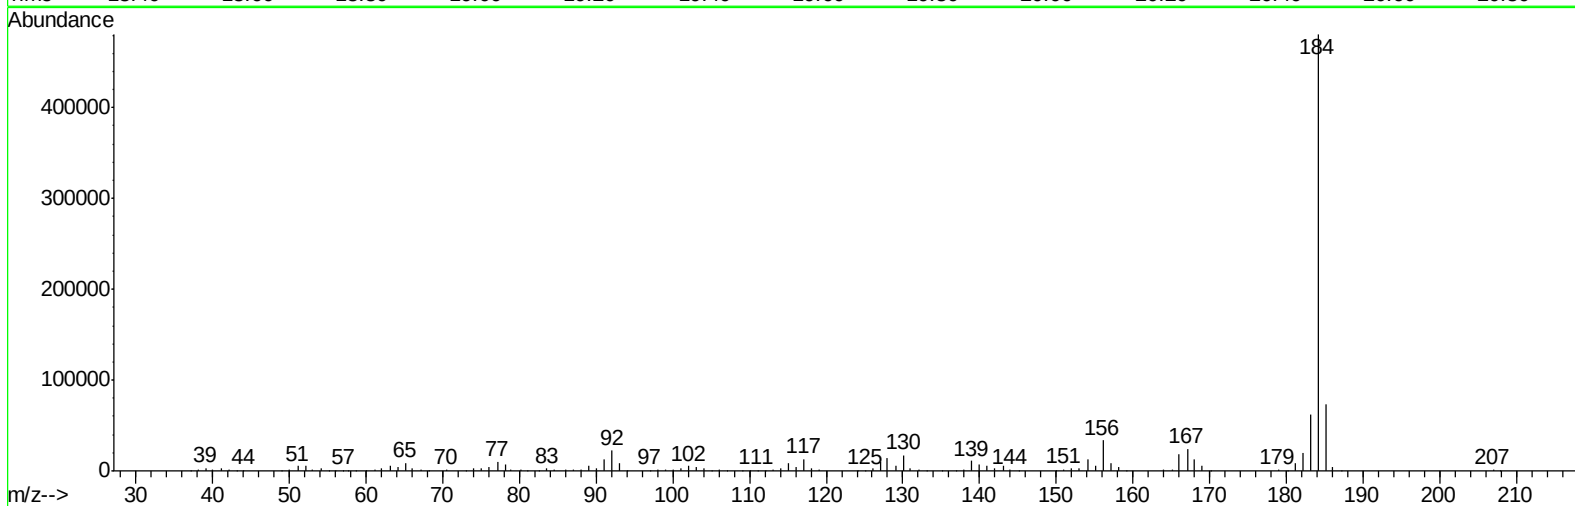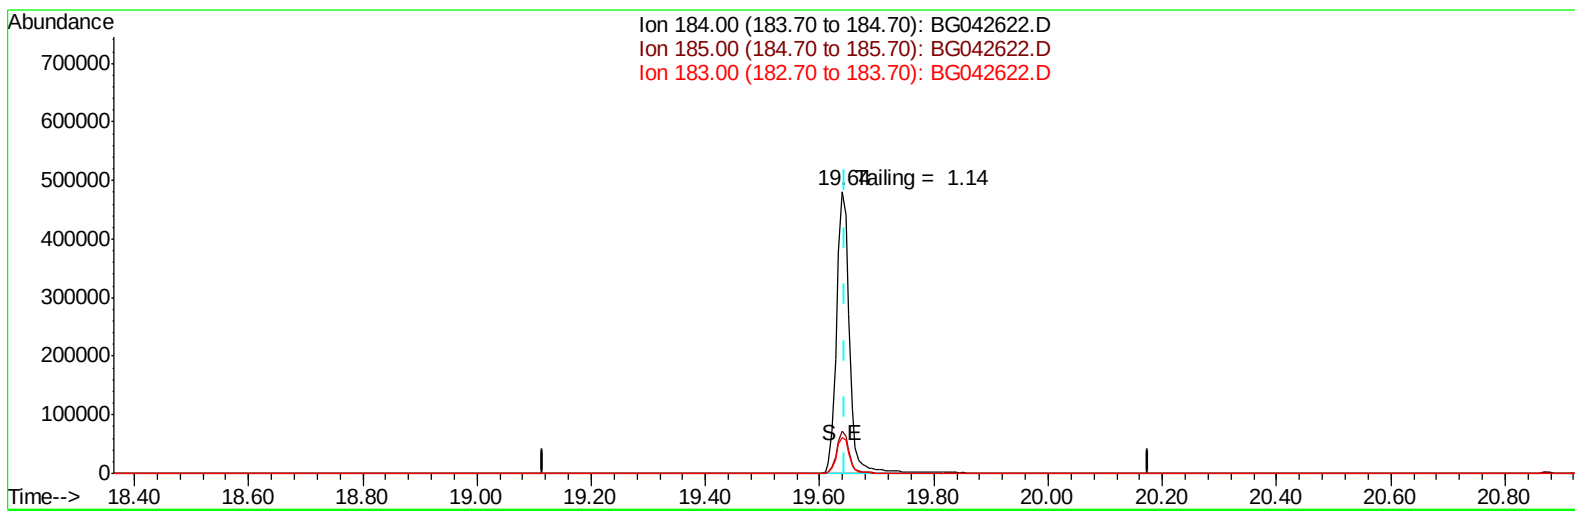

TIC: BG042622.D

(77) Benzidine

19.639min (-0.006) 11596.60ng

response 760713

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	15.12
183.00	13.50	12.97
0.00	0.00	0.00