
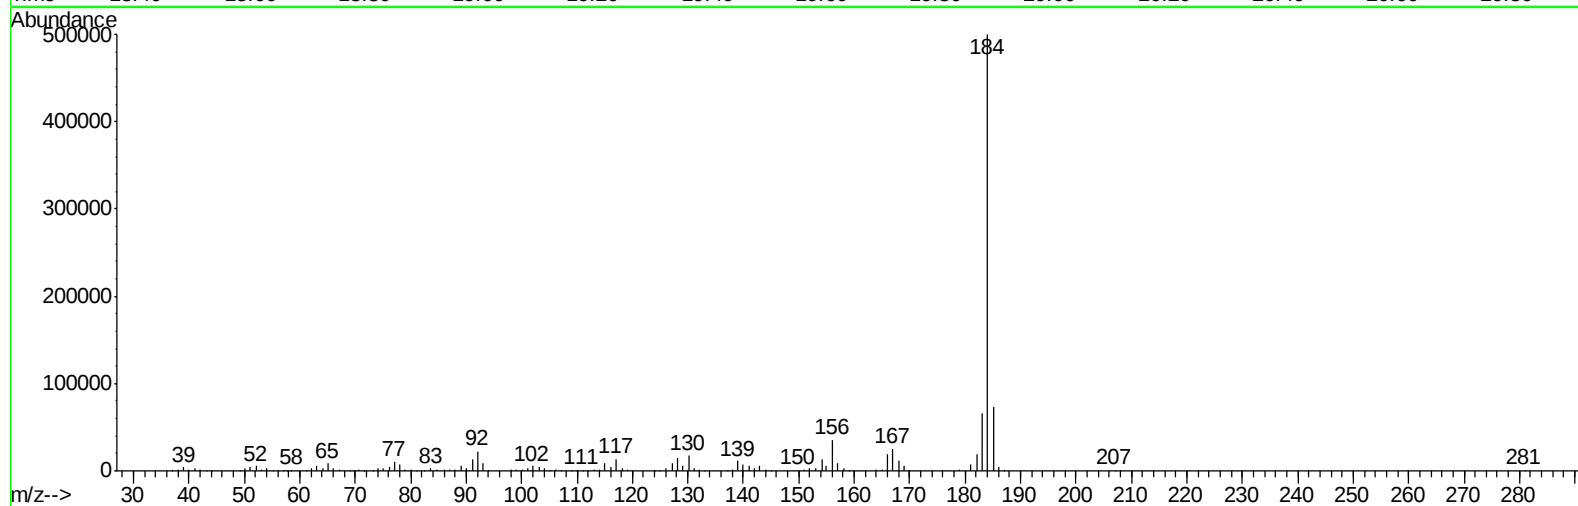


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083119\
 Data File : BG042641.D
 Acq On : 31 Aug 2019 20:58
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 00:59:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 22 14:29:15 2019
 Response via : Initial Calibration

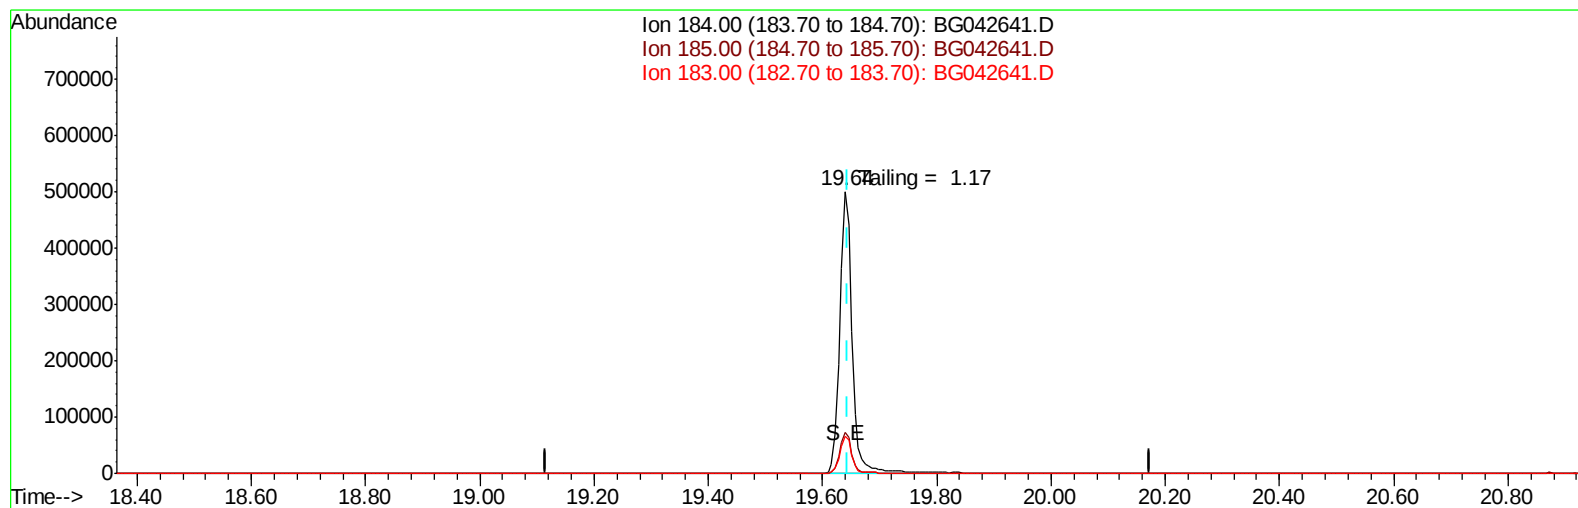

TIC: BG042641.D

(77) Benzidine




19.639min (-0.006) 17171.41ng

response 750775

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.73
183.00	13.50	13.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG083119\
Data File : BG042641.D
Acq On : 31 Aug 2019 20:58
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 00:59:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 22 14:29:15 2019
Response via : Initial Calibration

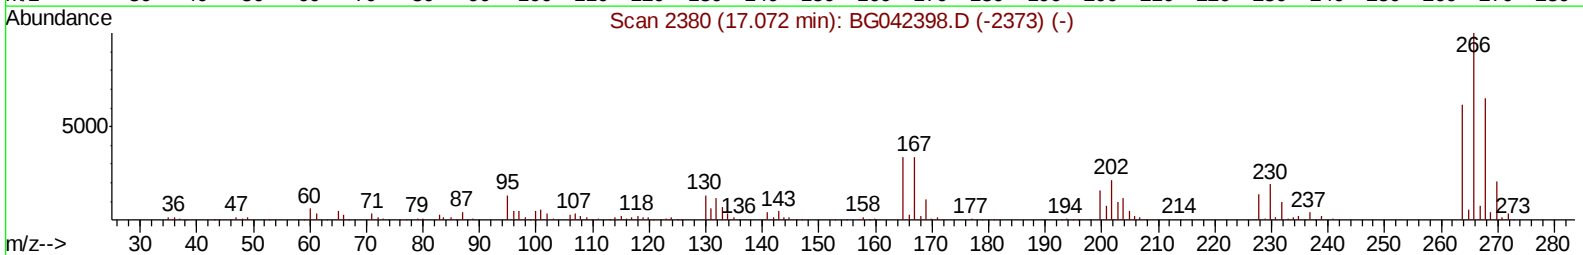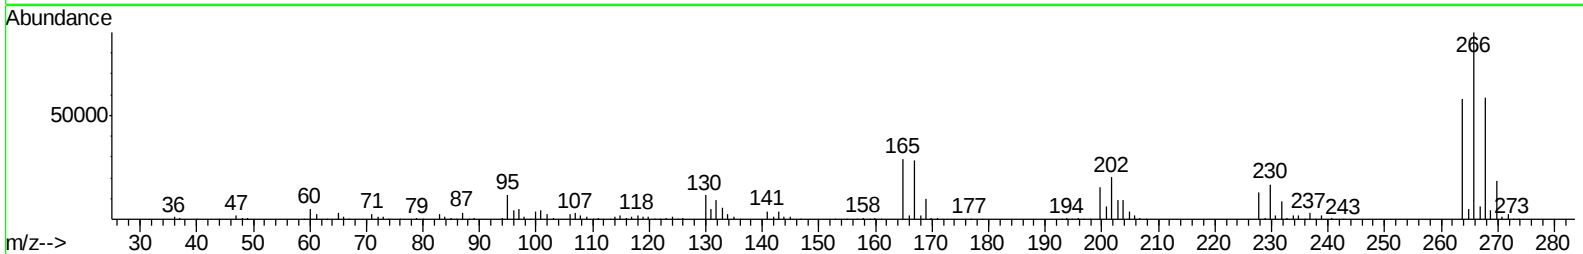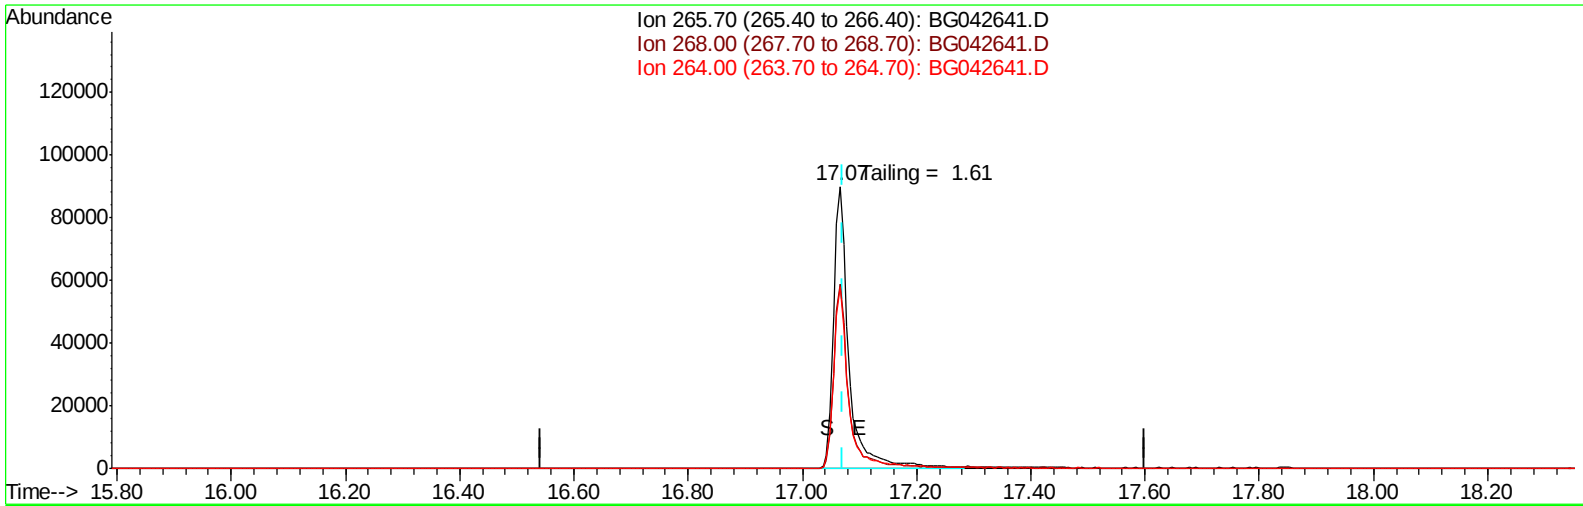

TIC: BG042641.D

(70) Pentachlorophenol (C)

17.066min (-0.006) 23195.31ng

response 161030

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	65.47
264.00	61.80	64.57
0.00	0.00	0.00